

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091420\
 Data File : BP003270.D
 Acq On : 14 Sep 2020 16:00
 Operator : CG/JU
 Sample : PB131580BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131580BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.252	396	402	420	rBV	1553693	2462149	34.10%	8.214%
2	6.834	664	671	694	rBV	1371294	2398011	33.22%	8.000%
3	7.640	801	808	818	rBV	434663	685533	9.50%	2.287%
4	8.787	995	1003	1033	rBV	922691	1730709	23.97%	5.774%
5	10.422	1273	1281	1306	rBV	410386	949628	13.15%	3.168%
6	12.904	1695	1703	1730	rBV	2632767	4592754	63.62%	15.323%
7	14.287	1931	1938	1956	rBV	695313	1259637	17.45%	4.202%
8	15.781	2185	2192	2220	rBV	1715398	3195809	44.27%	10.662%
9	17.039	2399	2406	2428	rBV	748829	1519252	21.04%	5.069%
10	19.616	2838	2844	2861	rBV	5481169	7219401	100.00%	24.086%
11	21.139	3097	3103	3114	rBV	1173726	1906762	26.41%	6.361%
12	23.368	3475	3482	3499	rVB2	981434	2053919	28.45%	6.852%


Sum of corrected areas: 29973564

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091420\
Data File : BP003270.D
Acq On : 14 Sep 2020 16:00
Operator : CG/JU
Sample : PB131580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131580BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

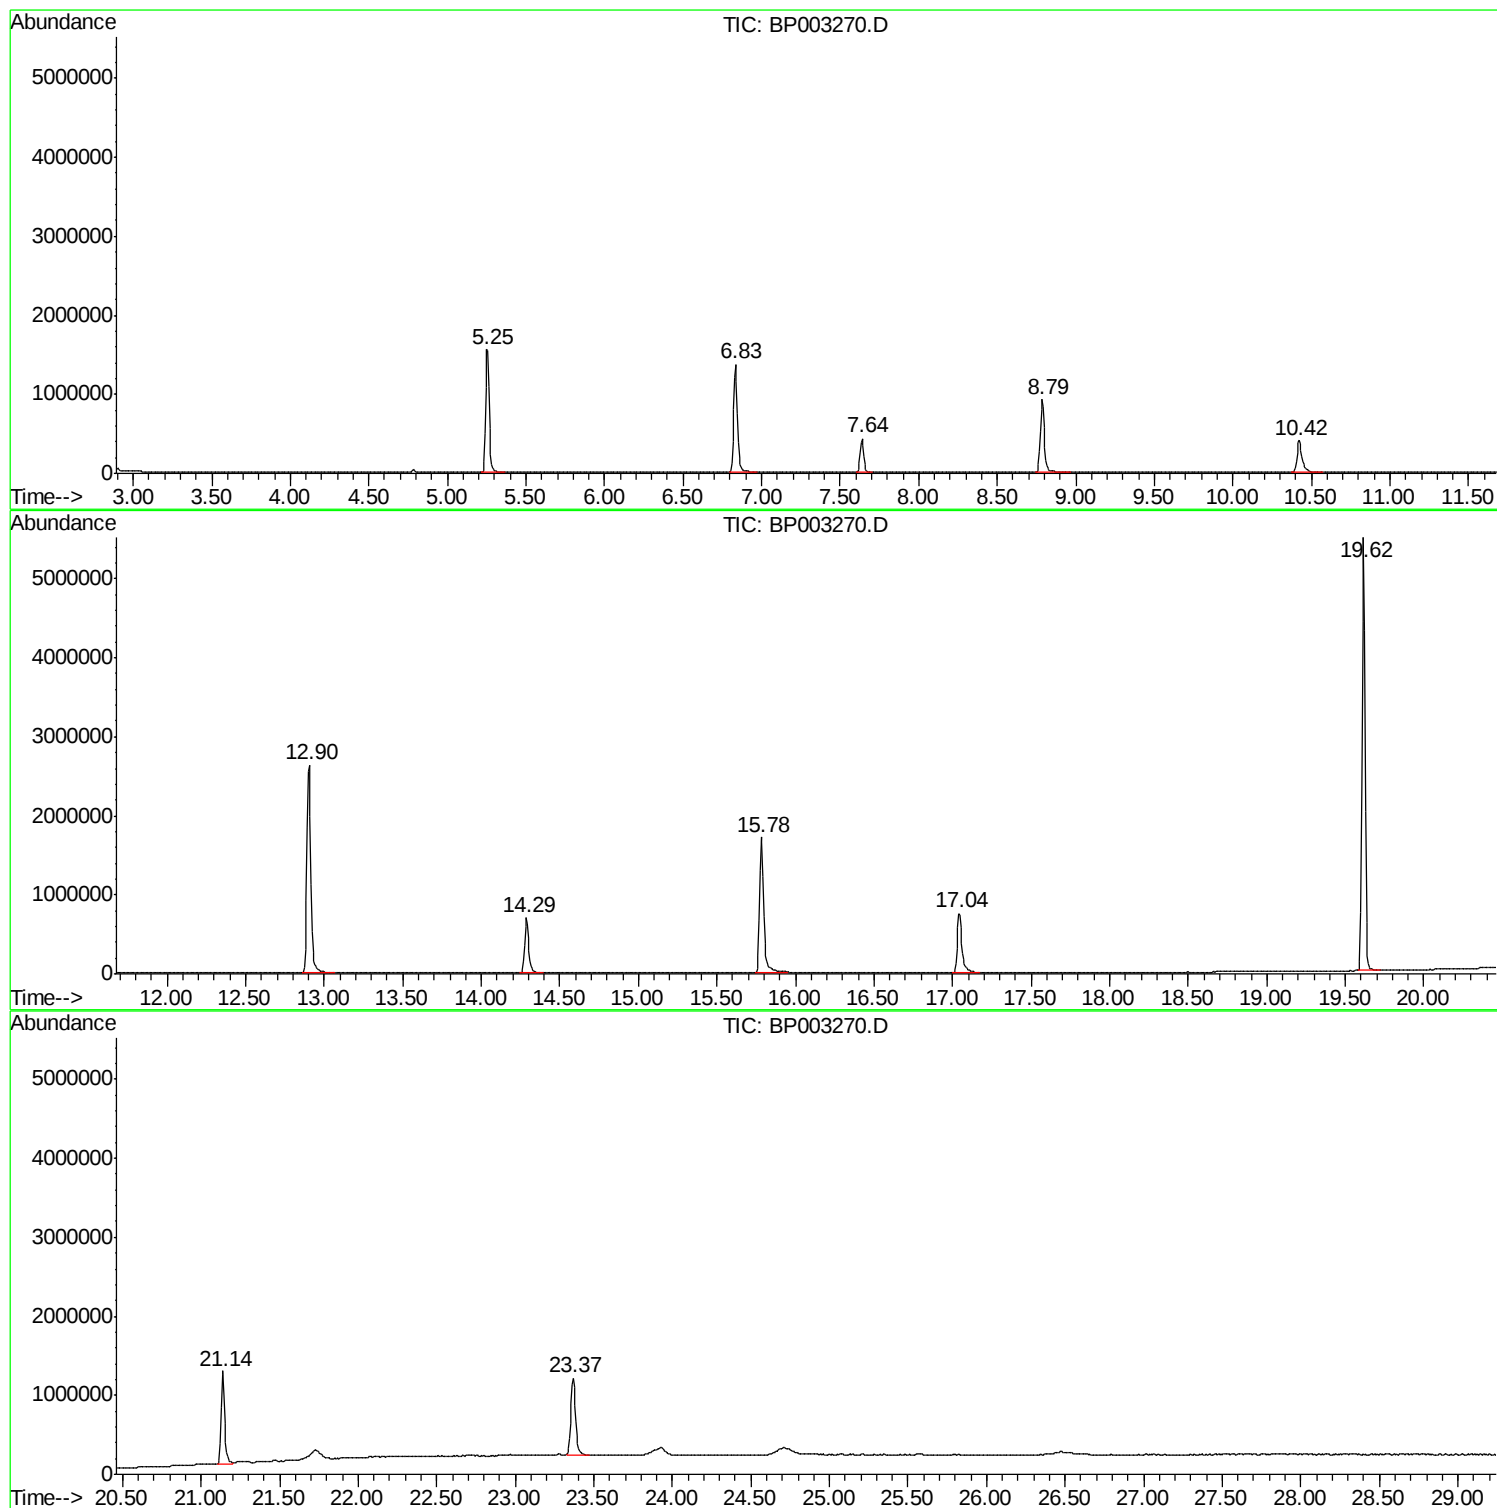

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091420\
Data File : BP003270.D
Acq On : 14 Sep 2020 16:00
Operator : CG/JU
Sample : PB131580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131580BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091420\
Data File : BP003270.D
Acq On : 14 Sep 2020 16:00
Operator : CG/JU
Sample : PB131580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131580BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc