


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091420\
 Data File : BP003268.D
 Acq On : 14 Sep 2020 14:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 14:37:05 2020

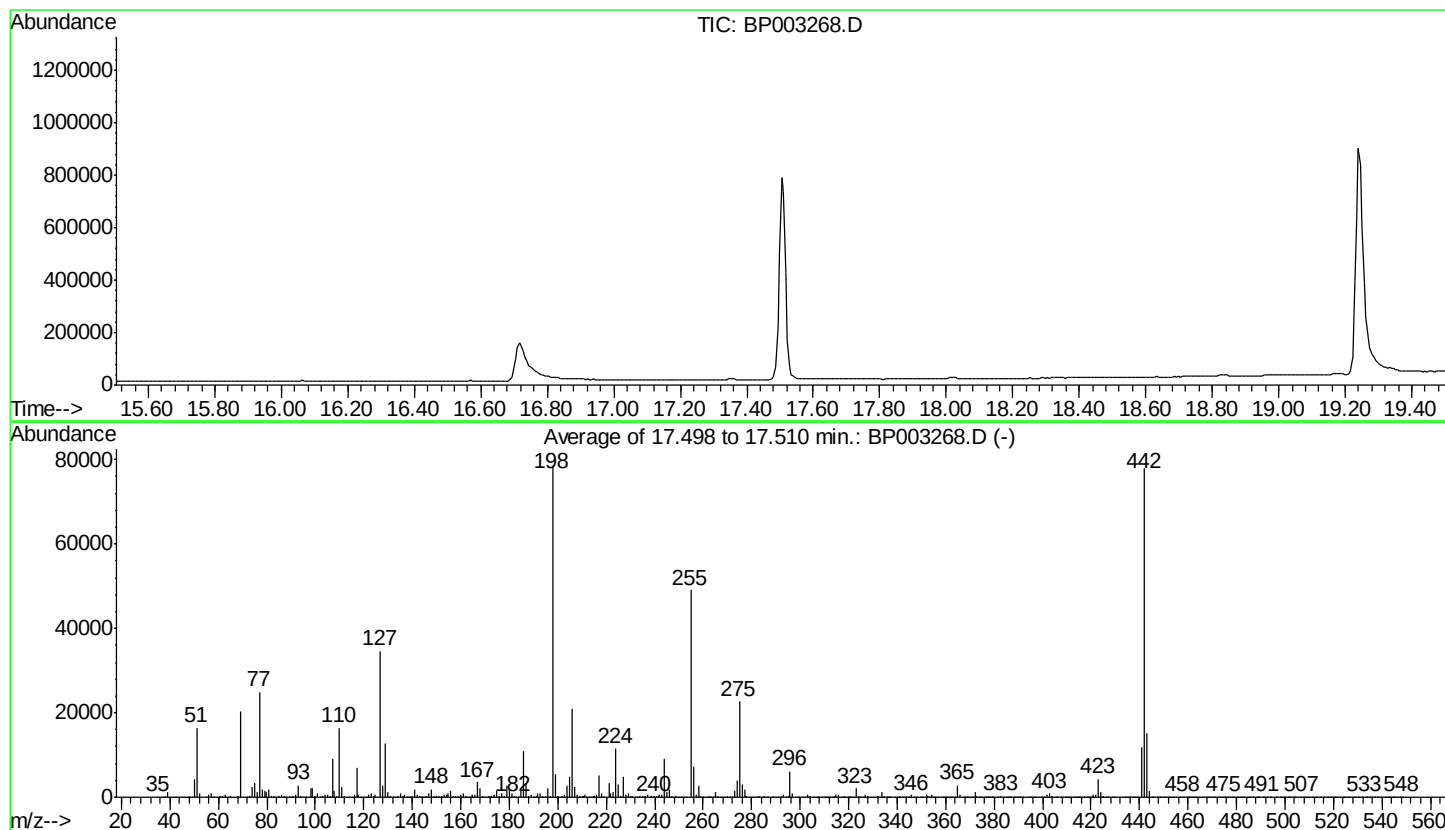

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	16534	PASS
68	69	0.00	2	1.9	380	PASS
69	198	0.00	100	25.8	20265	PASS
70	69	0.00	2	0.4	88	PASS
127	198	10	80	44.1	34650	PASS
197	198	0.00	2	0.3	236	PASS
198	198	100	100	100.0	78580	PASS
199	198	5	9	7.1	5545	PASS
275	198	10	60	28.9	22701	PASS
365	198	1	100	3.6	2848	PASS
441	198	0.01	100	15.0	11782	PASS
442	198	50	100	99.3	78018	PASS
443	442	15	24	19.6	15273	PASS