



Pentachlorophenol

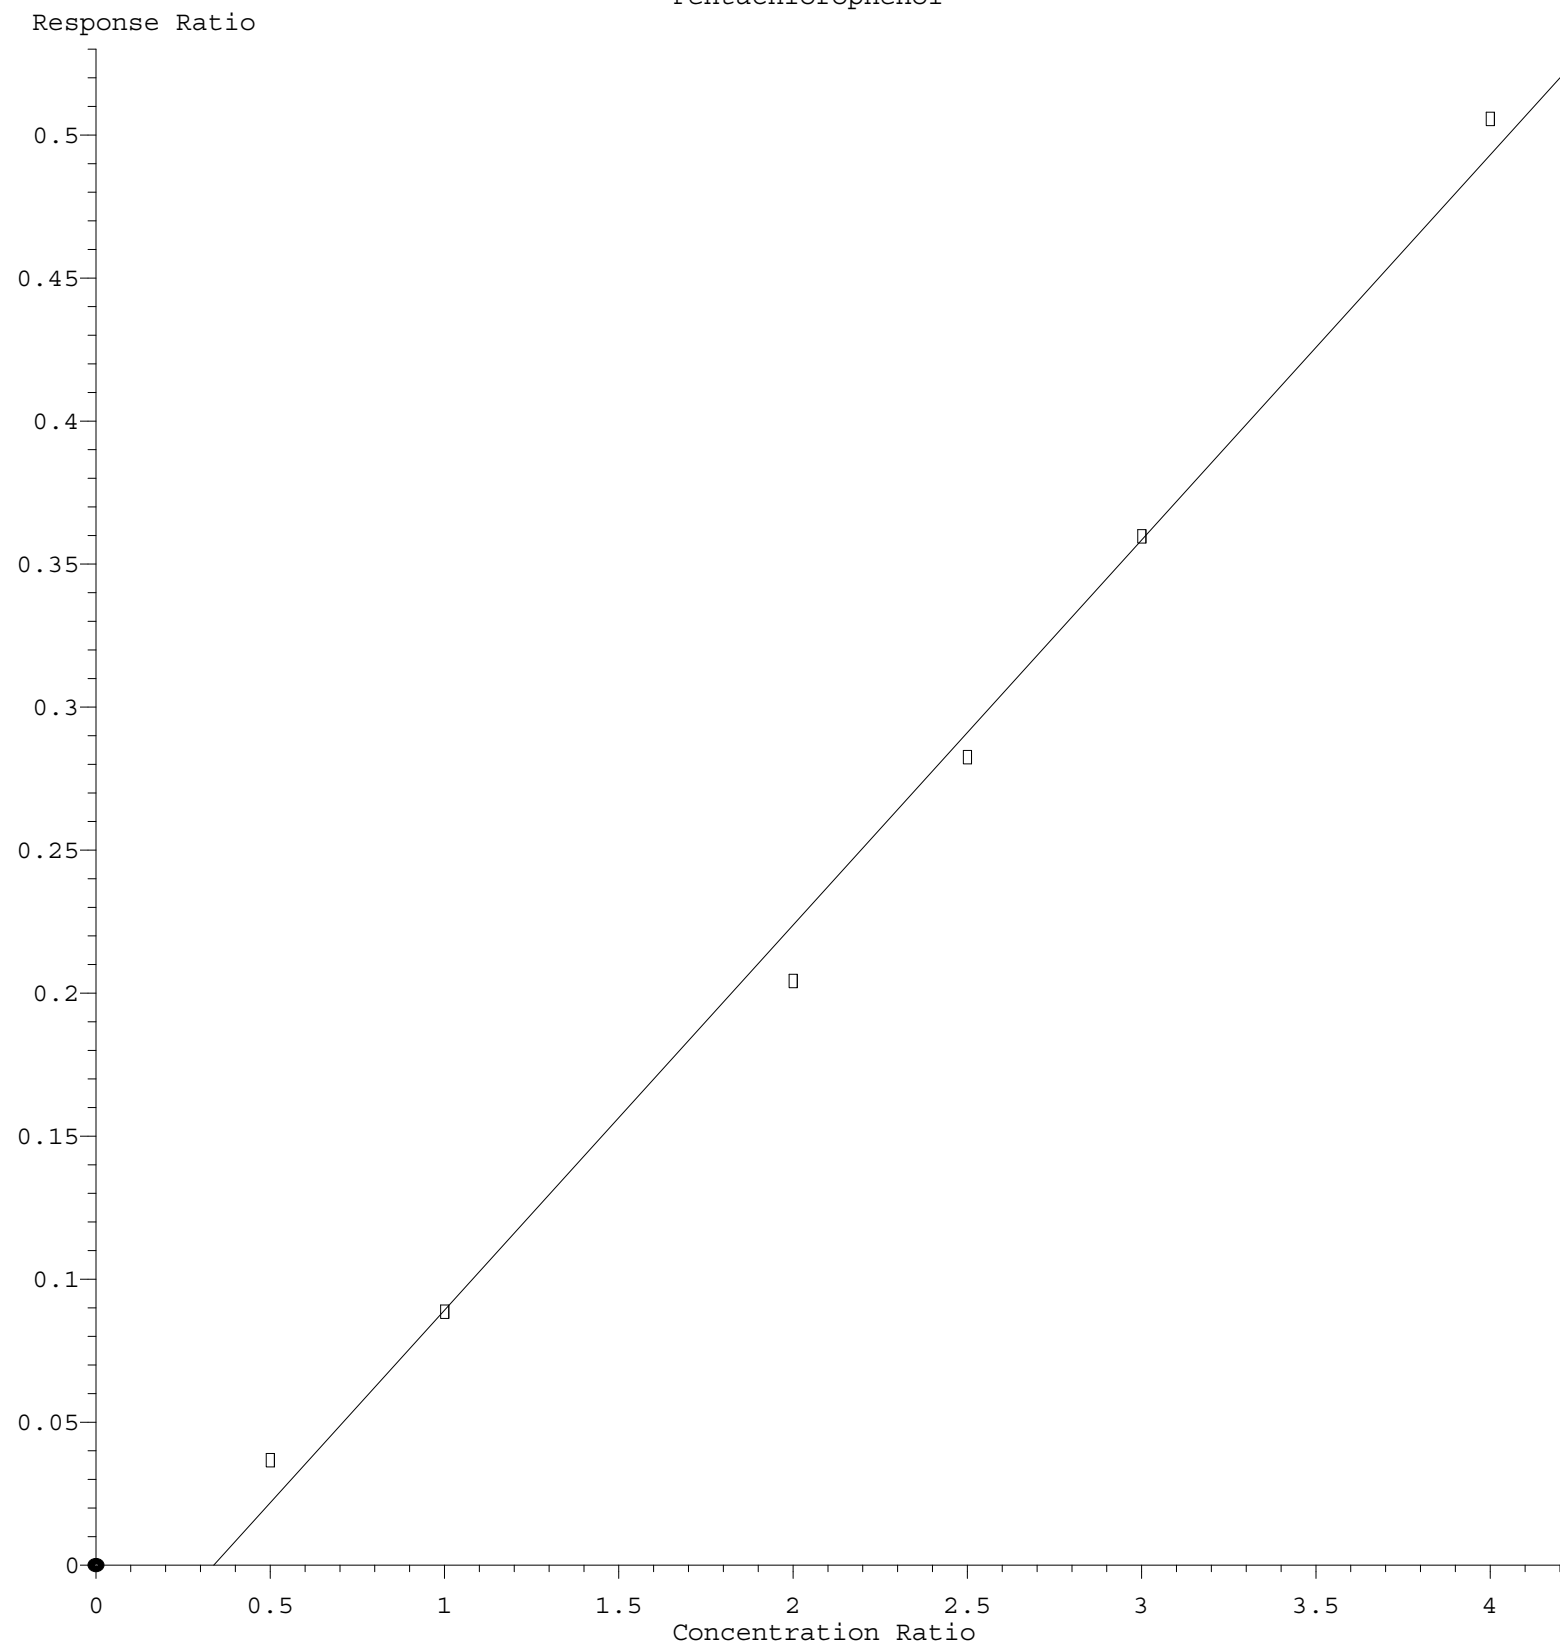

$\text{Response} = 1.347\text{e-}001 * \text{Amt} - 4.559\text{e-}002$
 Coef of Det (r^2) = 0.994500 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091520.M
 Calibration Table Last Updated: Wed Sep 16 13:18:39 2020


Benzoic acid

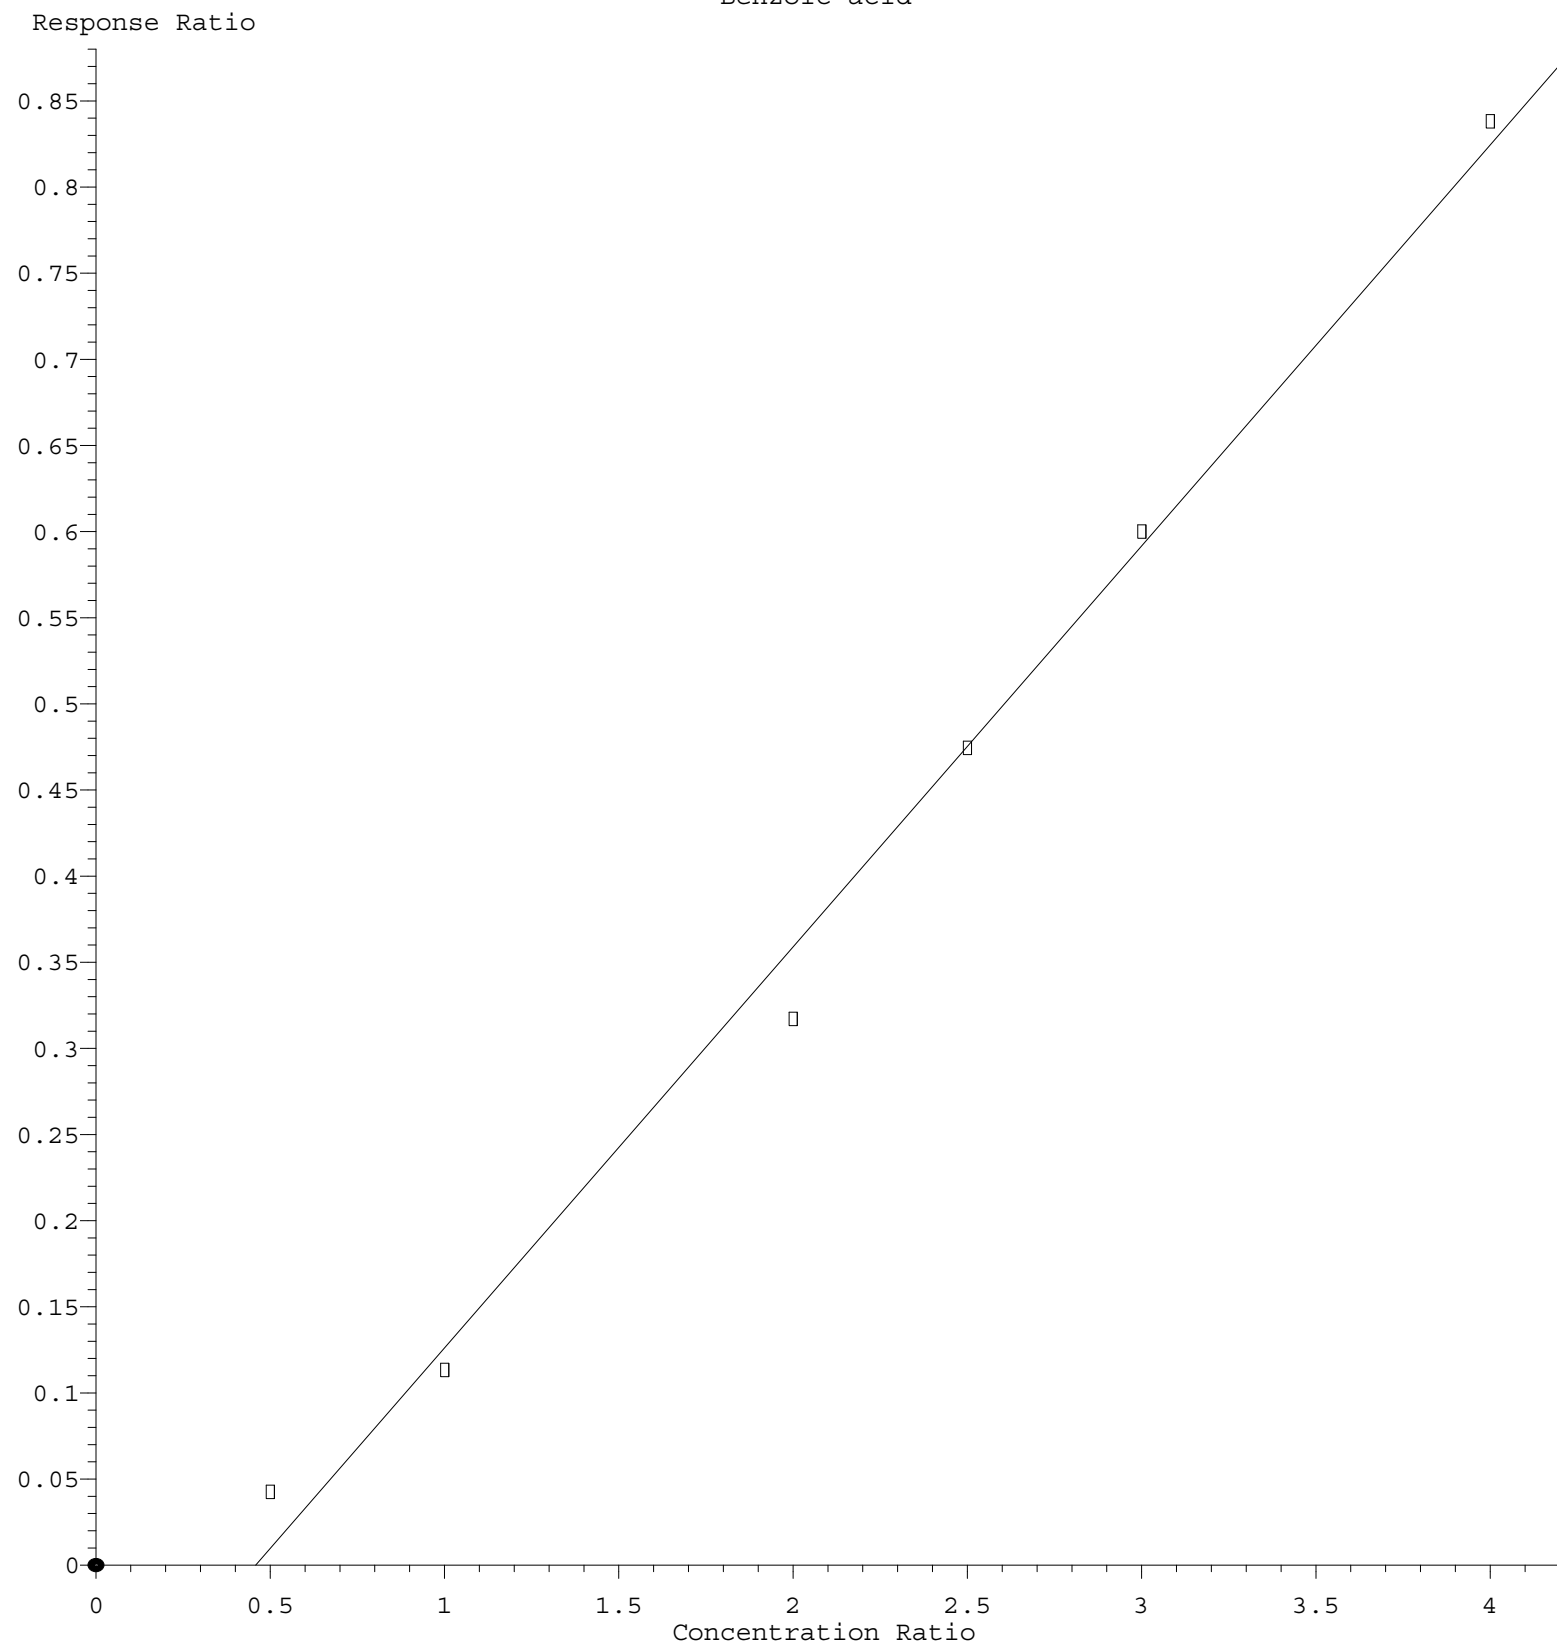

$\text{Response} = 2.327\text{e-}001 * \text{Amt} - 1.065\text{e-}001$
 Coef of Det (r^2) = 0.992849 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091520.M
 Calibration Table Last Updated: Wed Sep 16 13:18:39 2020


Hexachlorocyclopentadiene

Response Ratio

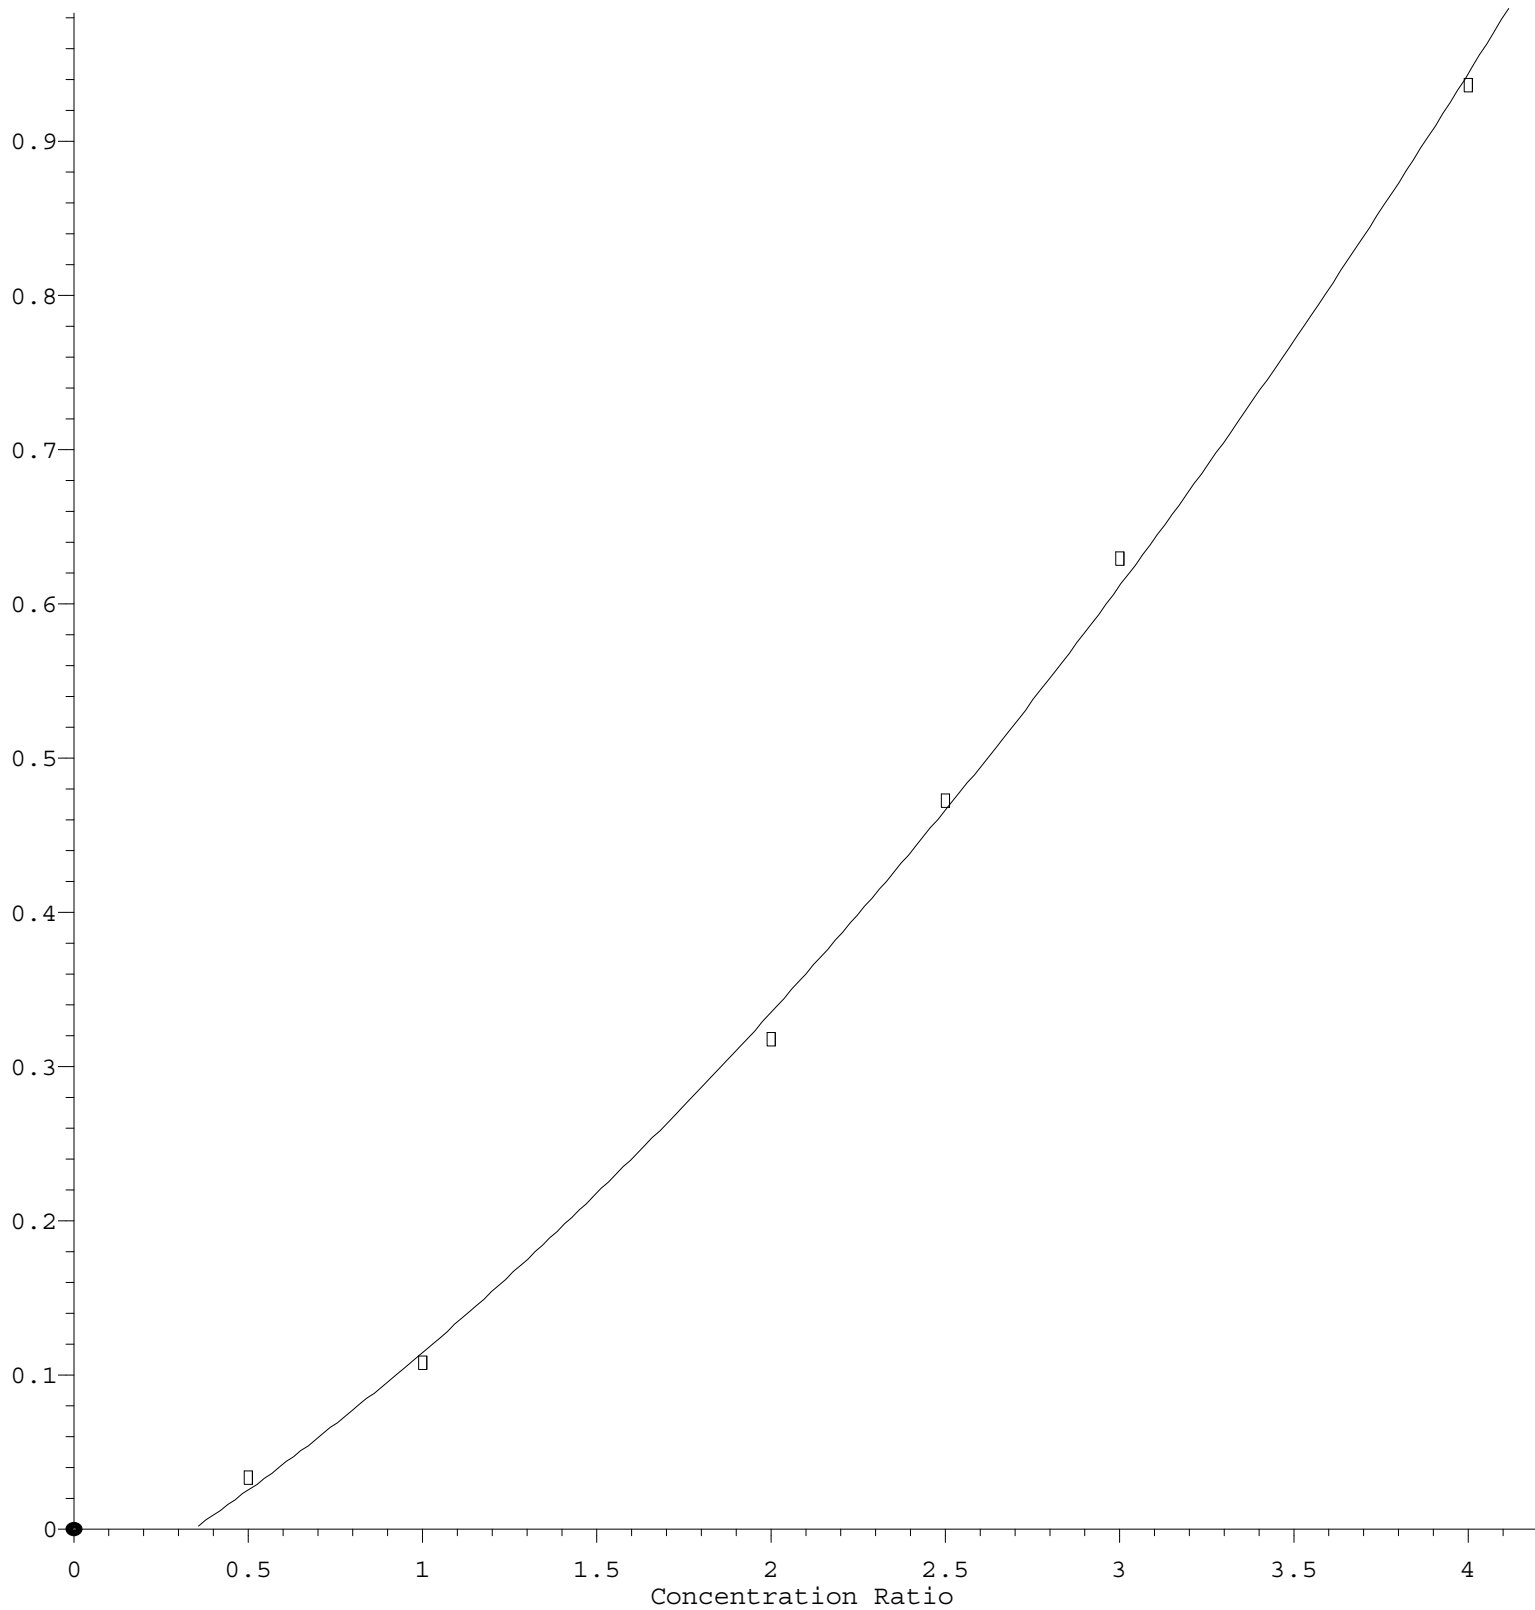

$R = 2.798e-002 A^2 + 1.366e-001 A - 4.995e-002$
Coef of Det (r^2) = 0.998551 Curve Fit: Quadratic
Method Name: Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091520.M
Calibration Table Last Updated: Wed Sep 16 13:18:39 2020

2,4-Dinitrophenol

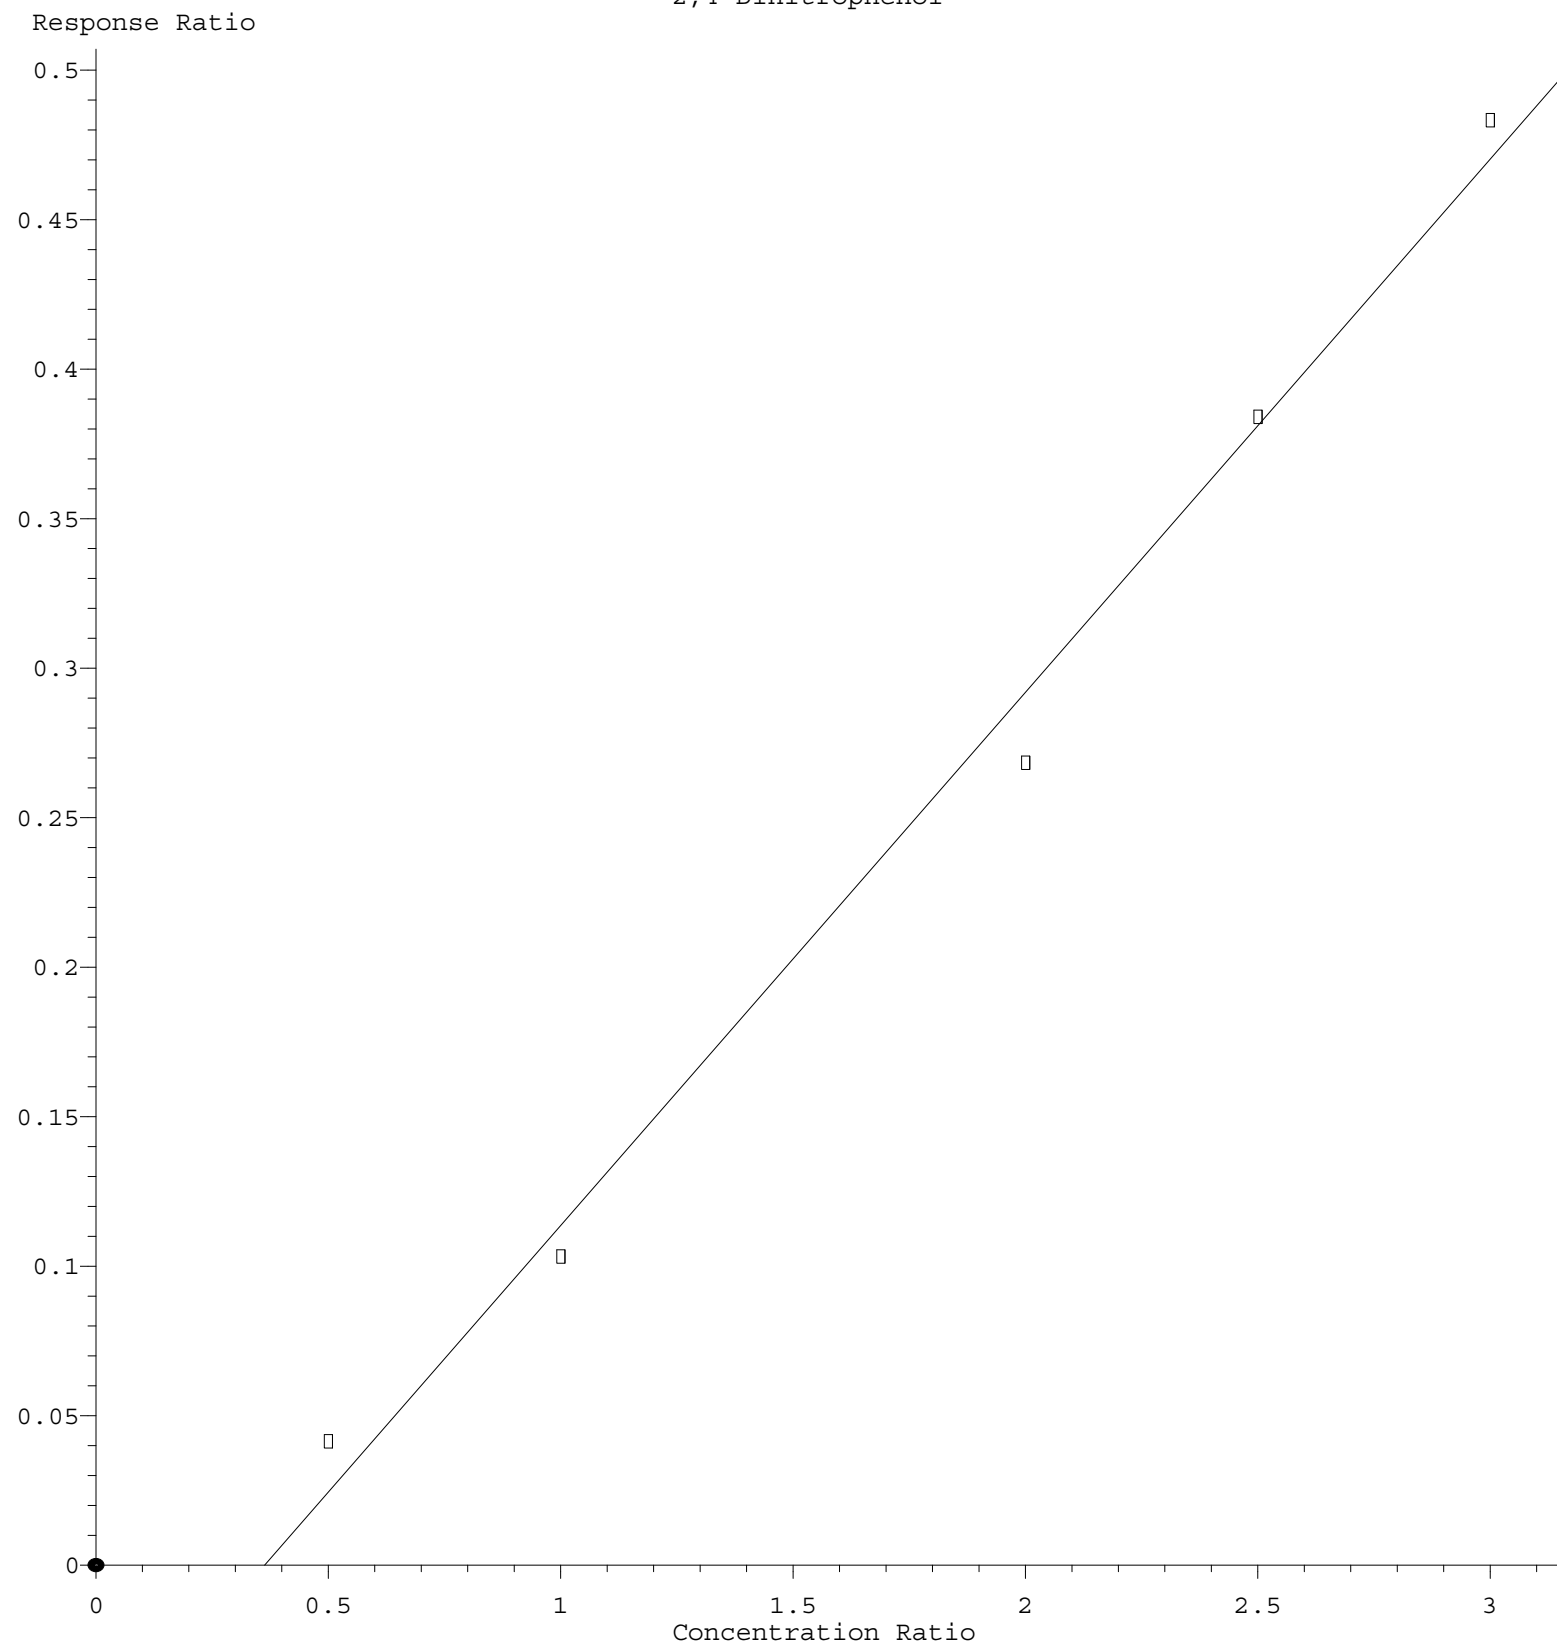

Response = $1.781e-001 * \text{Amt} - 6.459e-002$
 Coef of Det (r^2) = 0.991787 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091520.M
 Calibration Table Last Updated: Wed Sep 16 13:18:39 2020