

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091521\
 Data File : BP006978.D
 Acq On : 15 Sep 2021 16:47
 Operator : CG/JU
 Sample : PB138901BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	54	rVB	134925	180083	1.93%	0.180%
2	3.770	112	116	142	rBV	1423091	2368112	25.36%	2.366%
3	4.099	168	172	179	rVB	27630	37431	0.40%	0.037%
4	4.322	206	210	216	rVB6	9763	15458	0.17%	0.015%
5	4.734	278	280	290	rVB5	8609	12189	0.13%	0.012%
6	7.081	668	679	692	rBV	1636748	2654680	28.43%	2.653%
7	7.252	700	708	723	rBV	1419454	2245553	24.04%	2.244%
8	7.452	735	742	753	rBV	1755780	2774123	29.70%	2.772%
9	7.922	814	822	832	rBV	1490563	2378762	25.47%	2.377%
10	8.622	934	941	955	rBV	2163375	3370057	36.09%	3.367%
11	9.081	1011	1019	1028	rBV	1574035	2558154	27.39%	2.556%
12	9.805	1132	1142	1161	rBV	1222132	1979403	21.19%	1.978%
13	10.334	1224	1232	1245	rBV	2012135	3424681	36.67%	3.422%
14	10.722	1287	1298	1307	rBV	2077149	3449345	36.93%	3.447%
15	10.857	1312	1321	1339	rBV	2025125	3541522	37.92%	3.539%
16	12.310	1560	1568	1574	rBV	37436	68185	0.73%	0.068%
17	12.522	1600	1604	1610	rBV7	5963	9785	0.10%	0.010%
18	13.528	1771	1775	1779	rVB5	7440	12315	0.13%	0.012%
19	13.957	1841	1848	1859	rBV	3819893	5240862	56.12%	5.237%
20	14.240	1889	1896	1911	rBV	4408006	6436560	68.92%	6.431%
21	14.545	1941	1948	1961	rBV	3230954	4774968	51.13%	4.771%
22	14.728	1972	1979	1999	rBV	1493619	2271810	24.33%	2.270%
23	15.540	2110	2117	2129	rBV	5819976	8070533	86.42%	8.064%
24	15.651	2130	2136	2152	rVV	1413637	1942246	20.80%	1.941%
25	15.781	2153	2158	2164	rVB2	40081	64663	0.69%	0.065%
26	16.216	2228	2232	2240	rVB10	6613	13560	0.15%	0.014%
27	16.328	2245	2251	2256	rVB5	11131	19691	0.21%	0.020%
28	16.981	2356	2362	2366	rBV9	7951	13826	0.15%	0.014%
29	17.081	2375	2379	2388	rVB3	16259	28785	0.31%	0.029%
30	17.298	2409	2416	2425	rBV	3672937	5423416	58.07%	5.419%
31	17.392	2426	2432	2451	rVB	5717256	8429201	90.26%	8.422%
32	19.204	2736	2740	2745	rVB2	46736	64751	0.69%	0.065%
33	19.269	2747	2751	2758	rVV	64296	89700	0.96%	0.090%
34	19.628	2806	2812	2822	rBV	7002919	9339095	100.00%	9.332%
35	21.374	3104	3109	3118	rBV	3931436	4998698	53.52%	4.995%
36	23.639	3487	3494	3502	rBV2	3746579	7276884	77.92%	7.271%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091521\
Data File : BP006978.D
Acq On : 15 Sep 2021 16:47
Operator : CG/JU
Sample : PB138901BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK901

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Title : SVOA CALIBRATION

37	23.798	3514	3521	3534	rVB2	2206437	4501882	48.20%	4.498%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 100080969

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091521\
Data File : BP006978.D
Acq On : 15 Sep 2021 16:47
Operator : CG/JU
Sample : PB138901BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK901

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

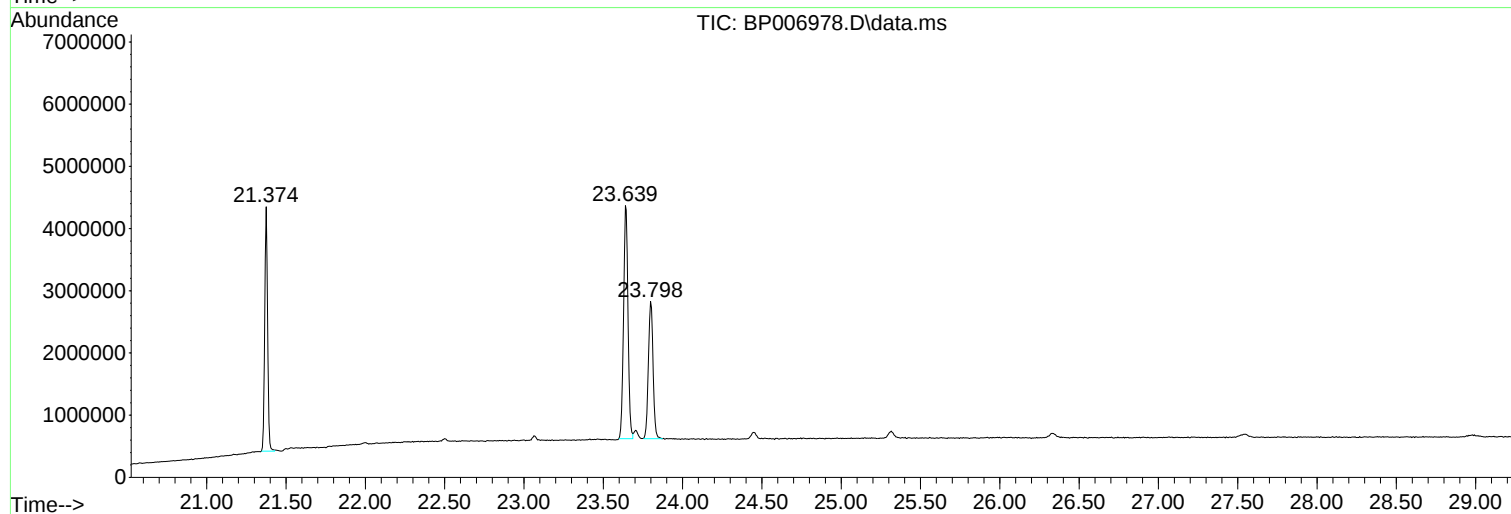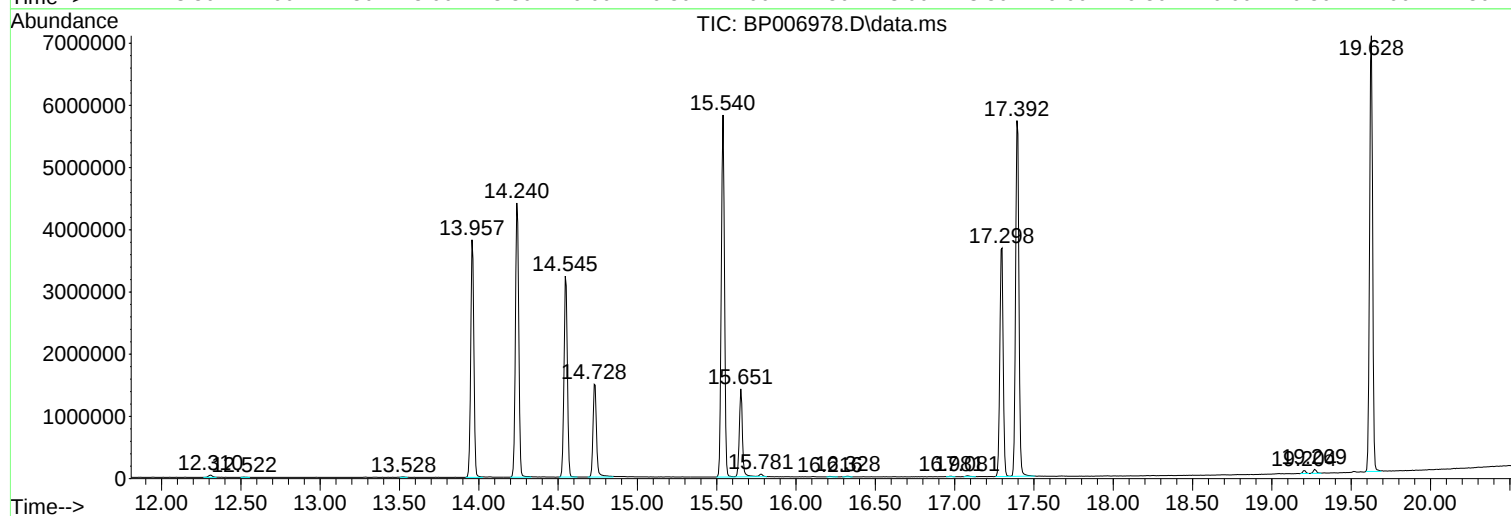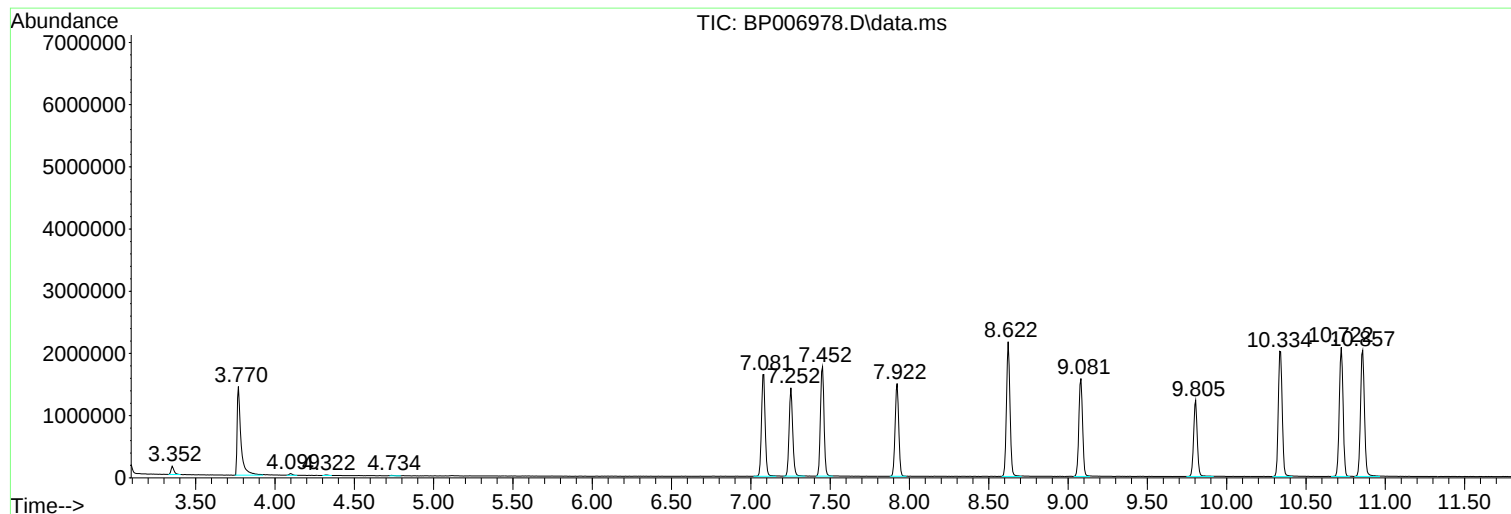

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091521\
Data File : BP006978.D
Acq On : 15 Sep 2021 16:47
Operator : CG/JU
Sample : PB138901BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK901

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091521\
Data File : BP006978.D
Acq On : 15 Sep 2021 16:47
Operator : CG/JU
Sample : PB138901BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK901

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
