
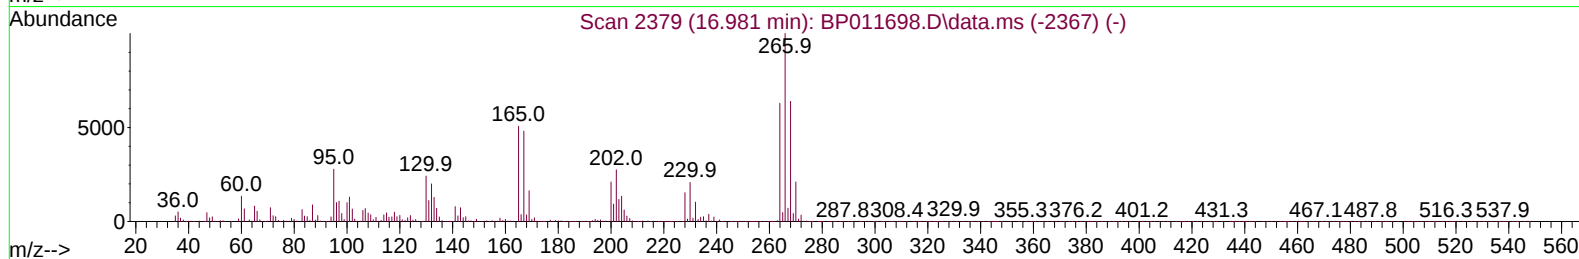
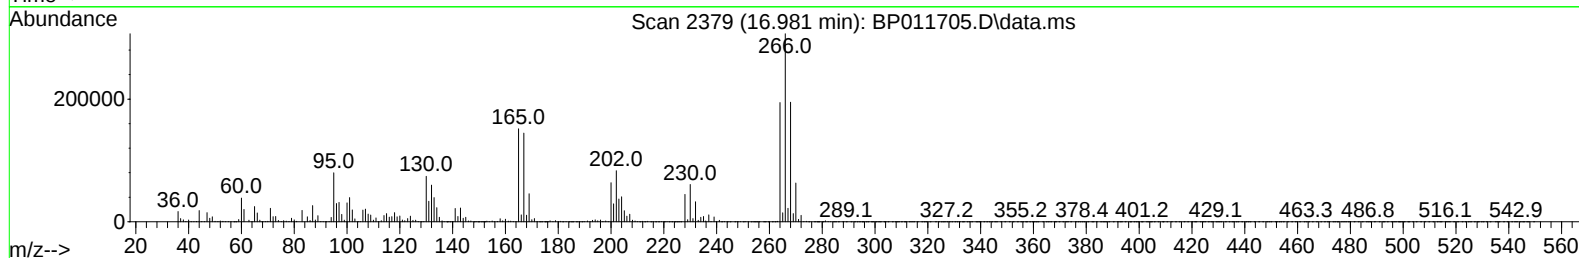


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
Data File : BP011705.D
Acq On : 15 Sep 2022 09:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 15:58:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 19:12:50 2022
Response via : Initial Calibration

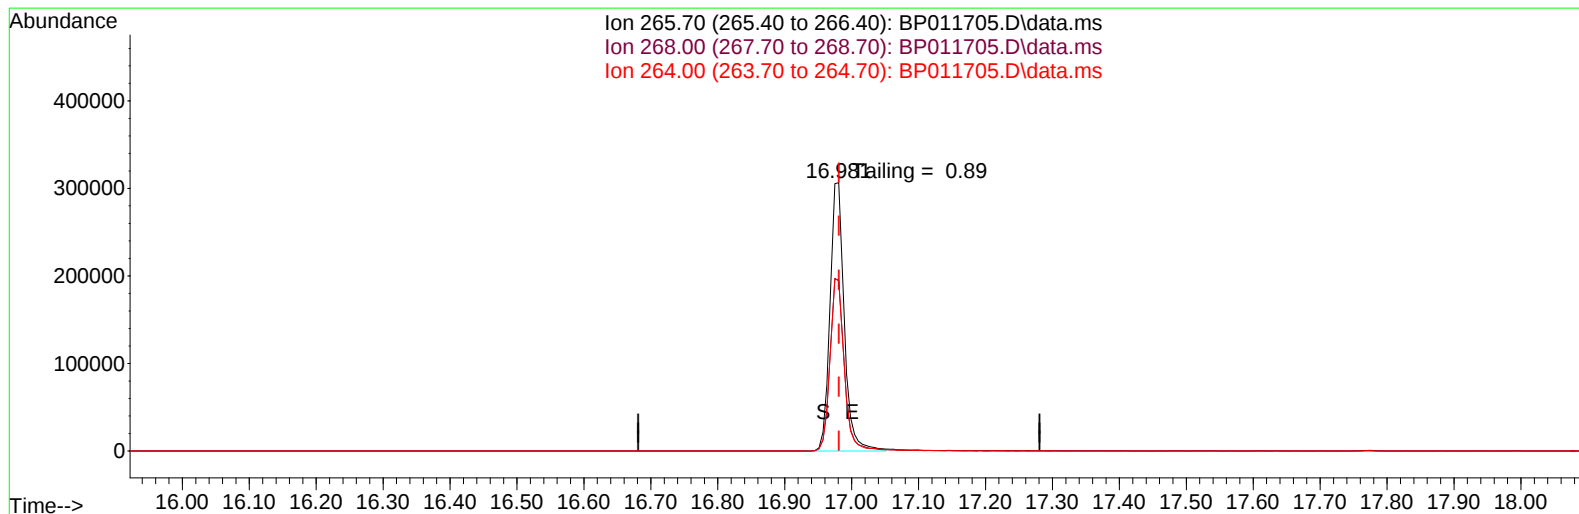

TIC: BP011705.D\data.ms

(70) Pentachlorophenol (C)




16.981min (-0.000) 336641.86 ng

response 458616

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.62
264.00	63.00	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
Data File : BP011705.D
Acq On : 15 Sep 2022 09:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 15:58:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 19:12:50 2022
Response via : Initial Calibration

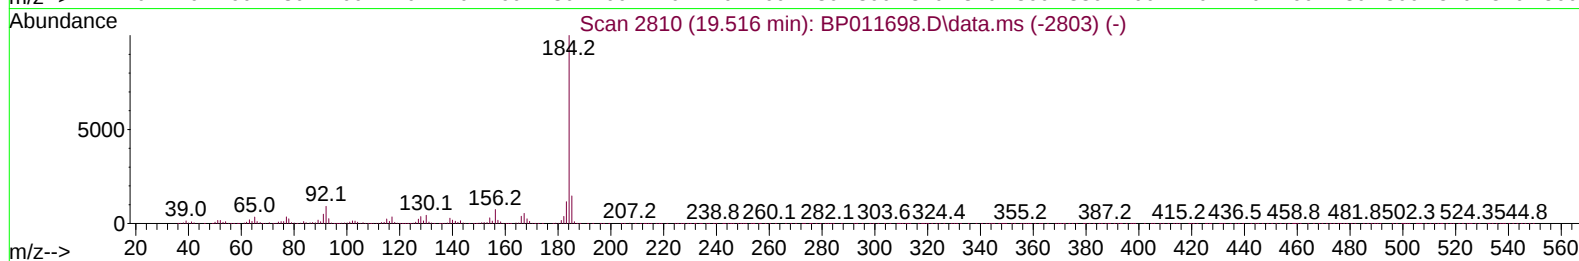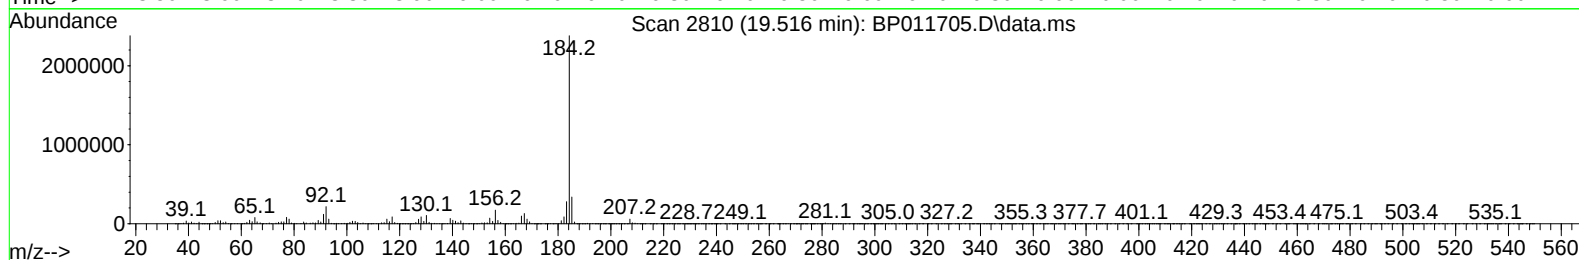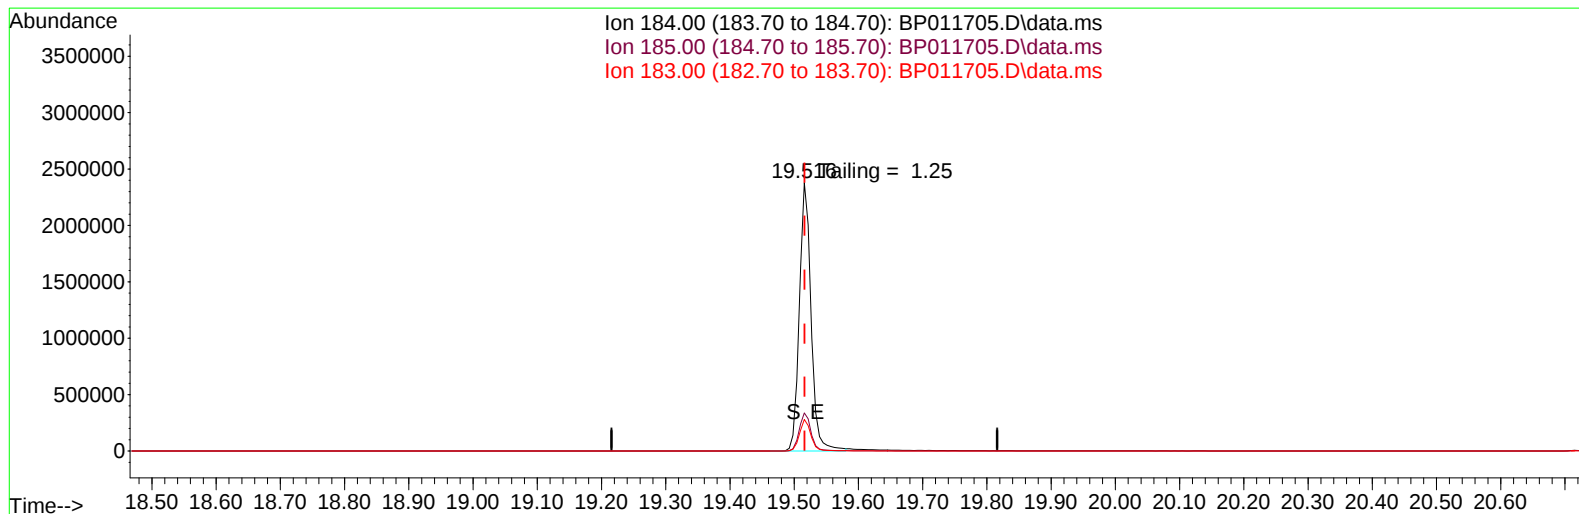

TIC: BP011705.D\data.ms

(77) Benzidine**19.516min (-0.000) 1528957.82 ng****response 3090706**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.19
183.00	11.30	11.78
0.00	0.00	0.00