
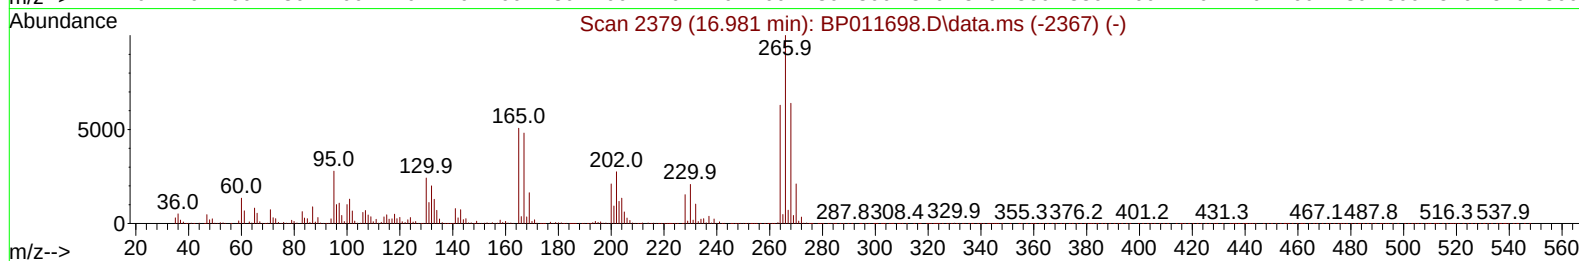
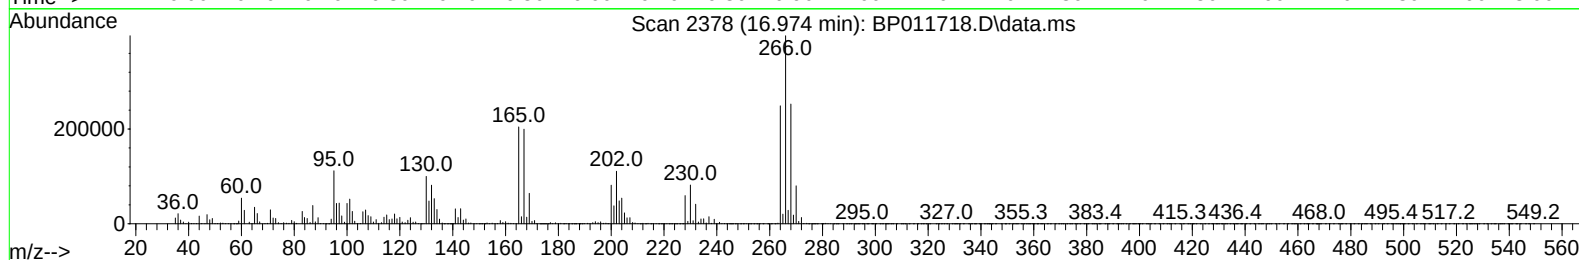


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
 Data File : BP011718.D
 Acq On : 15 Sep 2022 22:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 08:02:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 19:12:50 2022
 Response via : Initial Calibration

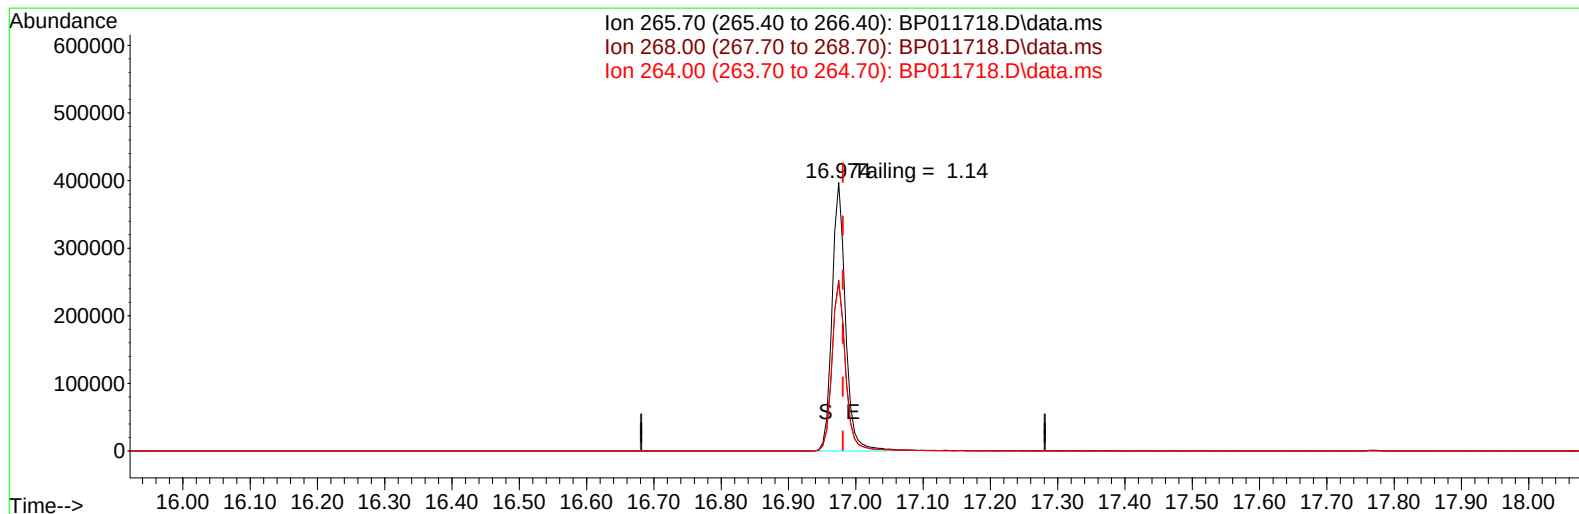

TIC: BP011718.D\data.ms

(70) Pentachlorophenol (C)




16.974min (-0.007) 3930232.50 ng

response 553022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.69
264.00	63.00	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
Data File : BP011718.D
Acq On : 15 Sep 2022 22:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 08:02:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 19:12:50 2022
Response via : Initial Calibration

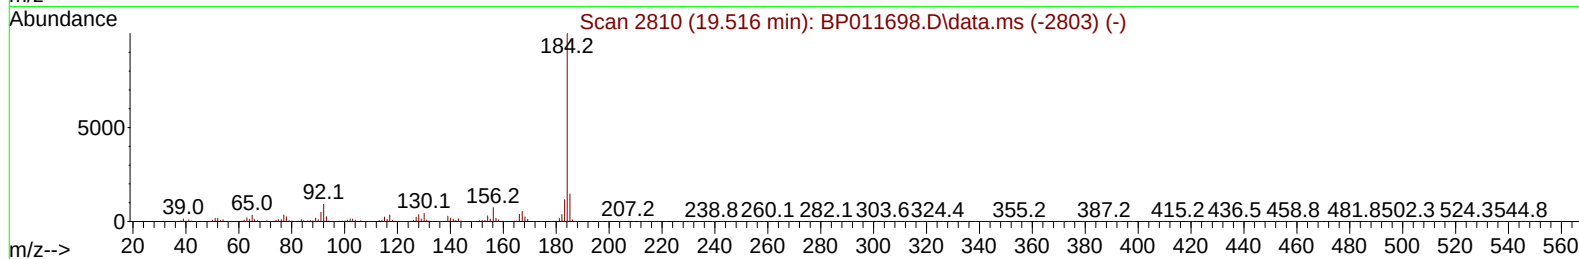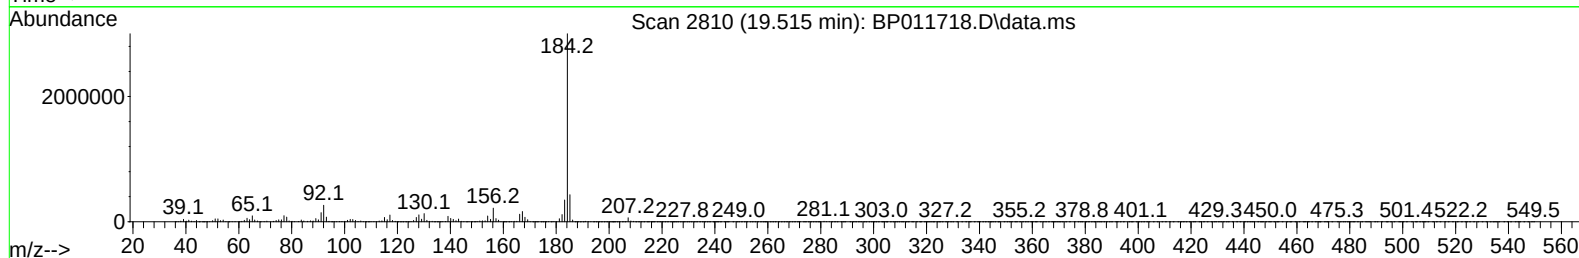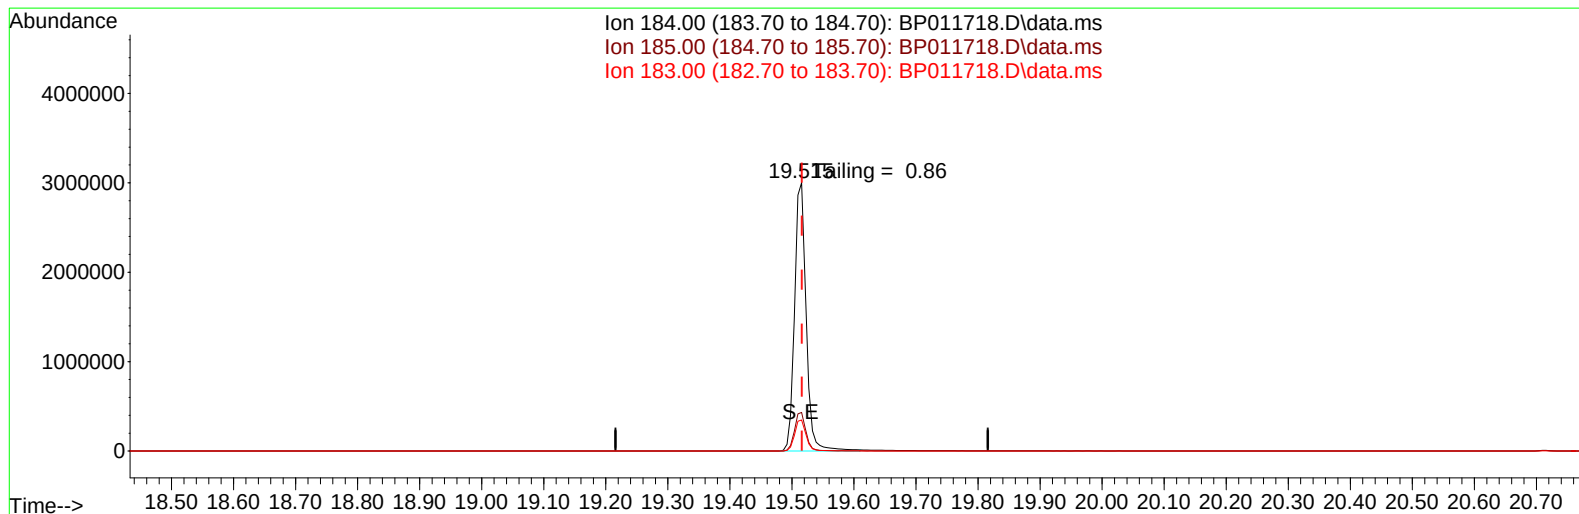

TIC: BP011718.D\data.ms

(77) Benzidine**19.515min (-0.000) 50973.74 ng****response 3962823**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.36
183.00	11.30	11.56
0.00	0.00	0.00