


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
 Data File : BP011705.D
 Acq On : 15 Sep 2022 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 19:12:50 2022

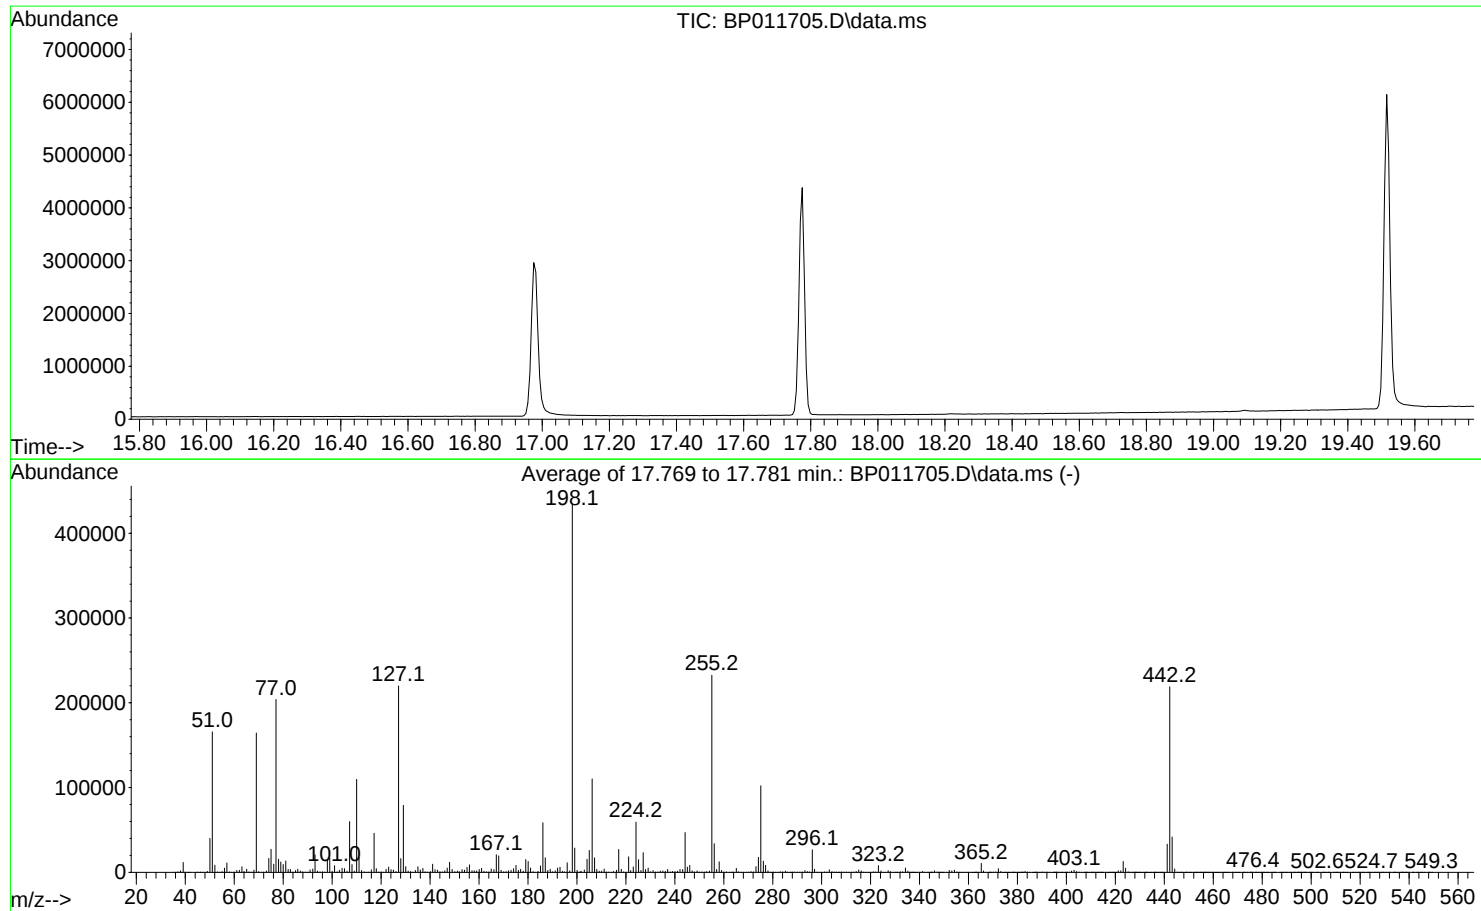




AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	165710	PASS
68	69	0.00	2	1.5	2514	PASS
69	198	0.00	100	37.9	164422	PASS
70	69	0.00	2	0.6	905	PASS
127	198	10	80	50.7	219910	PASS
197	198	0.00	2	0.4	1639	PASS
198	198	100	100	100.0	434048	PASS
199	198	5	9	6.6	28579	PASS
275	198	10	60	23.5	102094	PASS
365	198	1	100	2.4	10525	PASS
441	198	0.01	100	7.6	33075	PASS
442	442	100	100	100.0	218923	PASS
443	442	15	24	19.0	41654	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
 Data File : BP011705.D
 Acq On : 15 Sep 2022 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 15:58:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 19:12:50 2022
 Response via : Initial Calibration

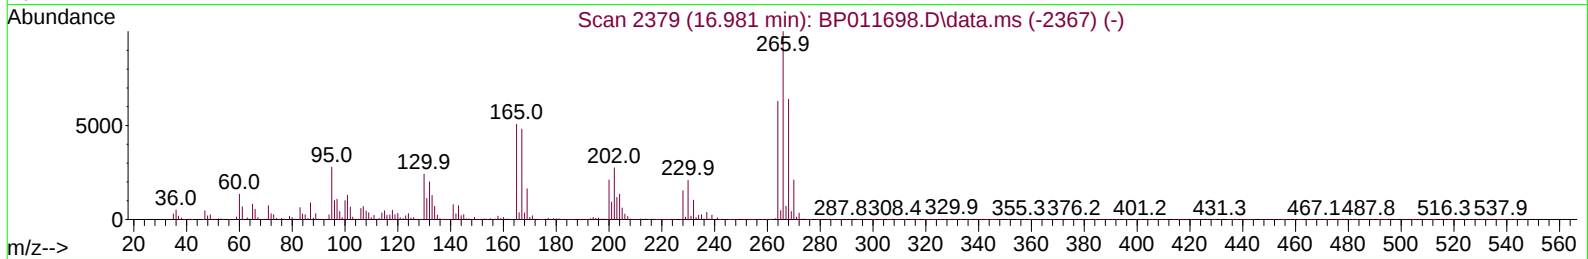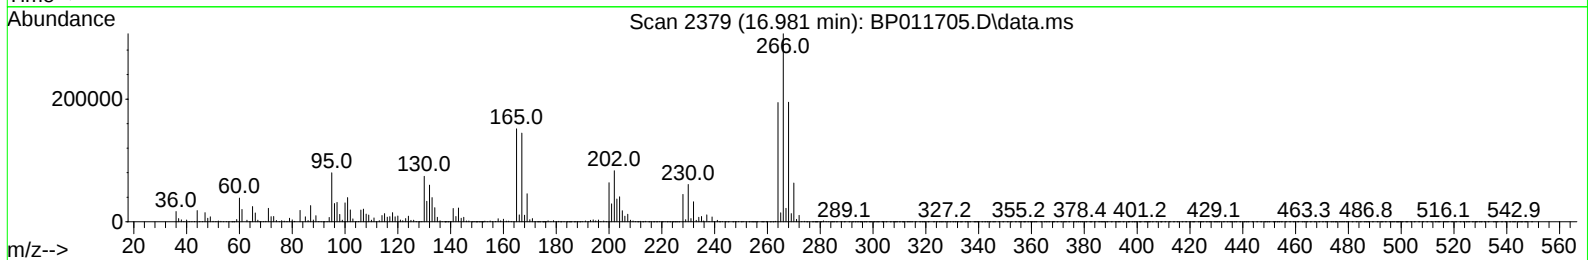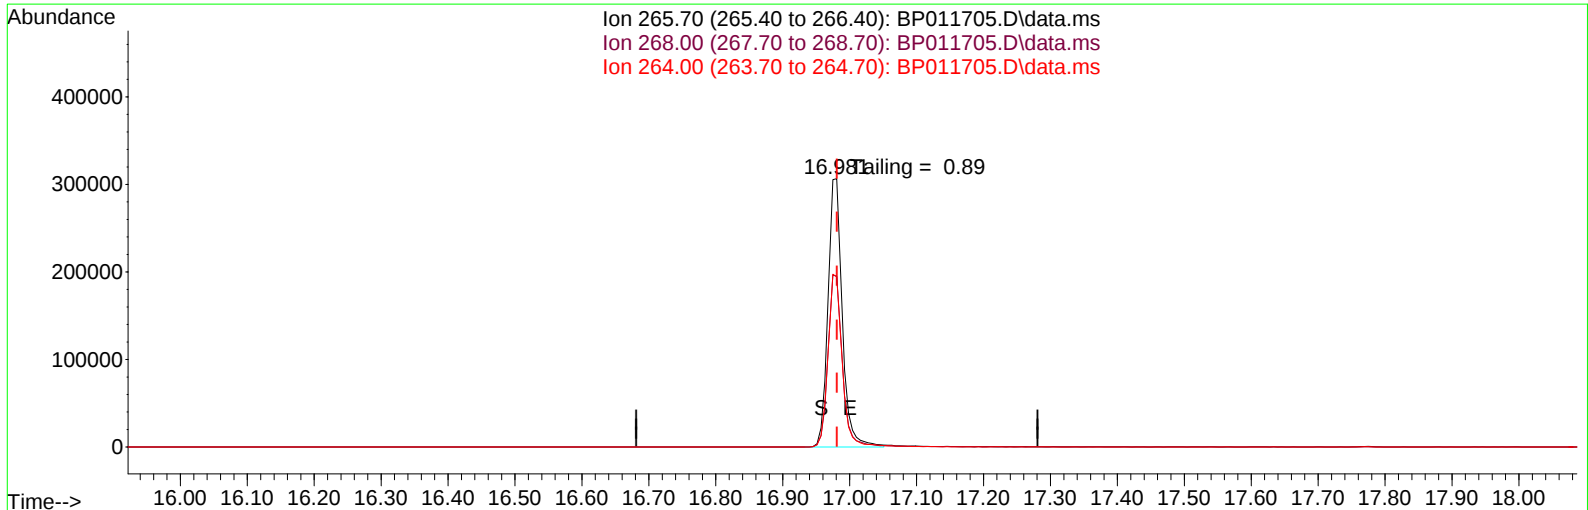

TIC: BP011705.D\data.ms

(70) Pentachlorophenol (C)

16.981min (-0.000) 336641.86 ng




response 458616

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.62
264.00	63.00	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
 Data File : BP011705.D
 Acq On : 15 Sep 2022 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 15:58:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 19:12:50 2022
 Response via : Initial Calibration

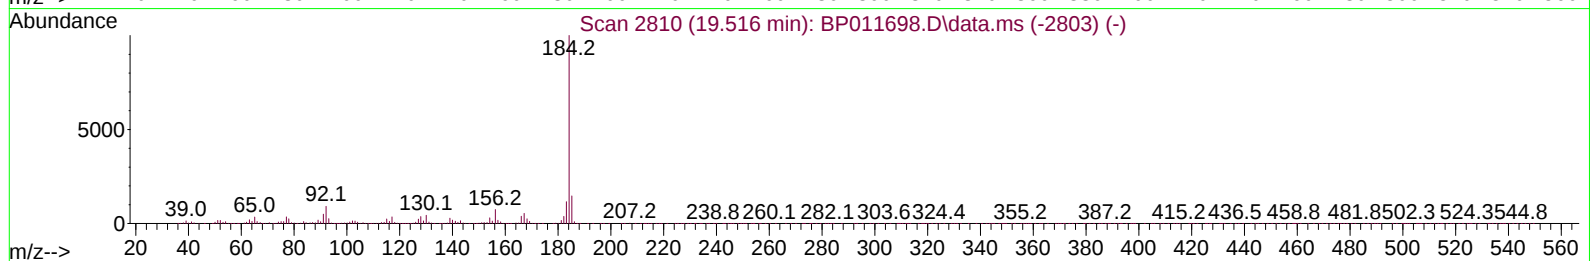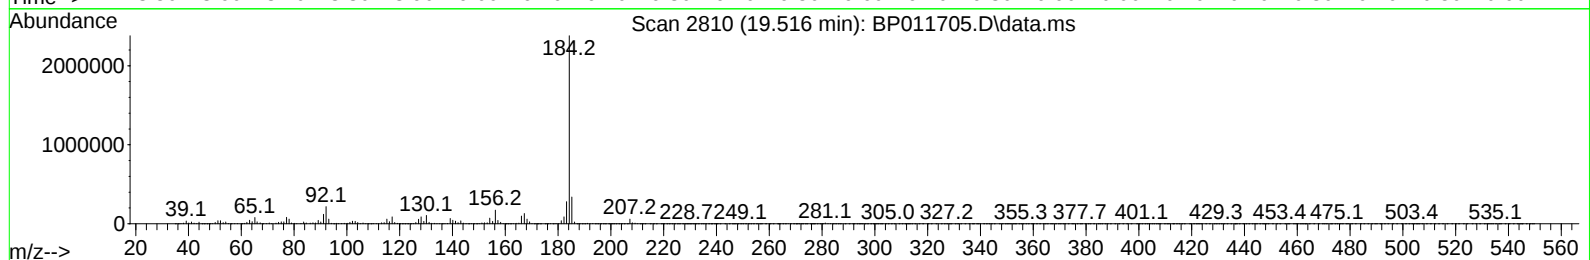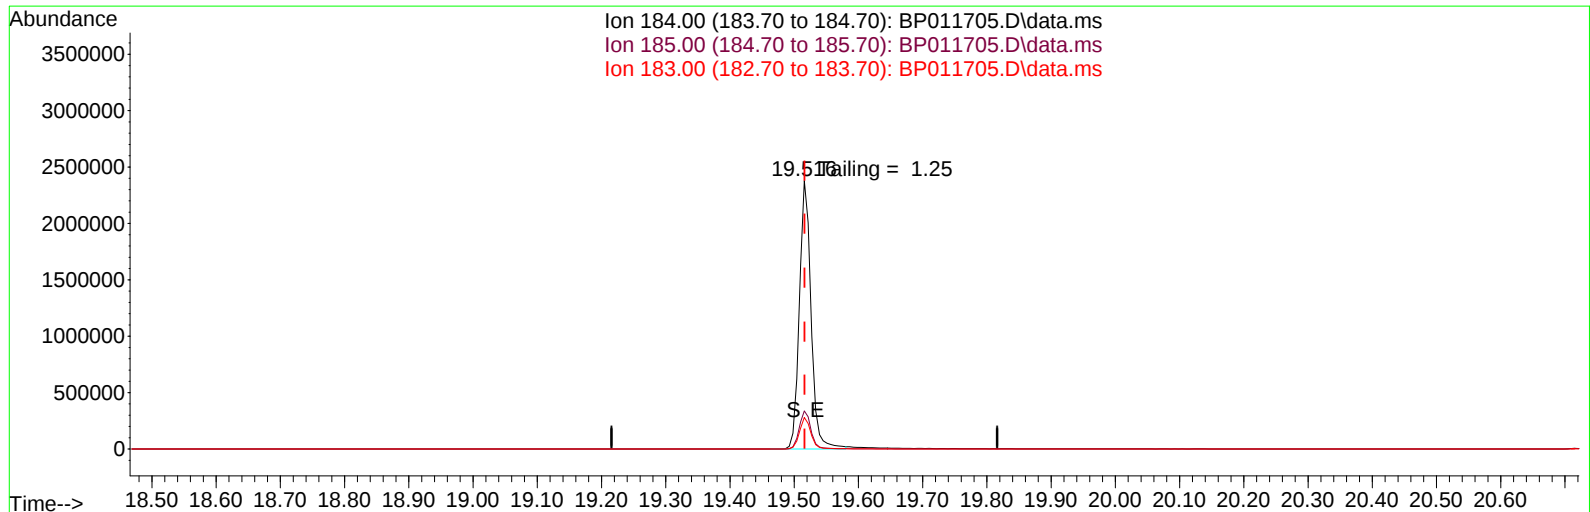

TIC: BP011705.D\data.ms

(77) Benzidine

19.516min (-0.000) 1528957.82 ng

response 3090706

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.19
183.00	11.30	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/15/2022	BNA_P	<u>BP011705.D</u>
Compound Name	Response	Retention Time
DDT	1402001	20.71
DDD	6621	20.28
DDE	1155	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7776	1409777	0.55

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP