


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
 Data File : BP011718.D
 Acq On : 15 Sep 2022 22:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 19:12:50 2022

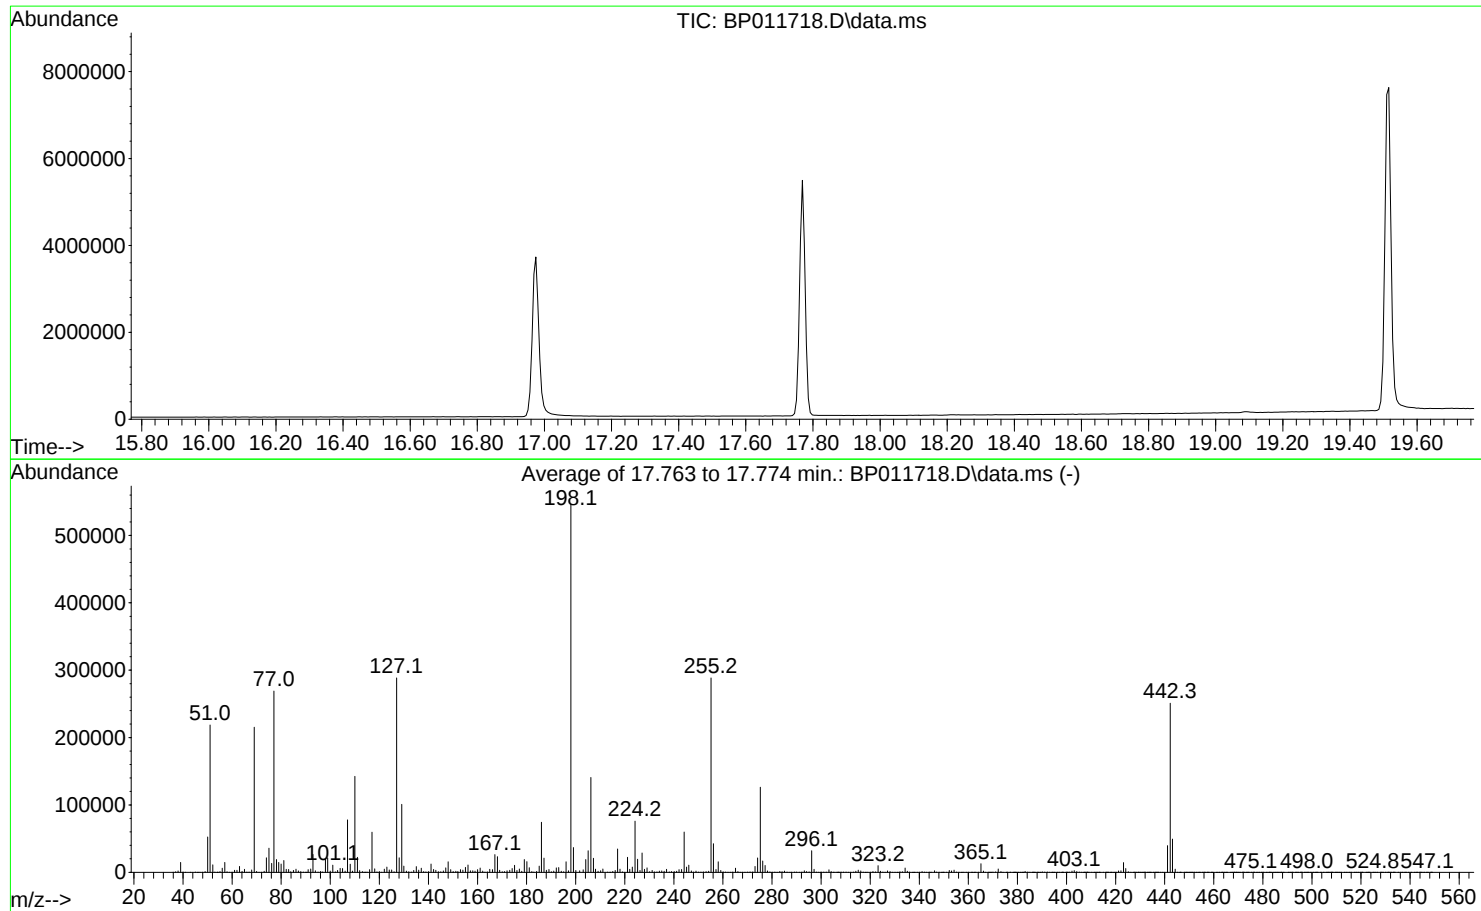




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	218783	PASS
68	69	0.00	2	1.6	3432	PASS
69	198	0.00	100	39.4	215422	PASS
70	69	0.00	2	0.6	1291	PASS
127	198	10	80	52.8	288504	PASS
197	198	0.00	2	0.4	2215	PASS
198	198	100	100	100.0	546094	PASS
199	198	5	9	6.7	36706	PASS
275	198	10	60	23.1	126147	PASS
365	198	1	100	2.3	12799	PASS
441	198	0.01	100	7.2	39464	PASS
442	442	100	100	100.0	250923	PASS
443	442	15	24	19.7	49416	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
Data File : BP011718.D
Acq On : 15 Sep 2022 22:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 08:02:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 19:12:50 2022
Response via : Initial Calibration

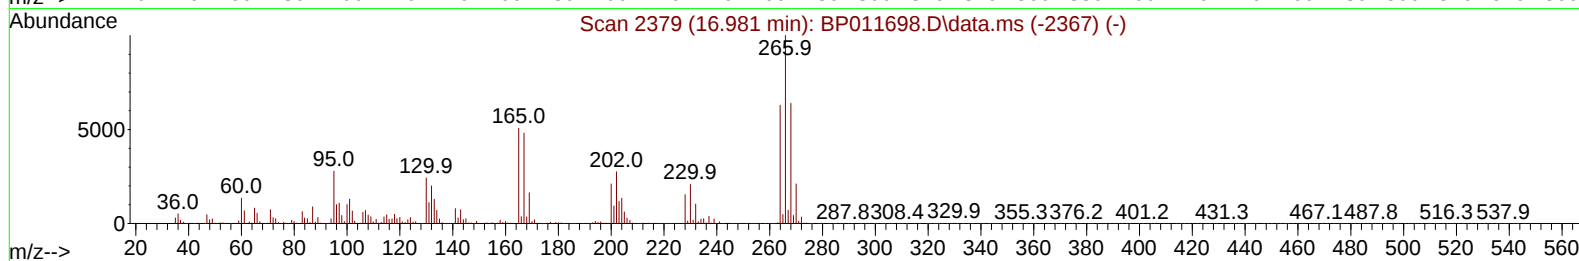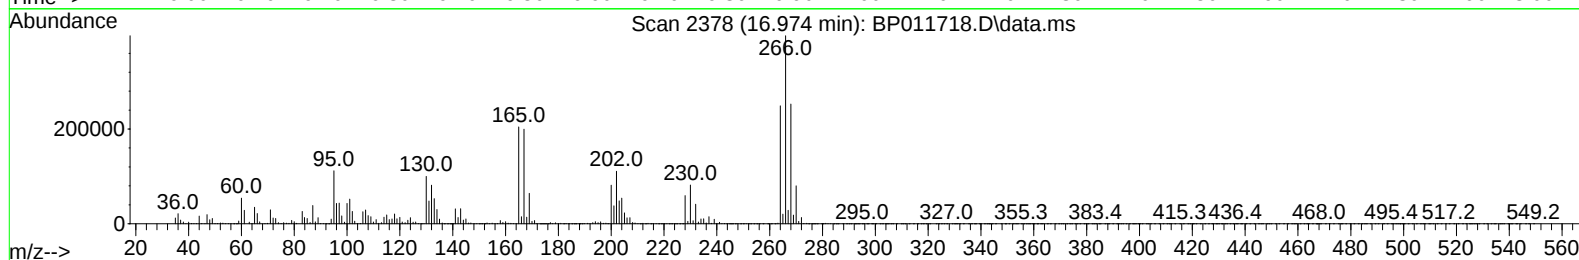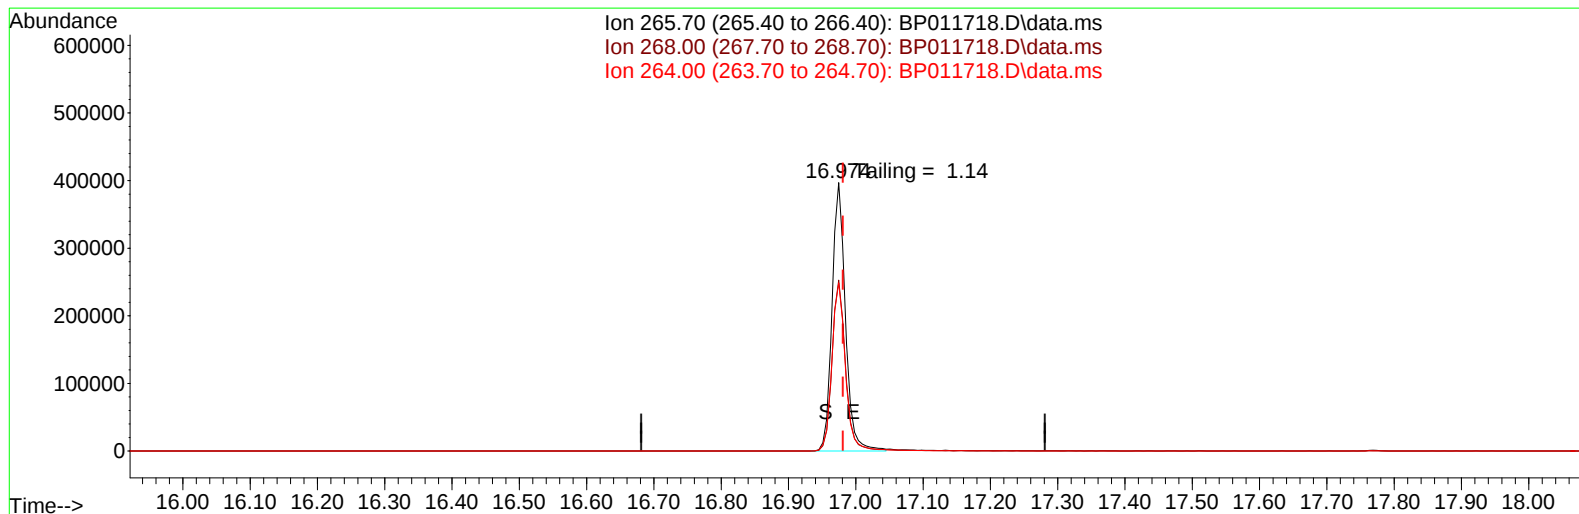

TIC: BP011718.D\data.ms

(70) Pentachlorophenol (C)

16.974min (-0.007) 3930232.50 ng




response 553022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.69
264.00	63.00	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091522\
 Data File : BP011718.D
 Acq On : 15 Sep 2022 22:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 16 08:02:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 19:12:50 2022
 Response via : Initial Calibration

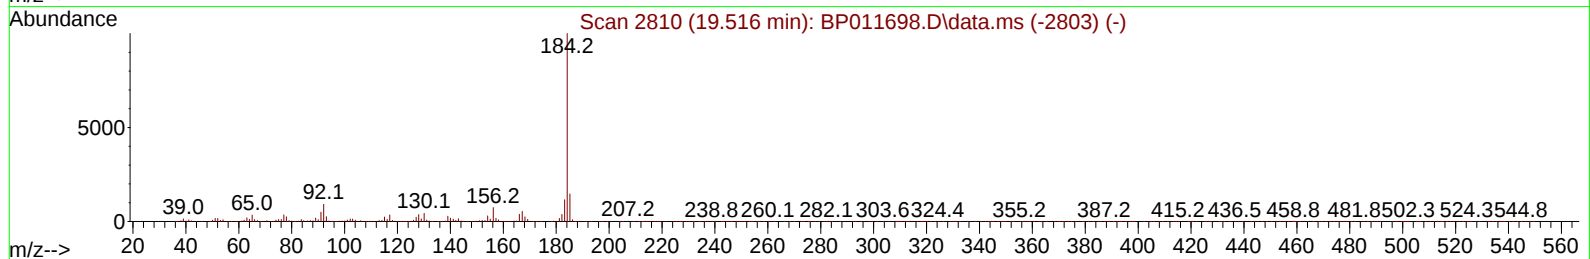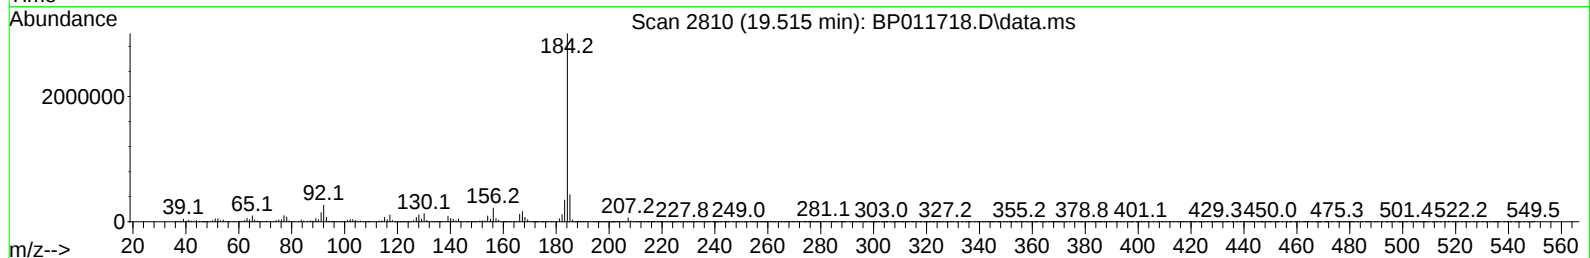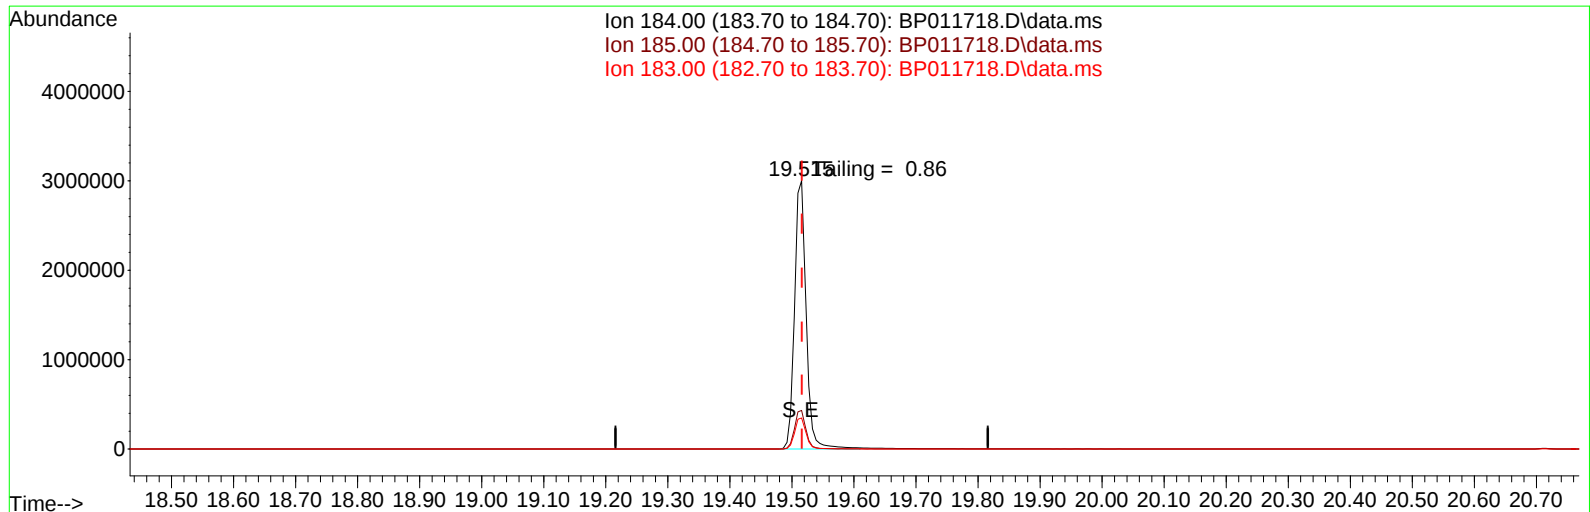

TIC: BP011718.D\data.ms

(77) Benzidine

19.515min (-0.000) 50973.74 ng

response 3962823

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.36
183.00	11.30	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/15/2022	BNA_P	<u>BP011718.D</u>
Compound Name	Response	Retention Time
DDT	1749886	20.715
DDD	16302	20.28
DDE	1039	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17341	1767227	0.98

Instrument :
BNA_P
ClientSampleId :
DFTPP