
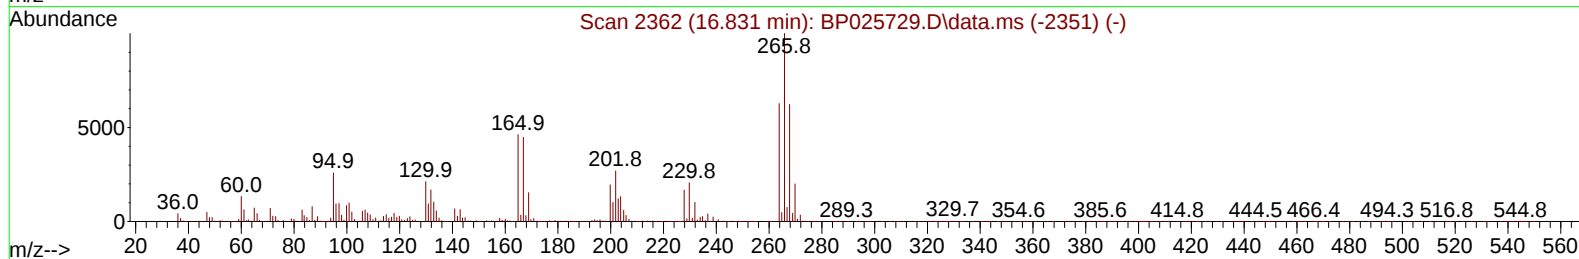
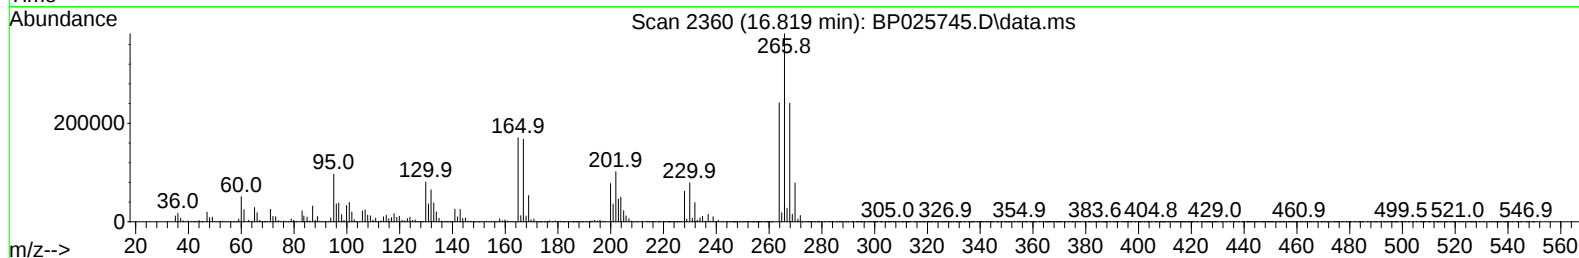


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091525\
Data File : BP025745.D
Acq On : 15 Sep 2025 09:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 12:29:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

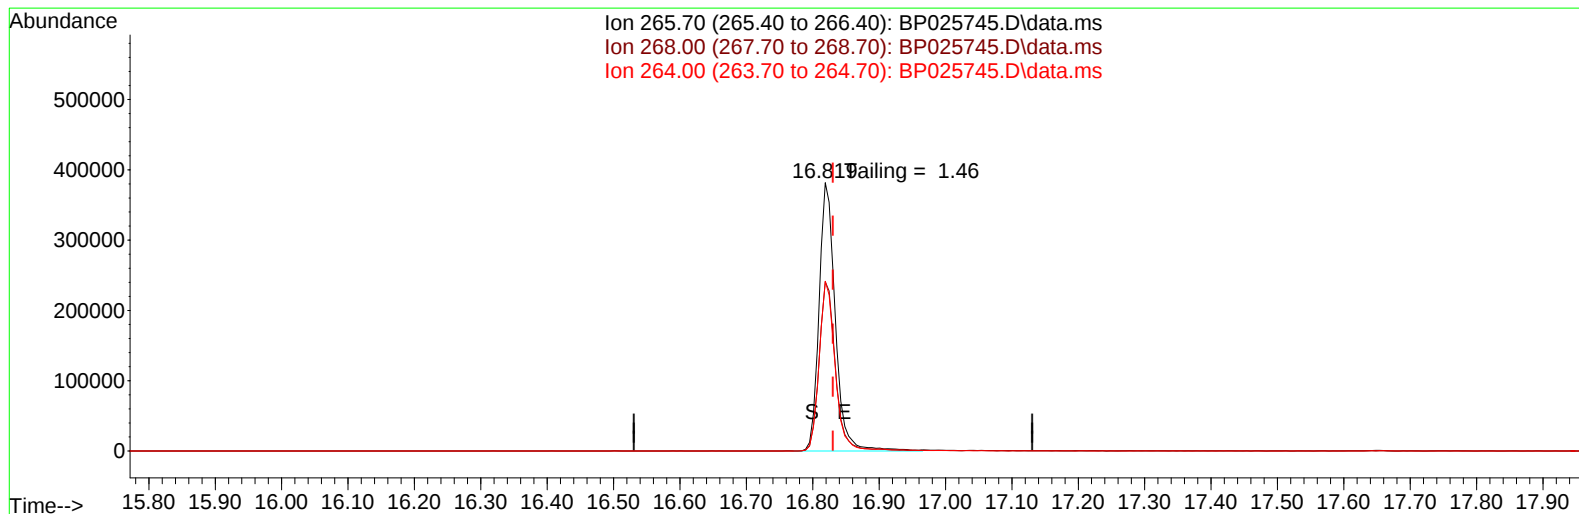

TIC: BP025745.D\data.ms

(70) Pentachlorophenol (C)




16.819min (-0.012) 162860.51 ng

response 649202

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.09
264.00	62.70	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091525\
Data File : BP025745.D
Acq On : 15 Sep 2025 09:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 12:29:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

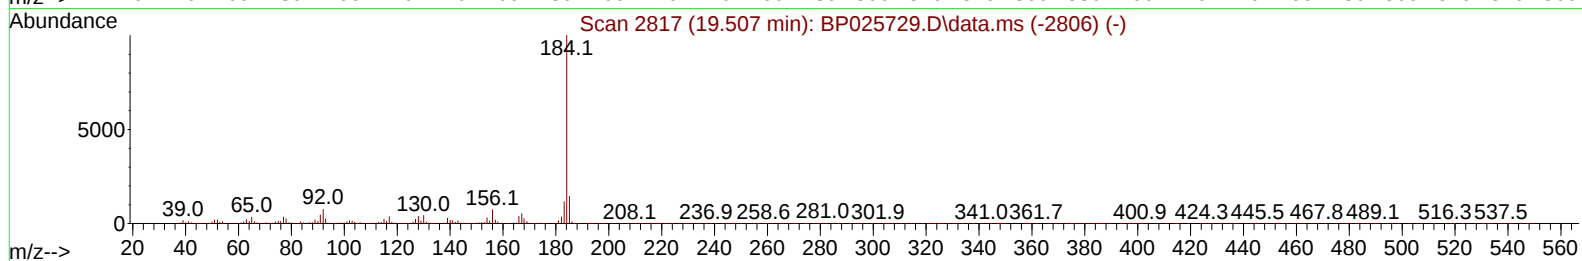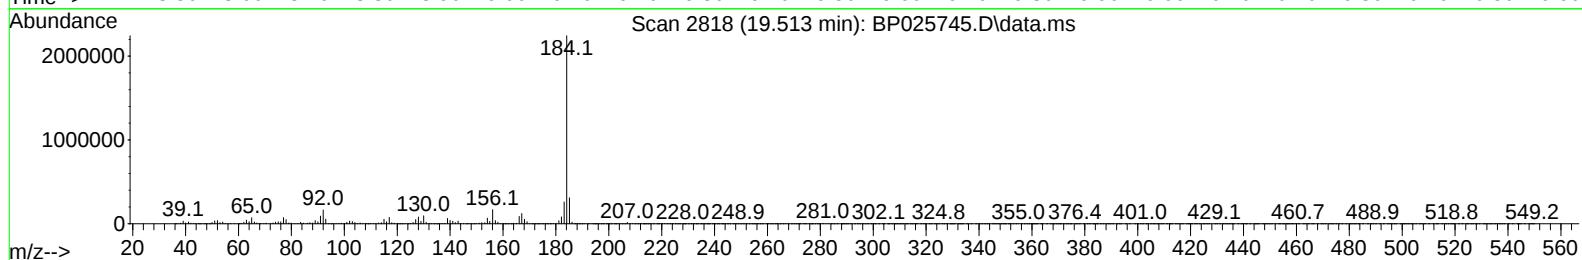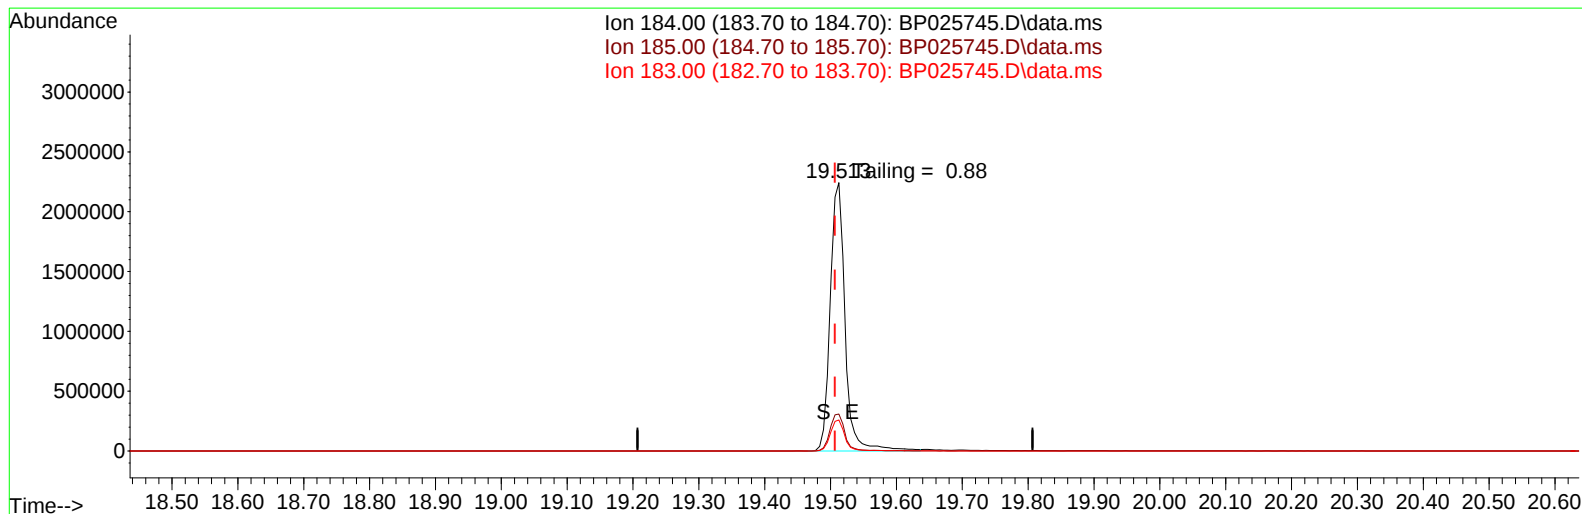

TIC: BP025745.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 1174.60 ng

response 3521053

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.77
183.00	11.50	11.57
0.00	0.00	0.00