


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091525\
Data File : BP025745.D
Acq On : 15 Sep 2025 09:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

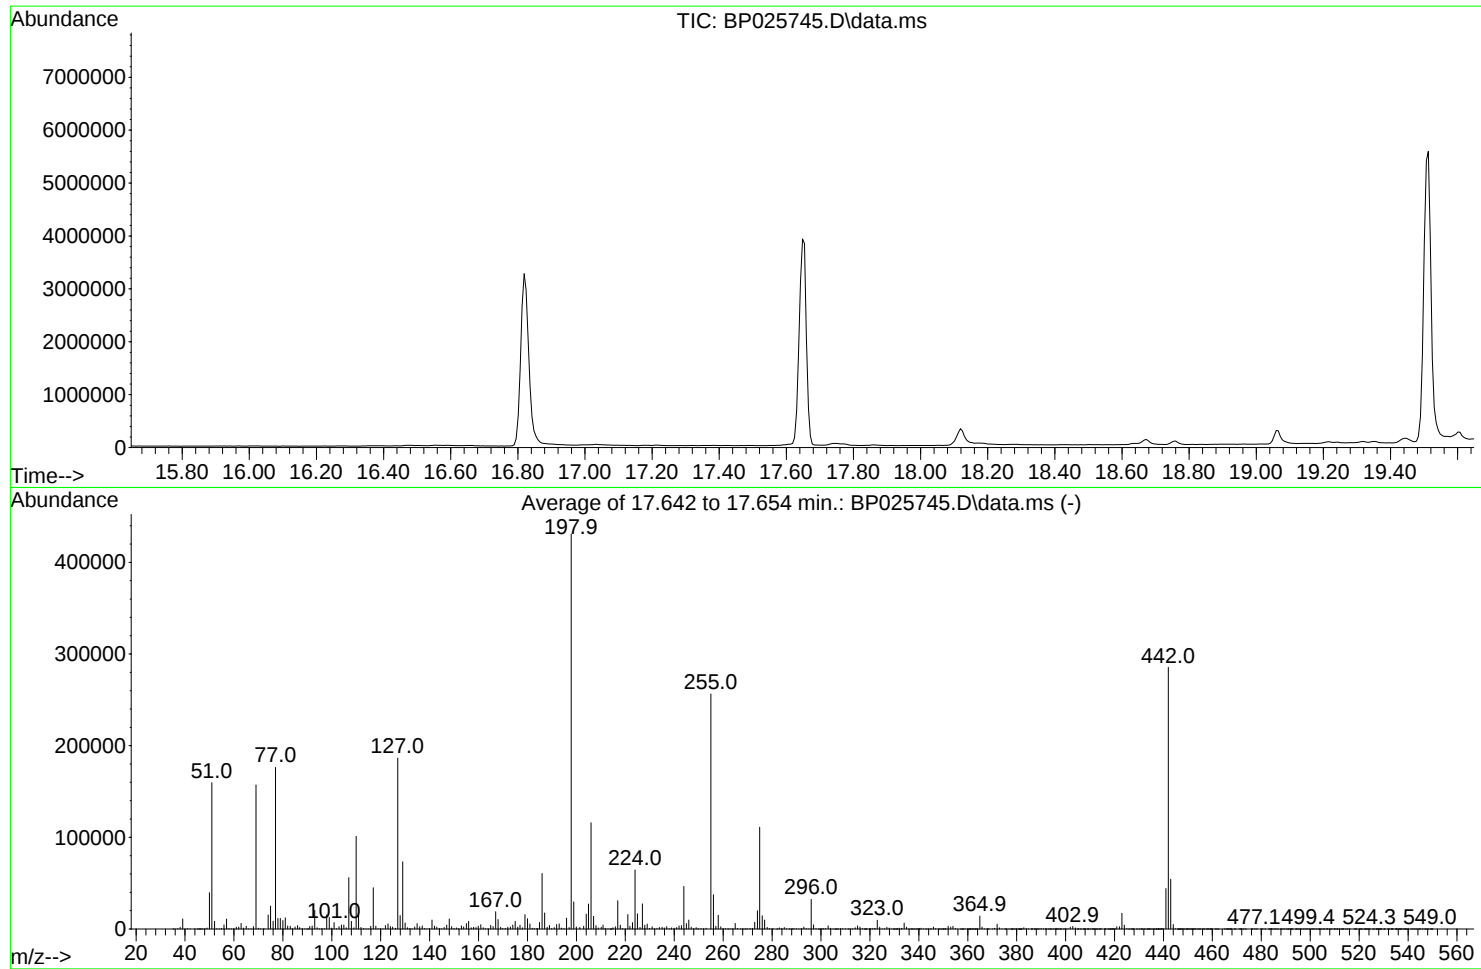

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2492

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2594	PASS
69	69	100	100	100.0	157118	PASS
70	69	0.00	2	0.5	844	PASS
197	198	0.00	2	0.4	1627	PASS
198	198	100	100	100.0	430779	PASS
199	198	5	9	6.9	29573	PASS
365	198	1	100	3.3	14228	PASS
441	443	0.01	150	81.2	44160	PASS
442	442	100	100	100.0	285418	PASS
443	442	15	24	19.0	54353	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/15/2025	BNA_P	<u>BP025745.D</u>
Compound Name	Response	Retention Time
DDT	188998	207995
DDD	26820	20.336
DDE	5032	19.813
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31852	220850	14.42

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091525\
Data File : BP025745.D
Acq On : 15 Sep 2025 09:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 15 12:29:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

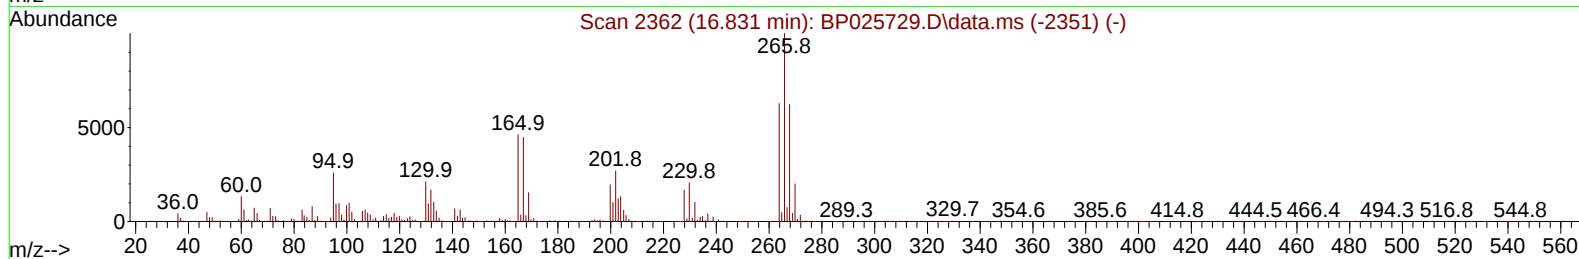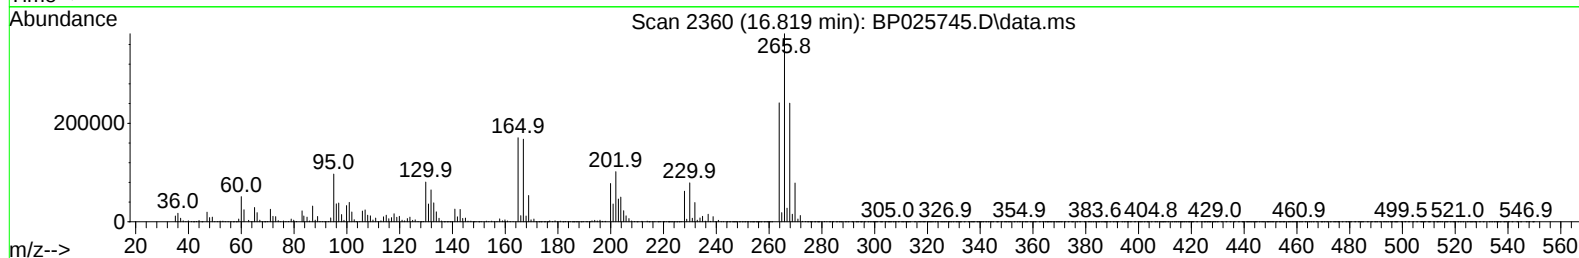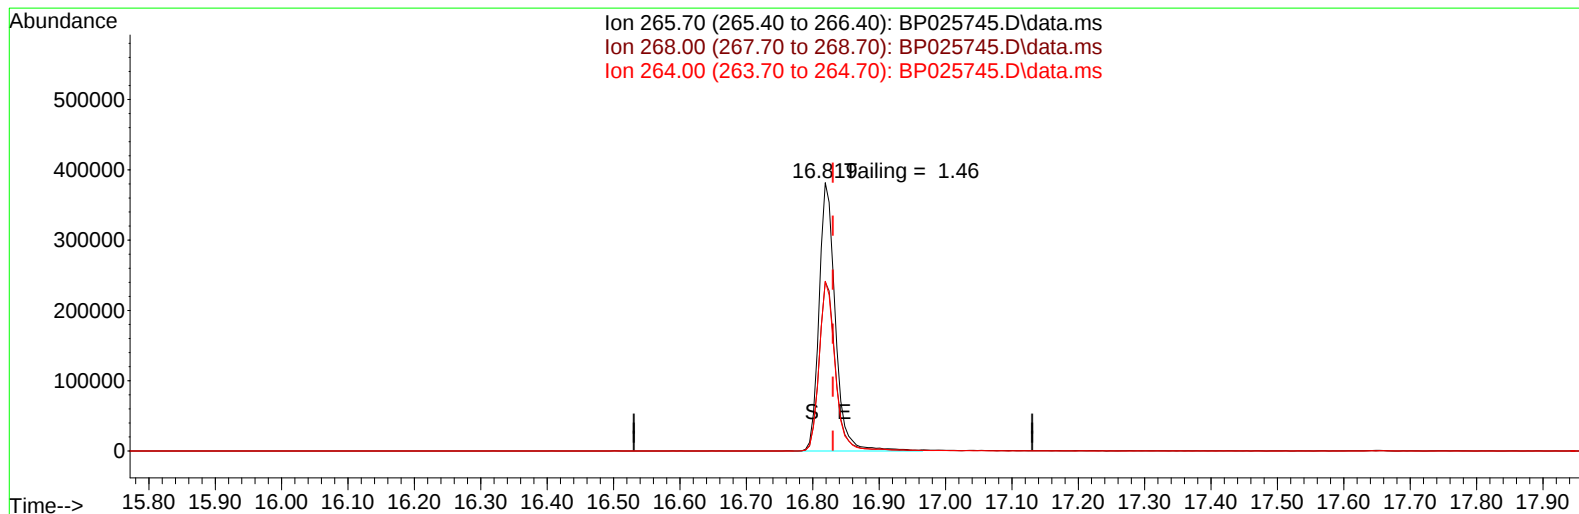

TIC: BP025745.D\data.ms

(70) Pentachlorophenol (C)

16.819min (-0.012) 162860.51 ng




response 649202

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.09
264.00	62.70	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091525\
Data File : BP025745.D
Acq On : 15 Sep 2025 09:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 15 12:29:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

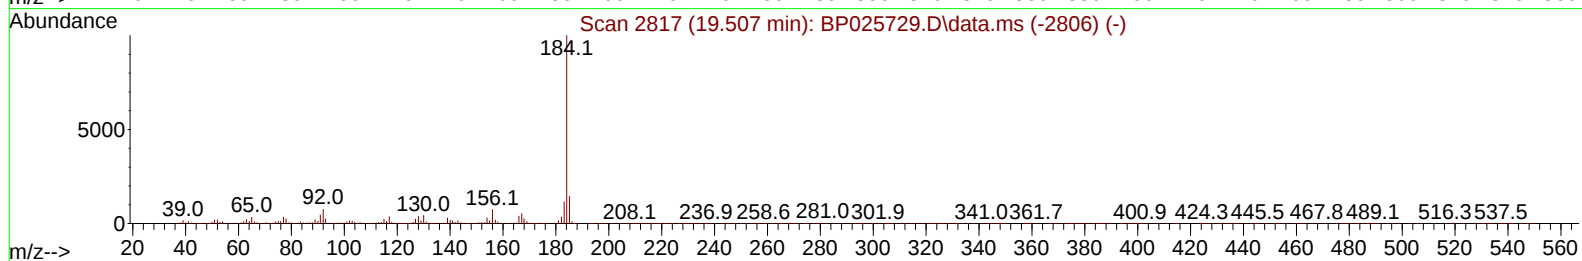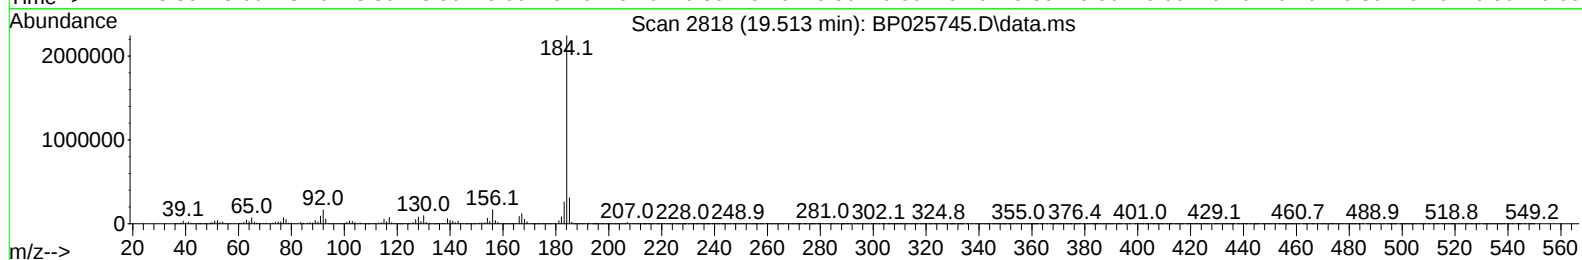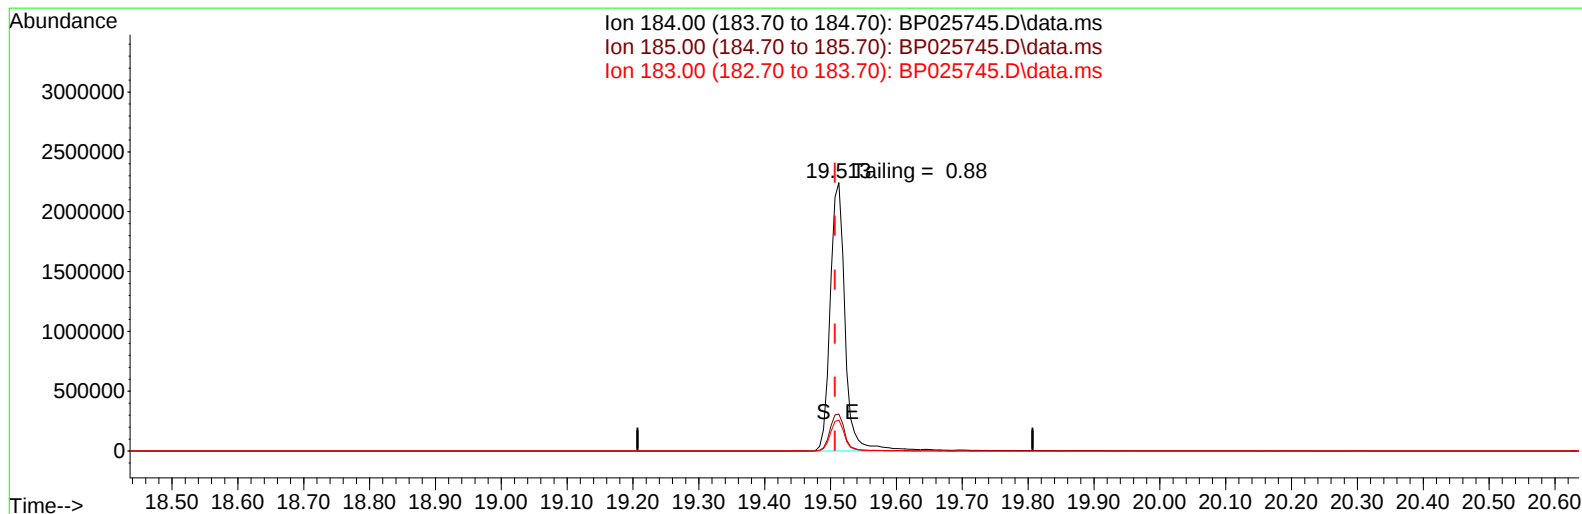

TIC: BP025745.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 1174.60 ng

response 3521053

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.77
183.00	11.50	11.57
0.00	0.00	0.00