
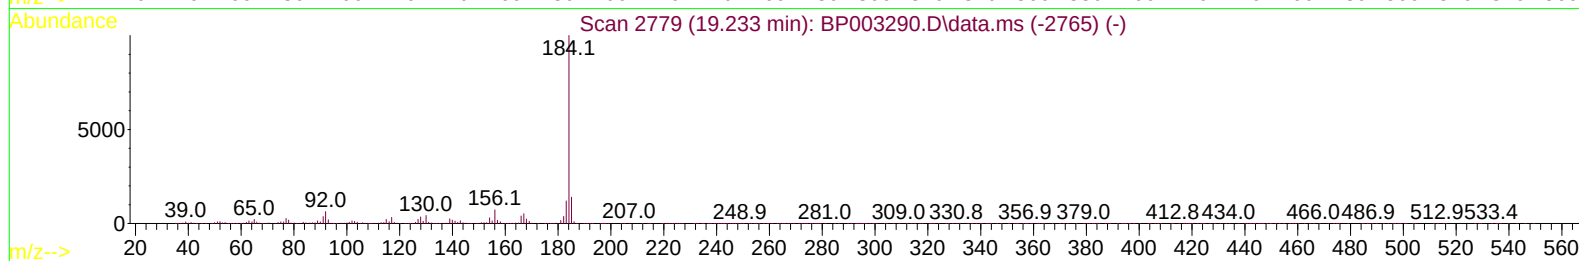
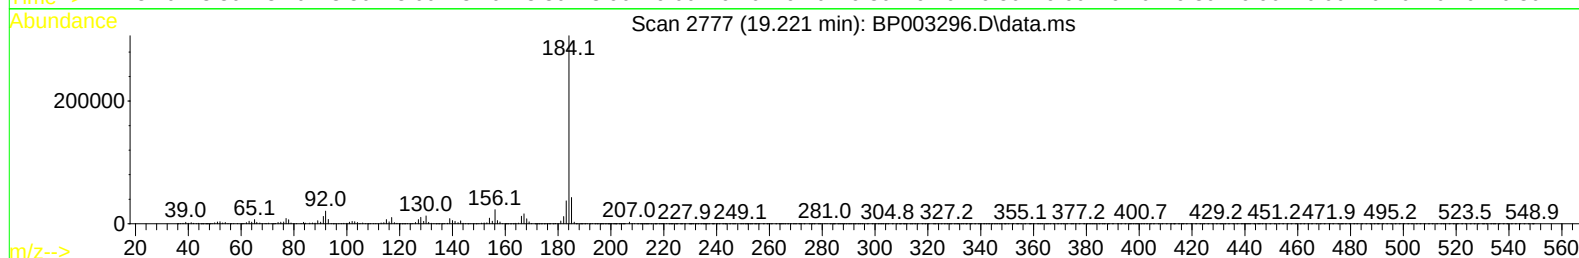


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091620\
 Data File : BP003296.D
 Acq On : 16 Sep 2020 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 16:51:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 16 13:18:39 2020
 Response via : Initial Calibration

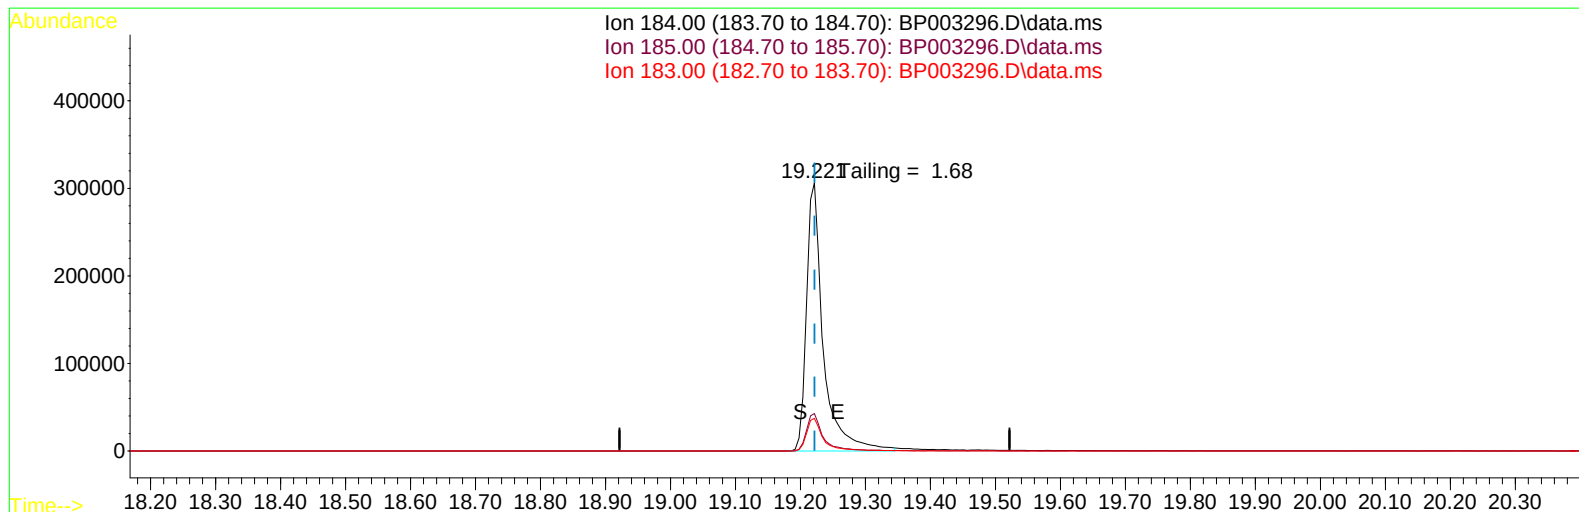




TIC: BP003296.D\data.ms

(77) Benzidine**19.221min (-0.000) 514066.73 ng****response 557921**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	12.00	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091620\
Data File : BP003296.D
Acq On : 16 Sep 2020 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 16:51:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 16 13:18:39 2020
Response via : Initial Calibration

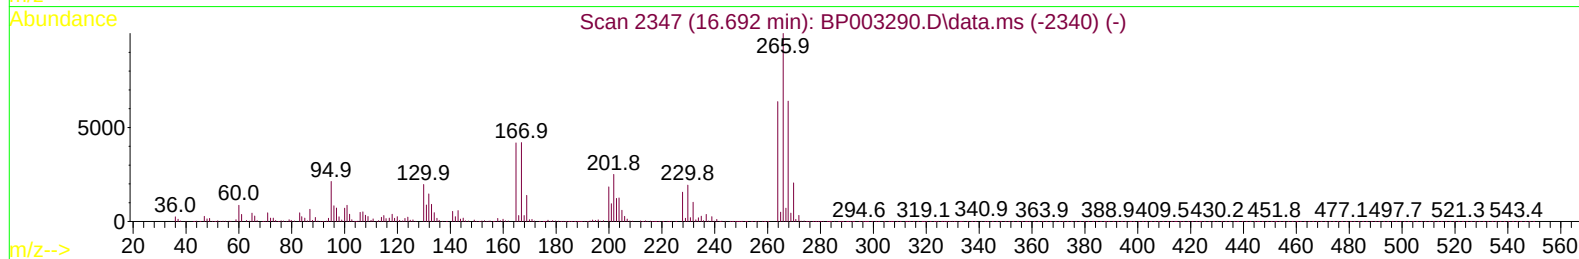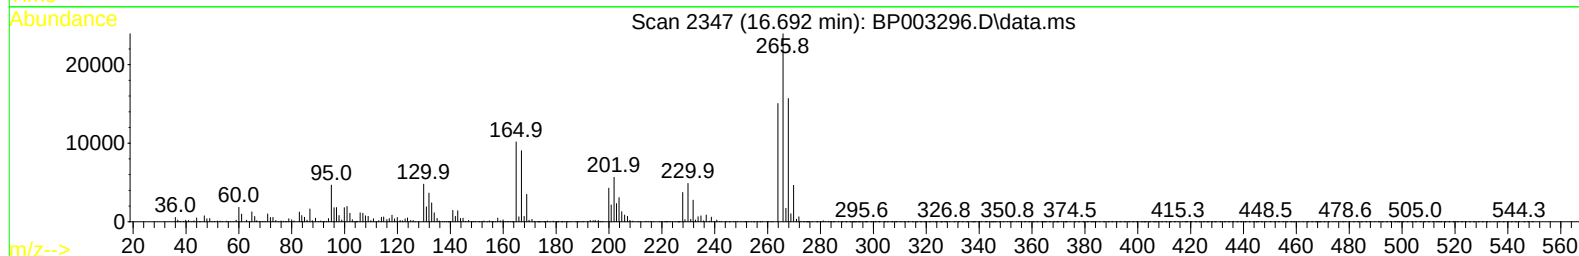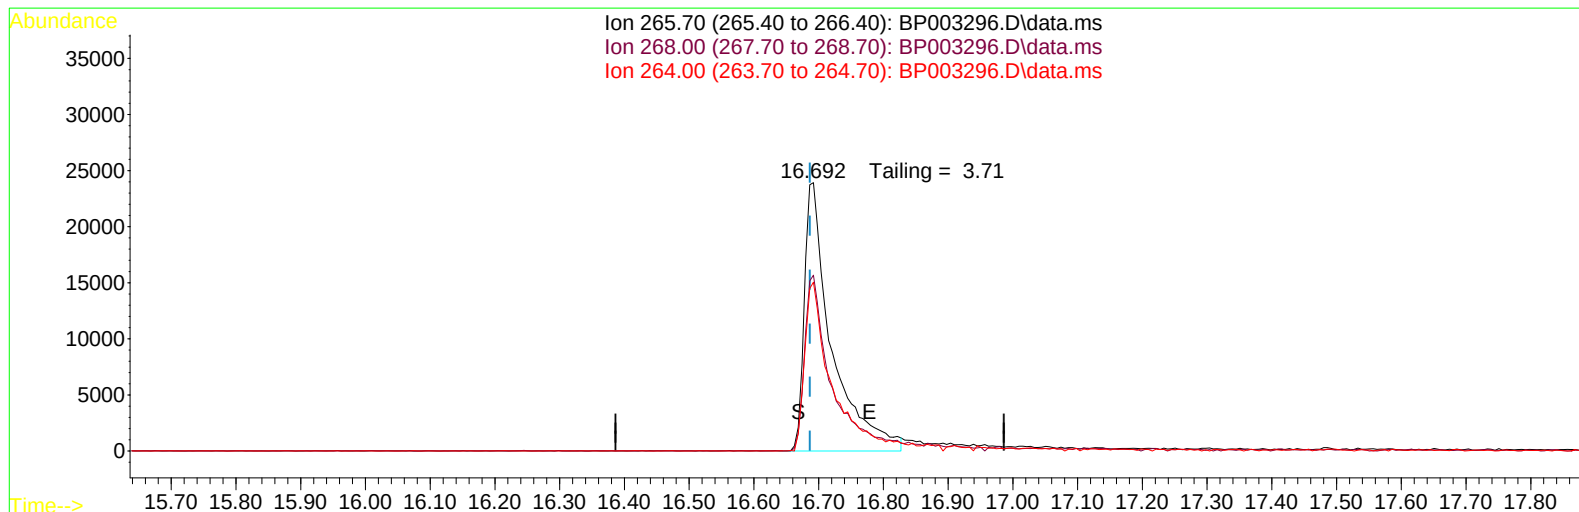

TIC: BP003296.D\data.ms

(70) Pentachlorophenol (C)

16.692min (+ 0.006) 2148506.60 ng

response 72338

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.53
264.00	63.30	62.88
0.00	0.00	0.00