
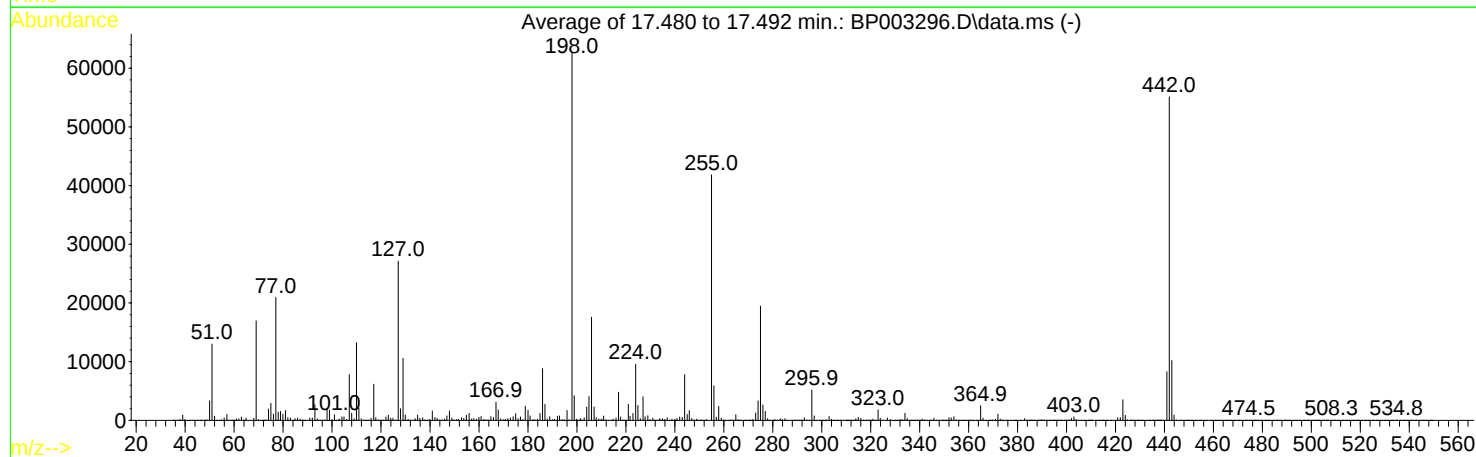


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091620\
 Data File : BP003296.D
 Acq On : 16 Sep 2020 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 16 13:18:39 2020

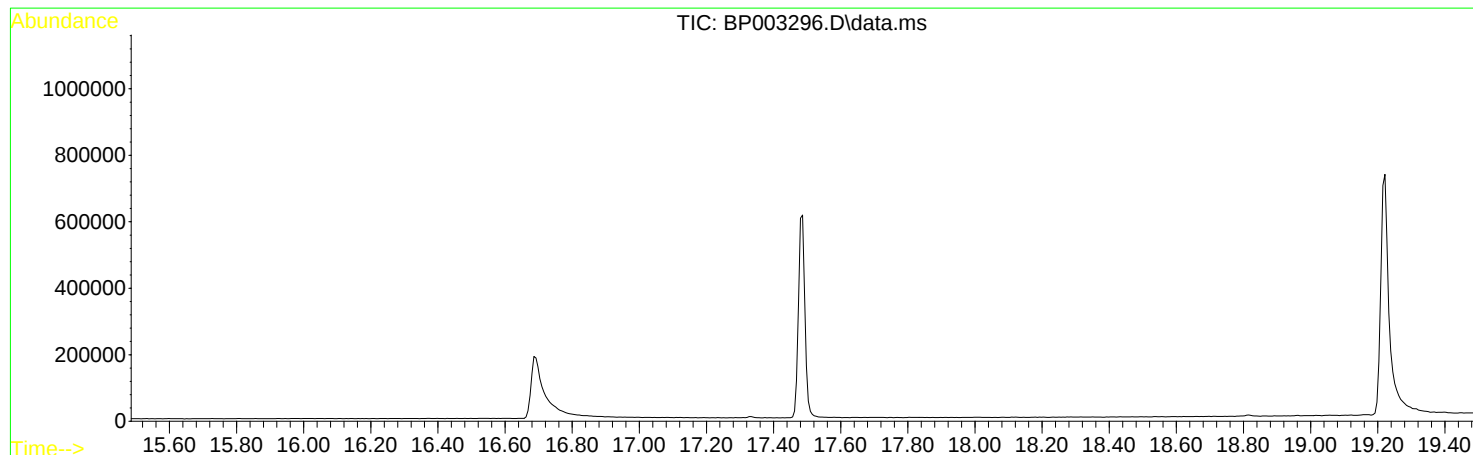

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.8	13015	PASS
68	69	0.00	2	2.0	339	PASS
69	198	0.00	100	27.1	16969	PASS
70	69	0.00	2	0.8	132	PASS
127	198	10	80	43.3	27119	PASS
197	198	0.00	2	0.2	114	PASS
198	198	100	100	100.0	62672	PASS
199	198	5	9	6.7	4206	PASS
275	198	10	60	31.1	19478	PASS
365	198	1	100	3.9	2470	PASS
441	198	0.01	100	13.2	8279	PASS
442	198	50	100	87.9	55112	PASS
443	442	15	24	18.5	10191	PASS