
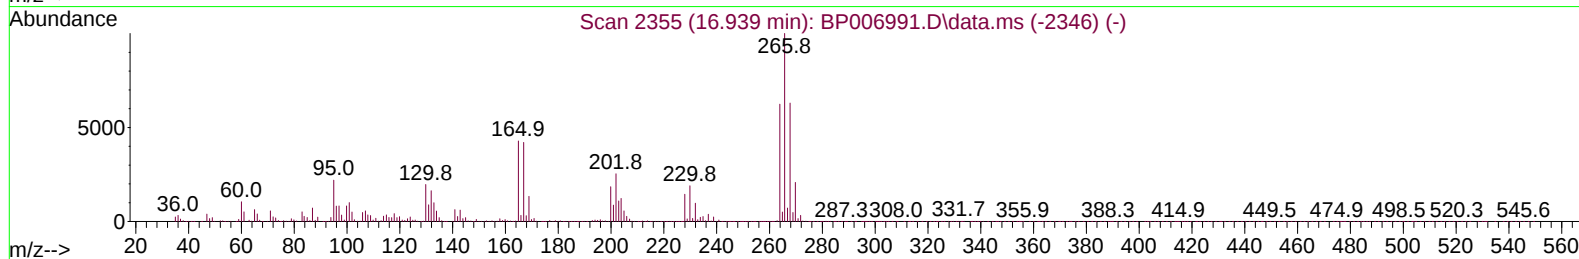
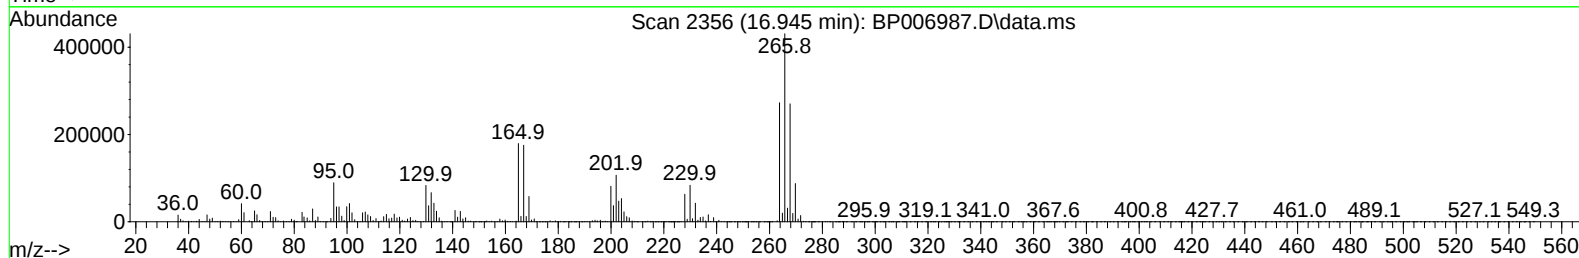


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
 Data File : BP006987.D
 Acq On : 16 Sep 2021 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 15:21:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 16 15:16:52 2021
 Response via : Initial Calibration

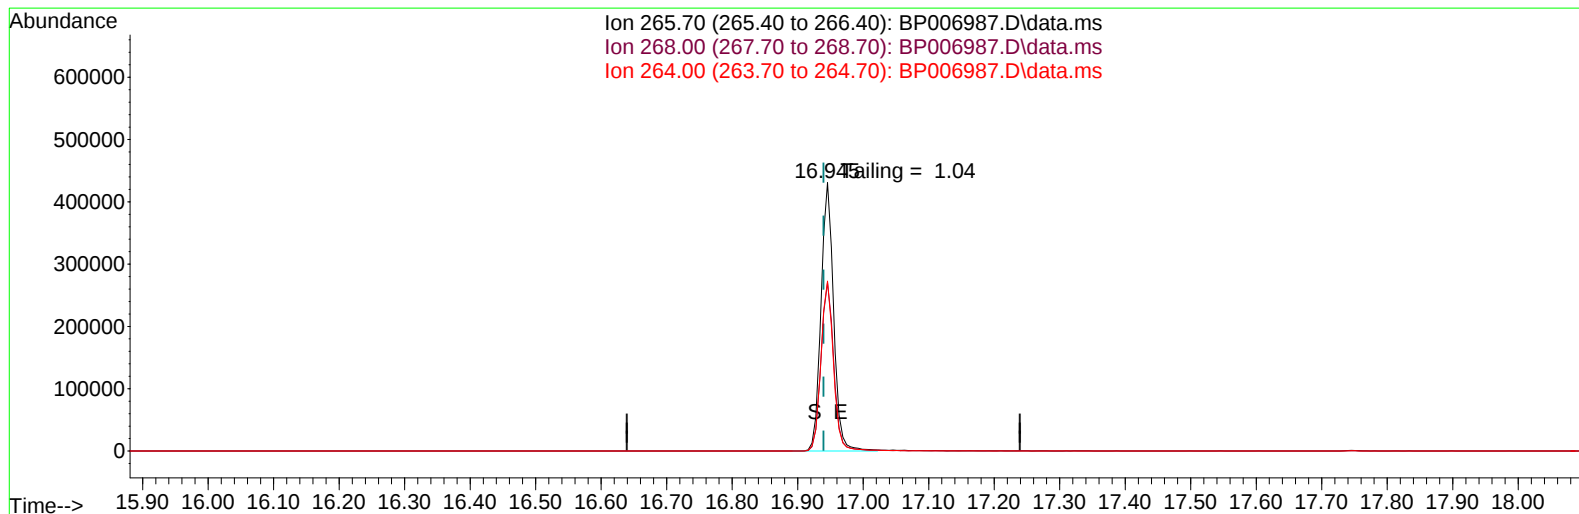




TIC: BP006987.D\data.ms

(70) Pentachlorophenol (C)**16.945min (+ 0.006) 1182205.43 ng****response 582301**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.76
264.00	62.90	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
 Data File : BP006987.D
 Acq On : 16 Sep 2021 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 15:21:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 16 15:16:52 2021
 Response via : Initial Calibration

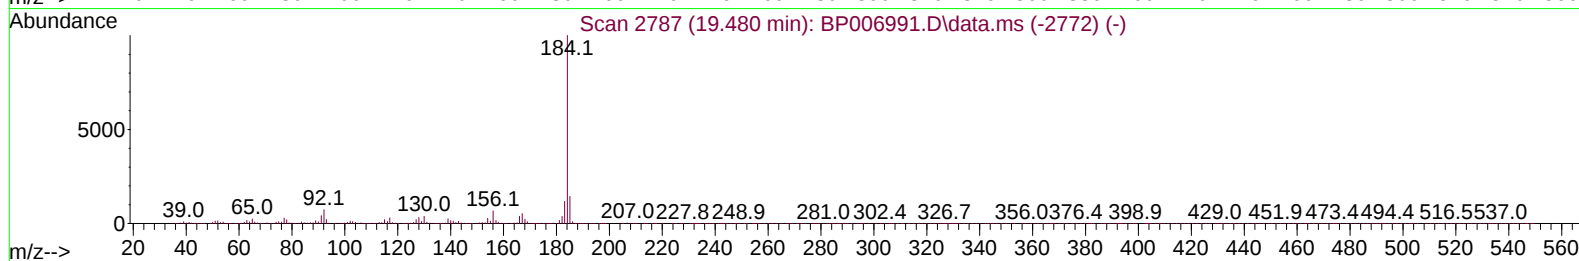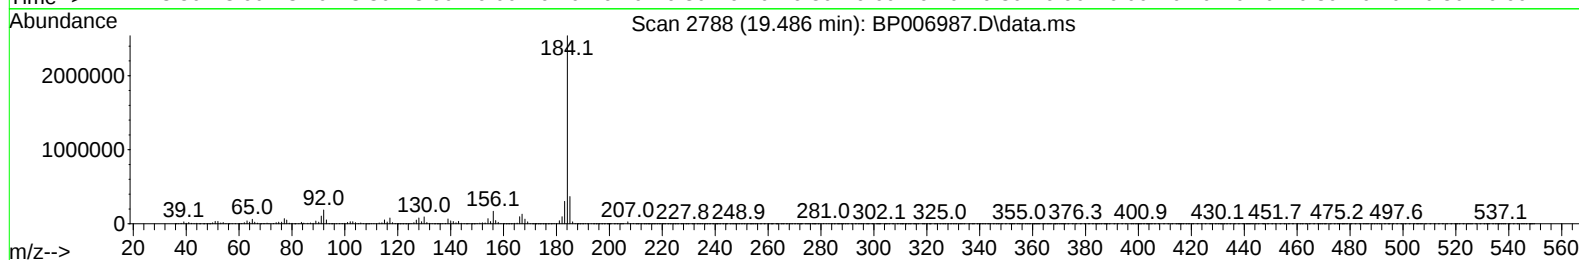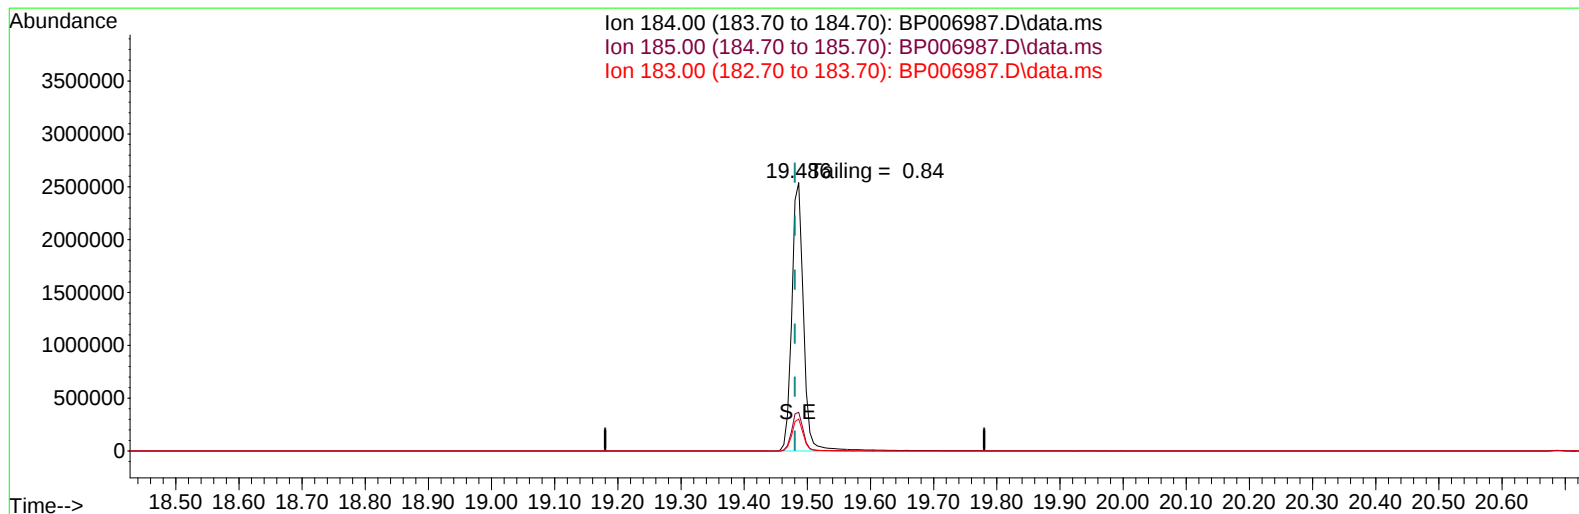

TIC: BP006987.D\data.ms

(77) Benzidine**19.486min (+ 0.006) -20.00 ng****response 3294981**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.46
183.00	11.90	11.94
0.00	0.00	0.00