
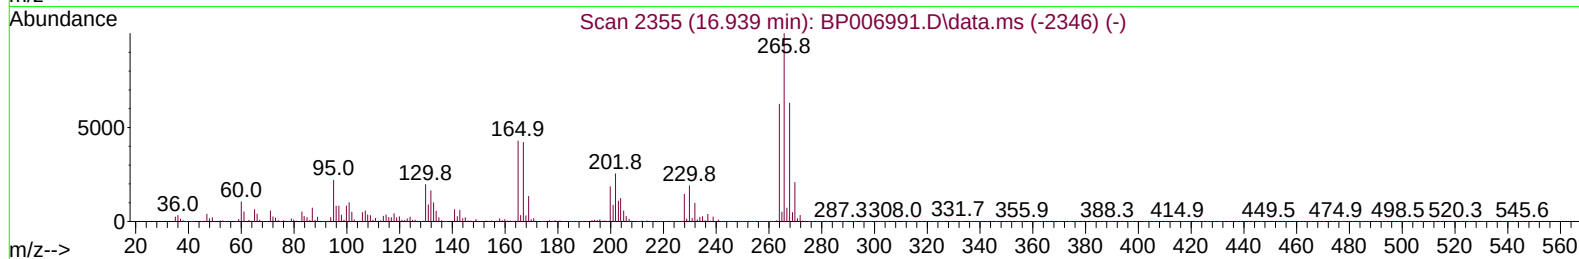
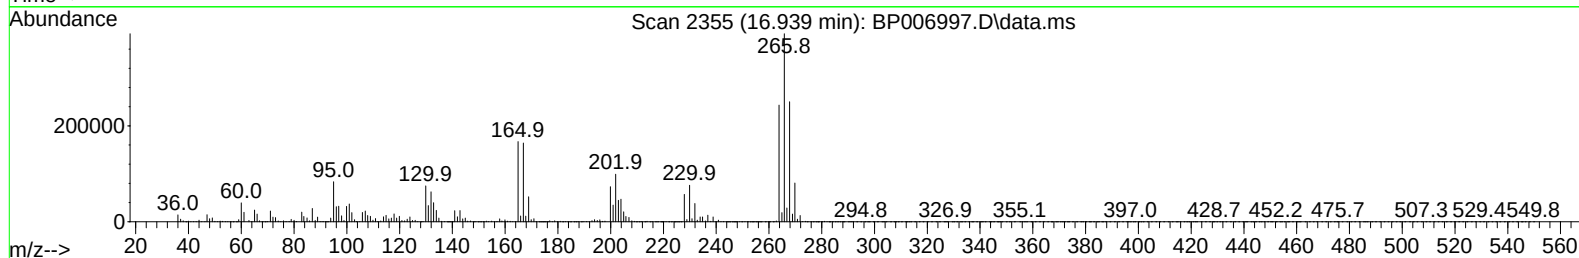


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
Data File : BP006997.D
Acq On : 16 Sep 2021 16:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 16:58:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 16 15:16:52 2021
Response via : Initial Calibration

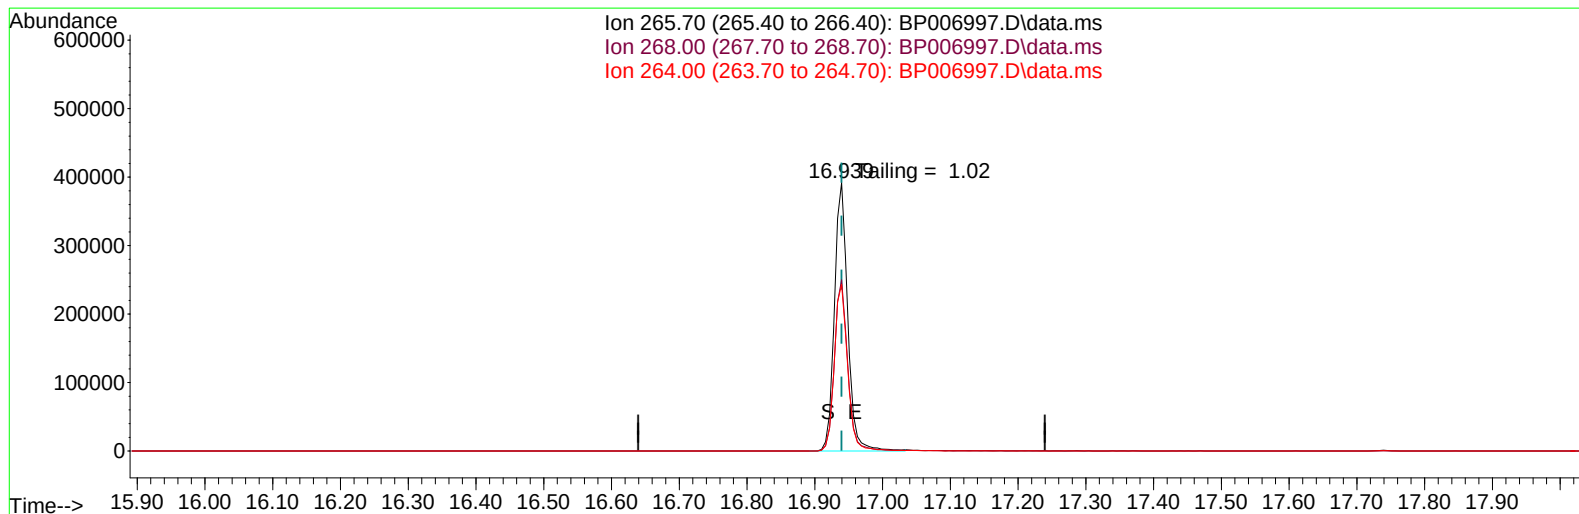

TIC: BP006997.D\data.ms

(70) Pentachlorophenol (C)




16.939min (-0.000) 72194.56 ng

response 537707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.82
264.00	62.90	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
 Data File : BP006997.D
 Acq On : 16 Sep 2021 16:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 16:58:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 16 15:16:52 2021
 Response via : Initial Calibration

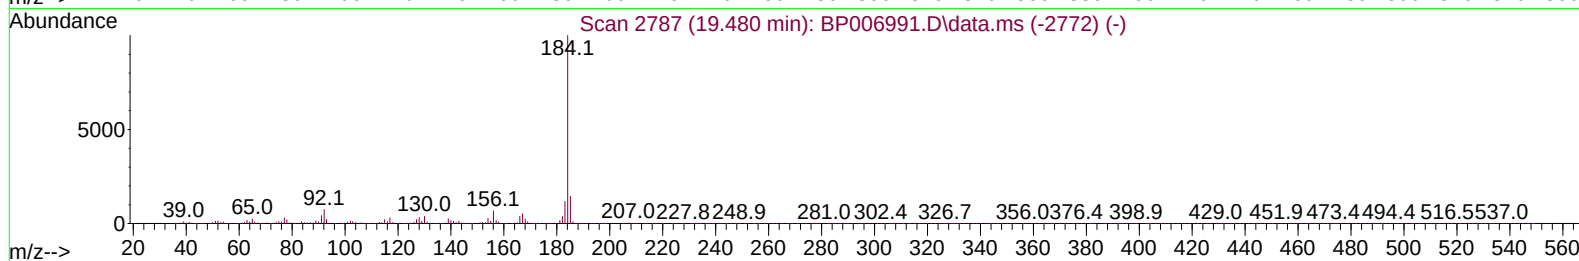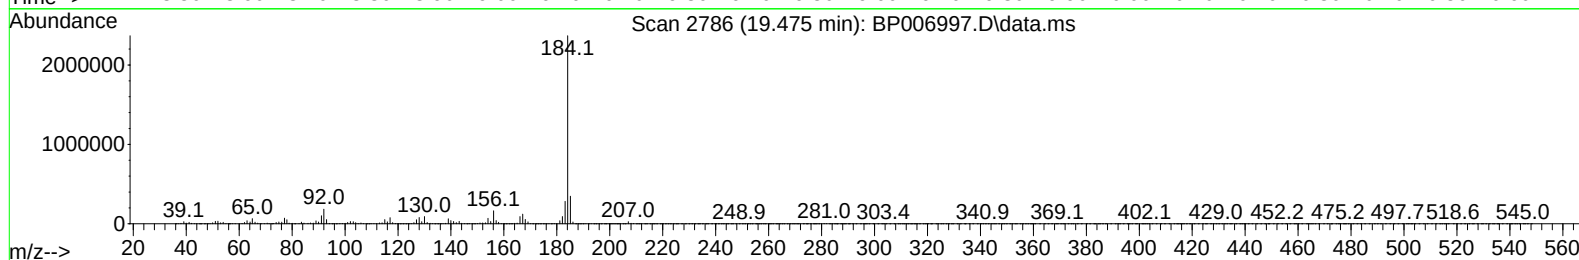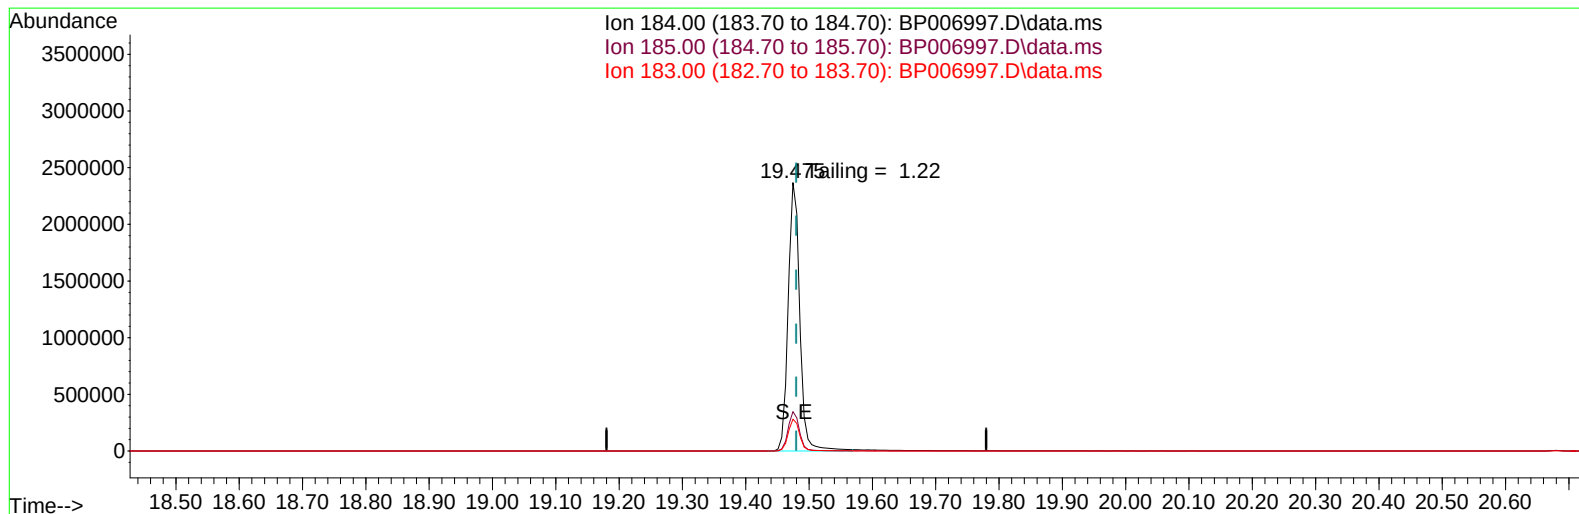

TIC: BP006997.D\data.ms

(77) Benzidine**19.475min (-0.005) -20.00 ng****response 3060901**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.68
183.00	11.90	11.88
0.00	0.00	0.00