
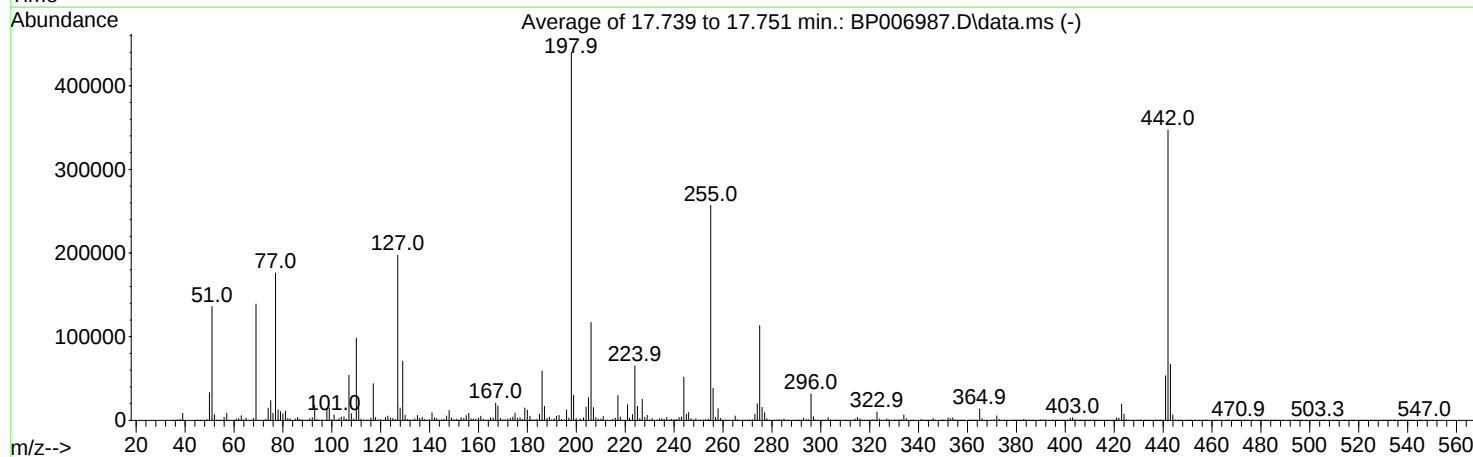


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
 Data File : BP006987.D
 Acq On : 16 Sep 2021 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 16 15:16:52 2021

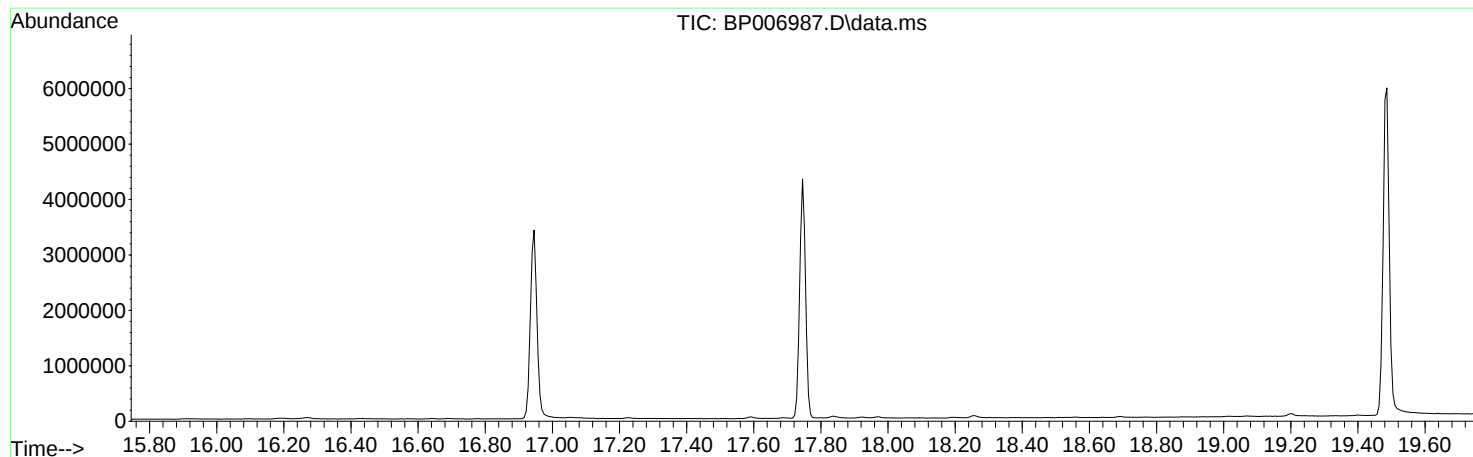

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	136016	PASS
68	69	0.00	2	1.6	2265	PASS
69	198	0.00	100	31.6	138804	PASS
70	69	0.00	2	0.2	233	PASS
127	198	10	80	44.9	197467	PASS
197	198	0.00	2	0.7	2899	PASS
198	198	100	100	100.0	439746	PASS
199	198	5	9	6.8	30046	PASS
275	198	10	60	25.7	113184	PASS
365	198	1	100	3.1	13540	PASS
441	198	0.01	100	12.1	53160	PASS
442	442	100	100	100.0	347243	PASS
443	442	15	24	19.3	66912	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/16/2021	BNA_P	<u>BP006987.D</u>
Compound Name	Response	Retention Time
DDT	1548814	20.69
DDD	3425	20.31
DDE	1567	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4992	1553806	0.32

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
Data File : BP006987.D
Acq On : 16 Sep 2021 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 15:21:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 16 15:16:52 2021
Response via : Initial Calibration

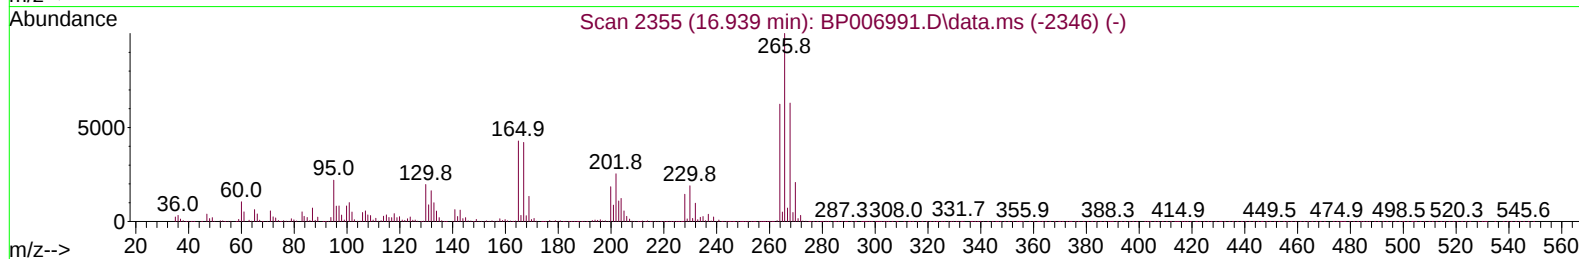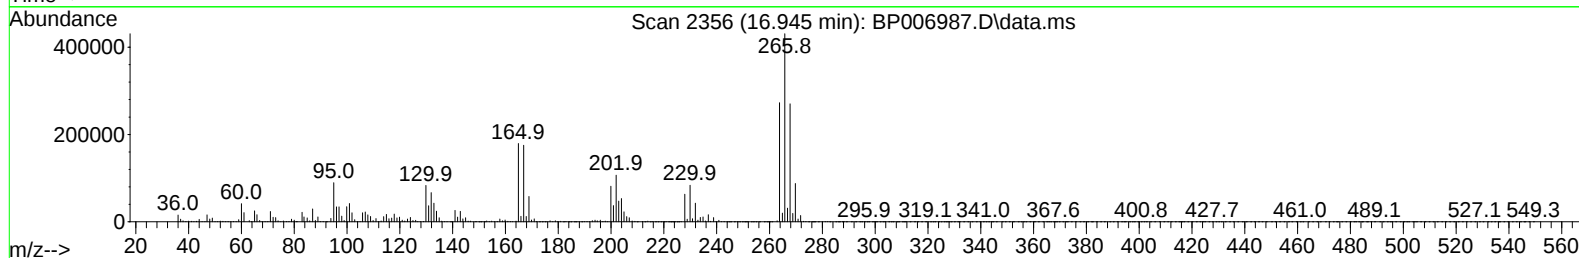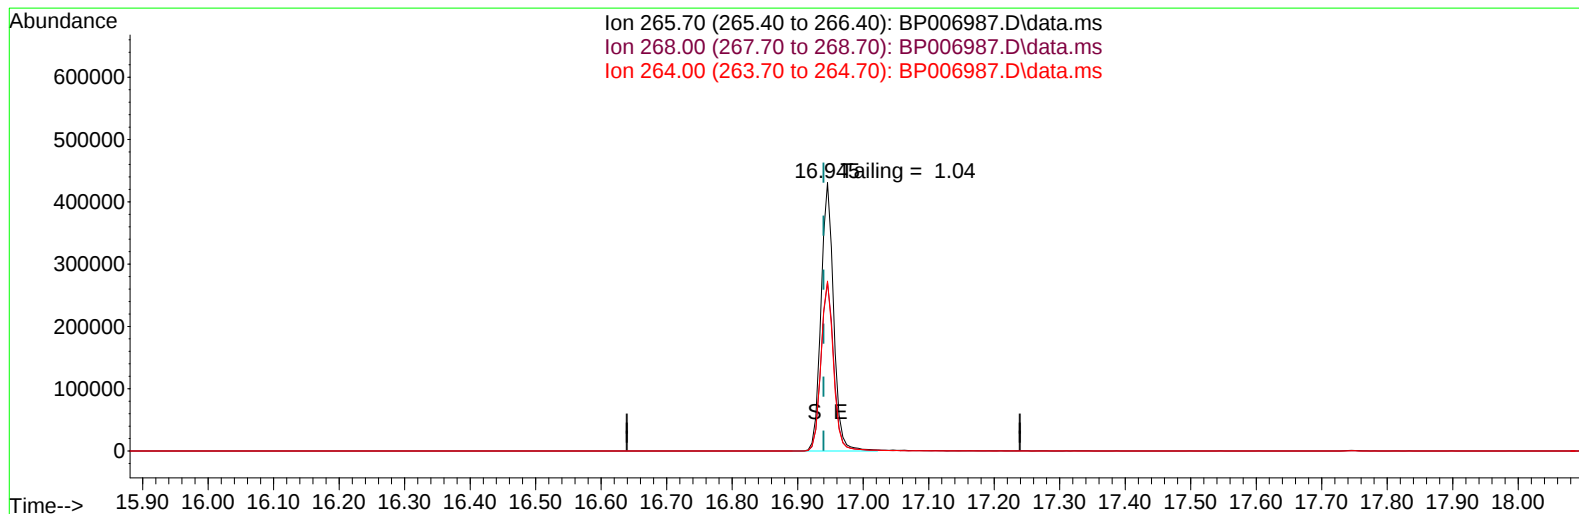

TIC: BP006987.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.006) 1182205.43 ng




response 582301

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.76
264.00	62.90	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
 Data File : BP006987.D
 Acq On : 16 Sep 2021 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 16 15:21:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 16 15:16:52 2021
 Response via : Initial Calibration

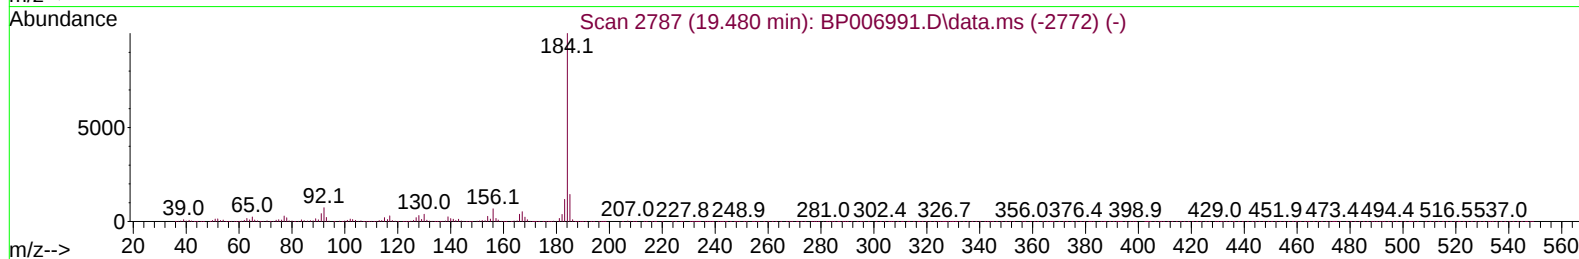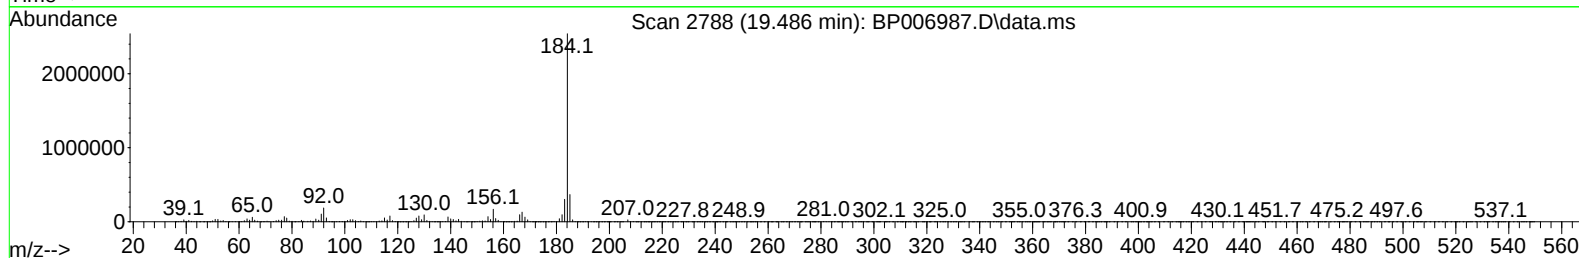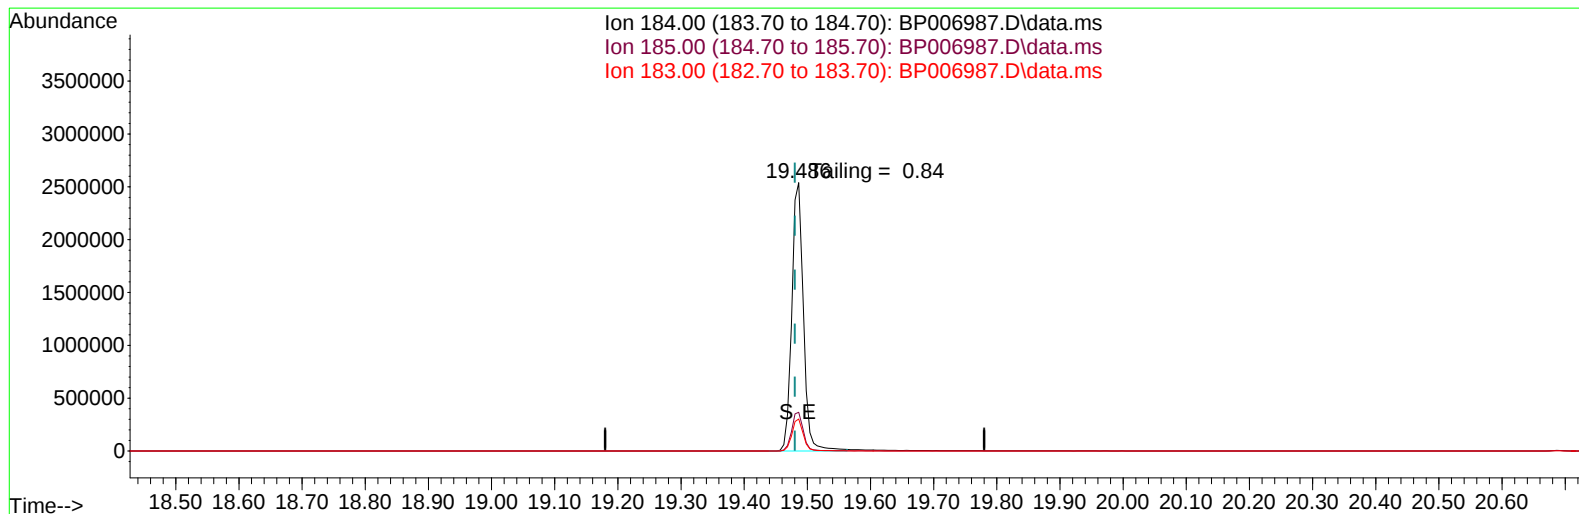

TIC: BP006987.D\data.ms

(77) Benzidine

19.486min (+ 0.006) -20.00 ng

response 3294981

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.46
183.00	11.90	11.94
0.00	0.00	0.00