
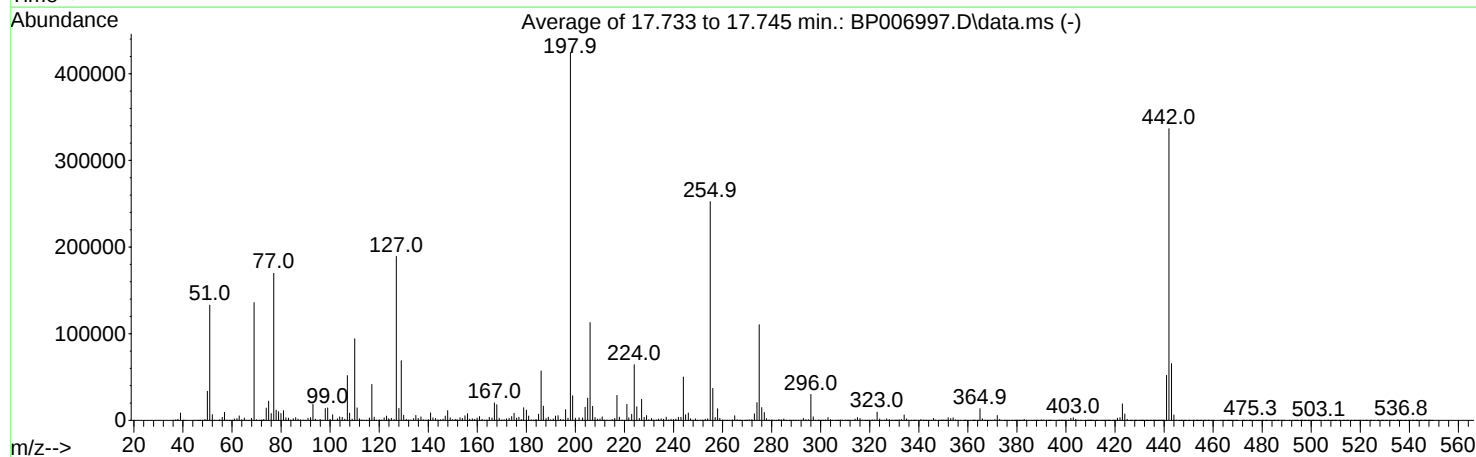


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
 Data File : BP006997.D
 Acq On : 16 Sep 2021 16:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 16 15:16:52 2021

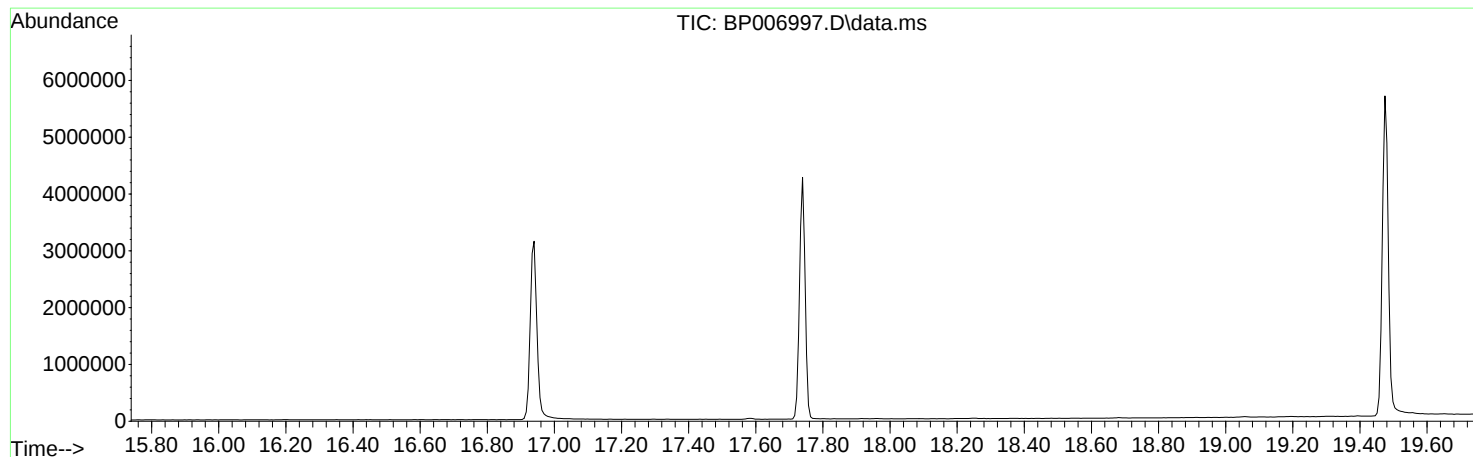

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	132992	PASS
68	69	0.00	2	1.8	2412	PASS
69	198	0.00	100	32.0	135841	PASS
70	69	0.00	2	0.5	673	PASS
127	198	10	80	44.6	189245	PASS
197	198	0.00	2	0.6	2617	PASS
198	198	100	100	100.0	424558	PASS
199	198	5	9	6.7	28373	PASS
275	198	10	60	26.0	110512	PASS
365	198	1	100	3.2	13465	PASS
441	198	0.01	100	12.3	52072	PASS
442	442	100	100	100.0	336576	PASS
443	442	15	24	19.5	65582	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/16/2021	BNA_P	<u>BP006997.D</u>
Compound Name	Response	Retention Time
DDT	1469573	20.68
DDD	4281	20.25
DDE	1807	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6088	1475661	0.41

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
Data File : BP006997.D
Acq On : 16 Sep 2021 16:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 16:58:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 16 15:16:52 2021
Response via : Initial Calibration

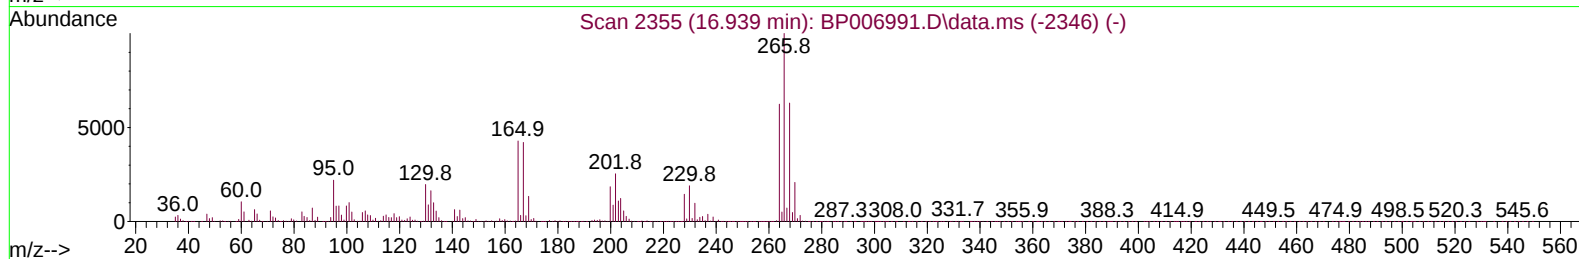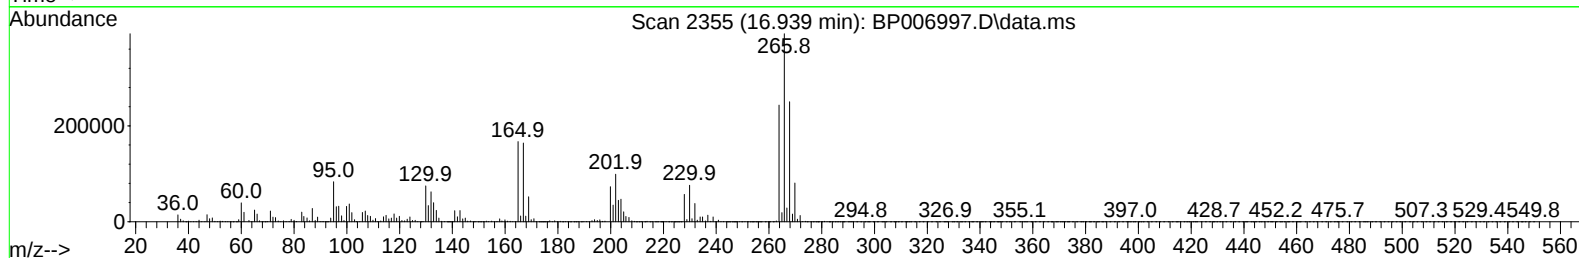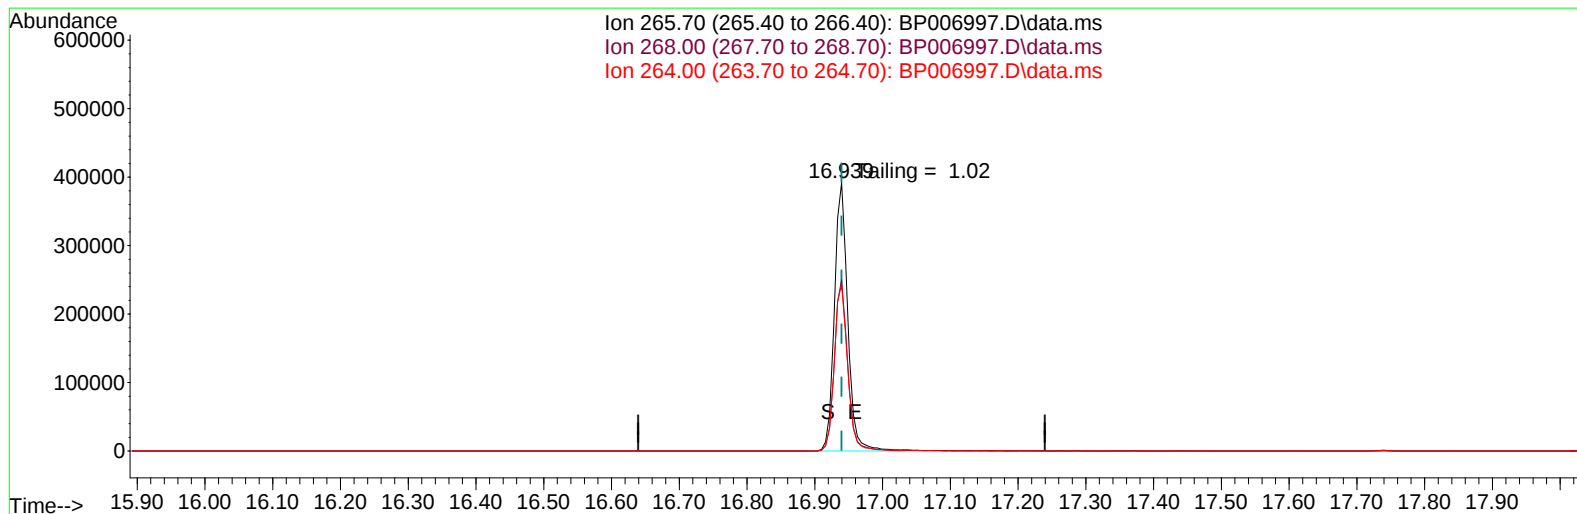

TIC: BP006997.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.000) 72194.56 ng




response 537707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.82
264.00	62.90	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091621\
 Data File : BP006997.D
 Acq On : 16 Sep 2021 16:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 16 16:58:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 16 15:16:52 2021
 Response via : Initial Calibration

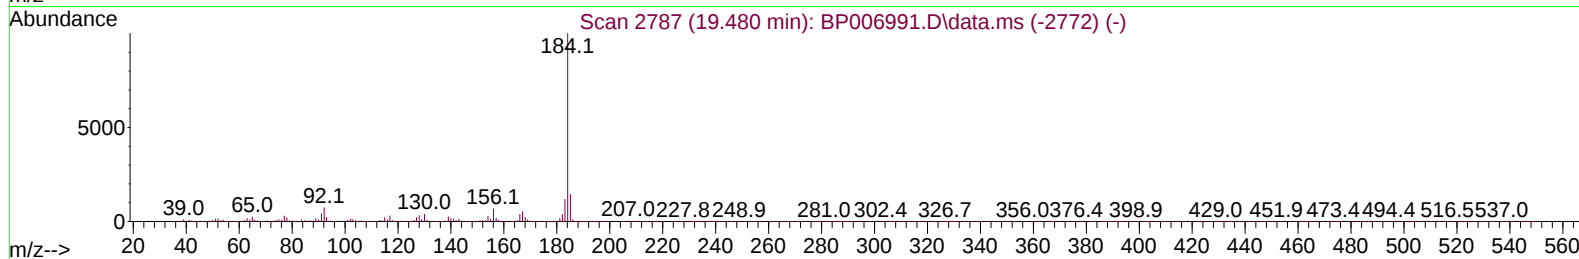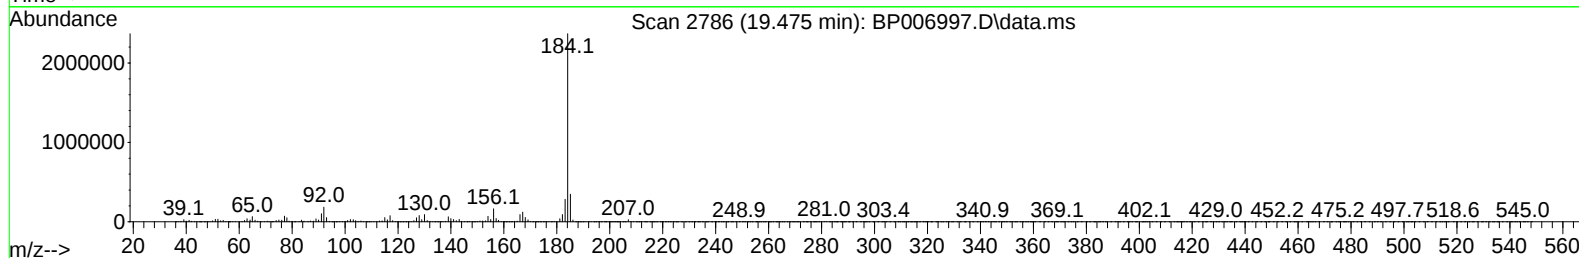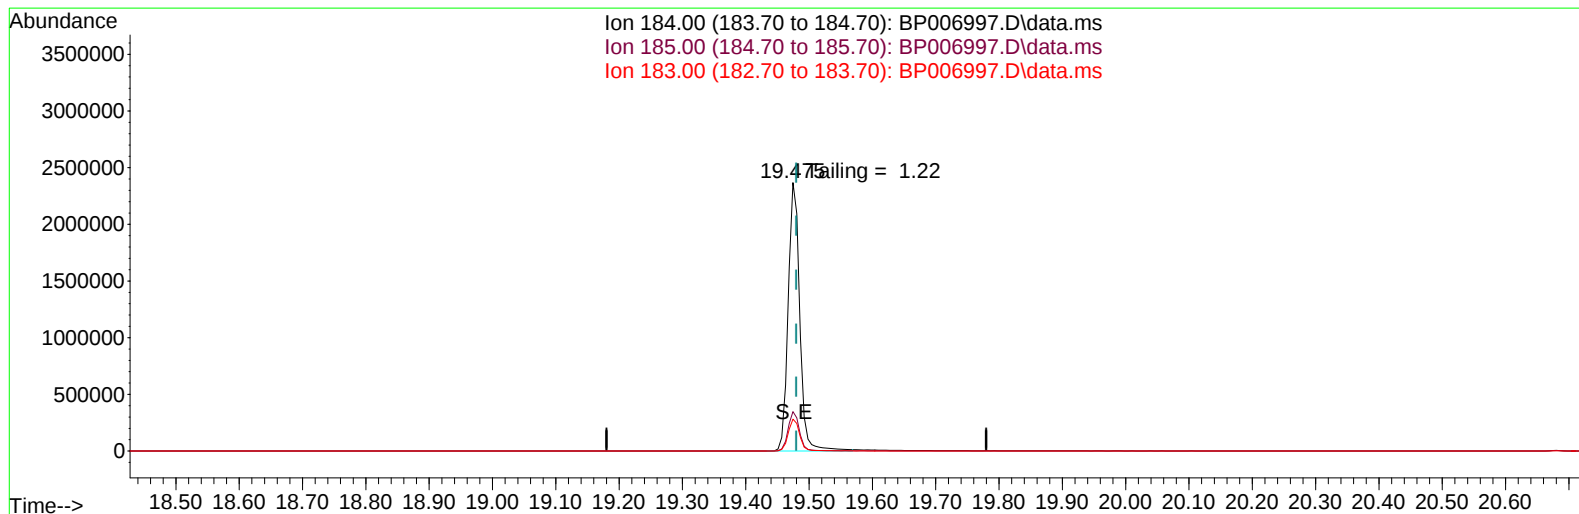

TIC: BP006997.D\data.ms

(77) Benzidine

19.475min (-0.005) -20.00 ng

response 3060901

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.68
183.00	11.90	11.88
0.00	0.00	0.00