
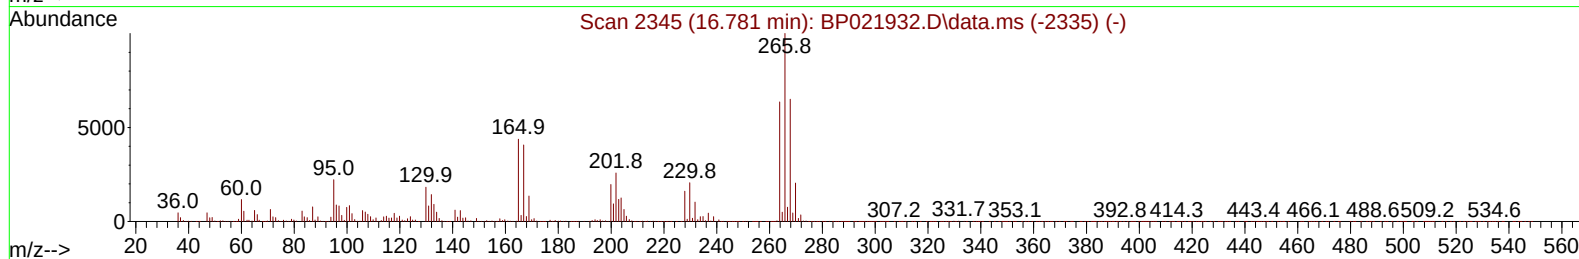
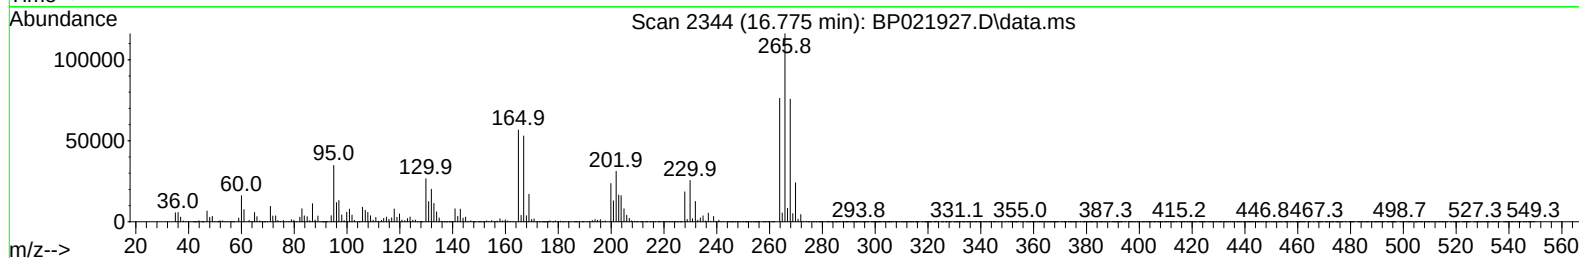


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091624\
Data File : BP021927.D
Acq On : 16 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 16:49:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 16 16:26:06 2024
Response via : Initial Calibration

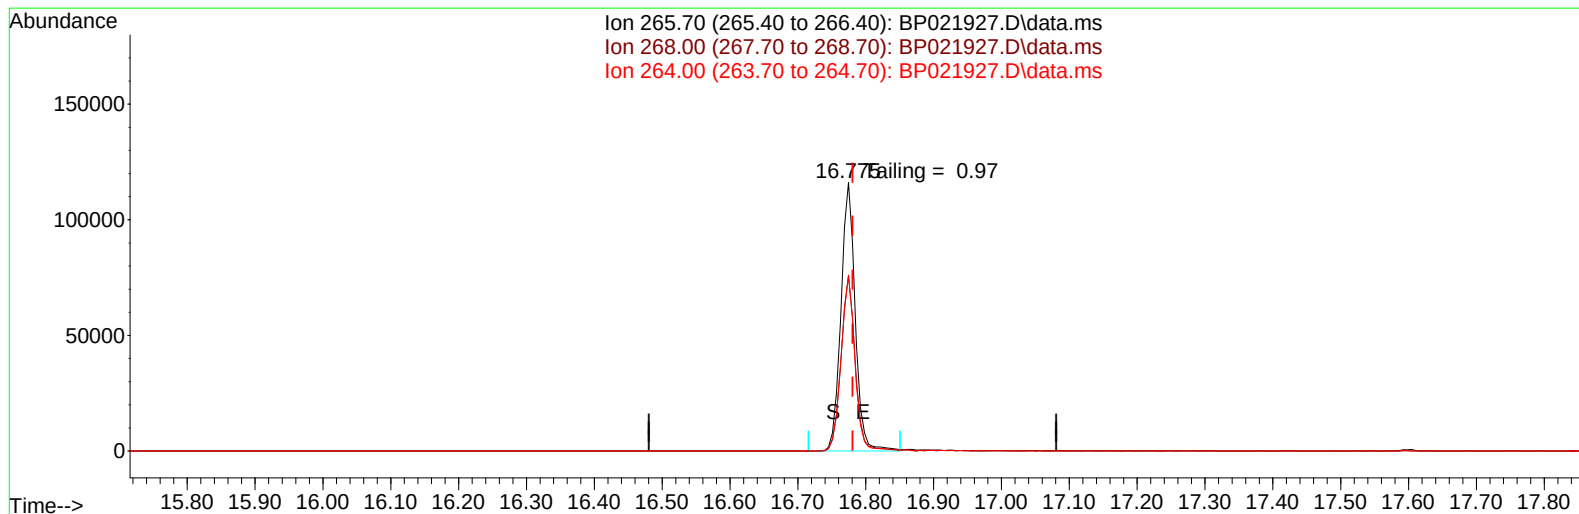

TIC: BP021927.D\data.ms

(70) Pentachlorophenol (C)




16.775min (-0.006) 2589960.09 ng

response 169375

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	65.19
264.00	63.60	65.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091624\
Data File : BP021927.D
Acq On : 16 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 16:49:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 16 16:26:06 2024
Response via : Initial Calibration

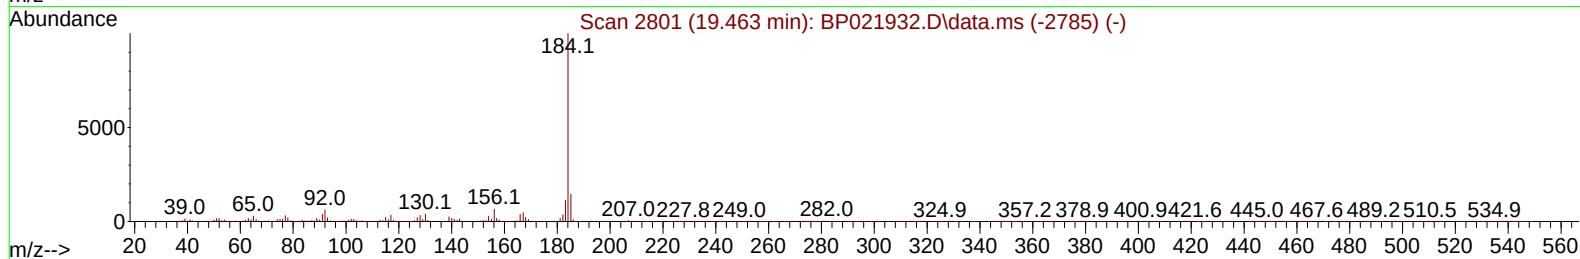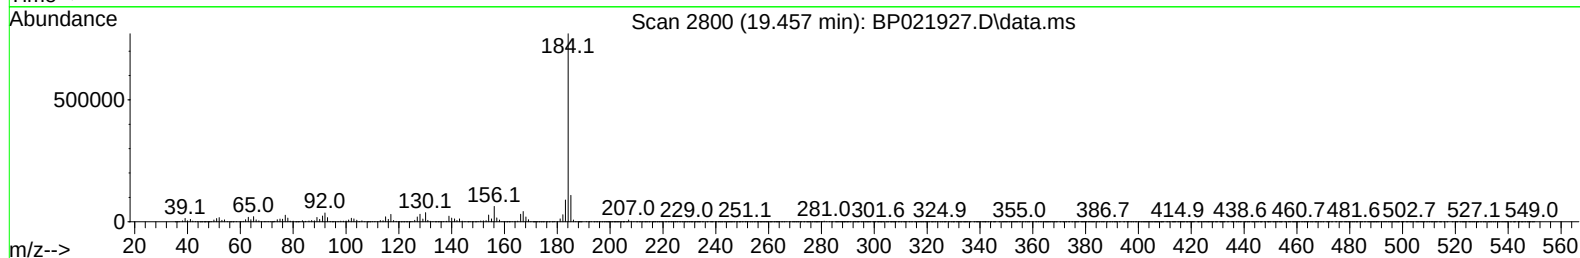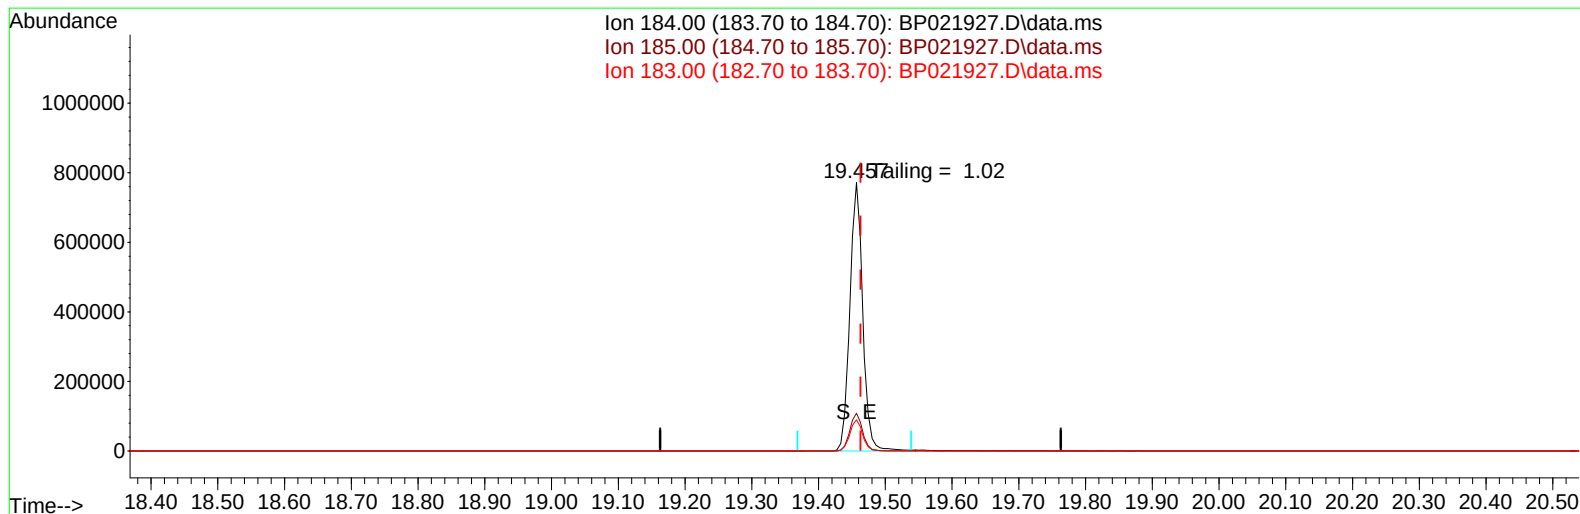

TIC: BP021927.D\data.ms

(77) Benzidine**19.457min (-0.006) 8876393.78 ng****response 1033431**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.06
183.00	11.20	11.62
0.00	0.00	0.00