


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091624\
Data File : BP021927.D
Acq On : 16 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 16 17:00:19 2024

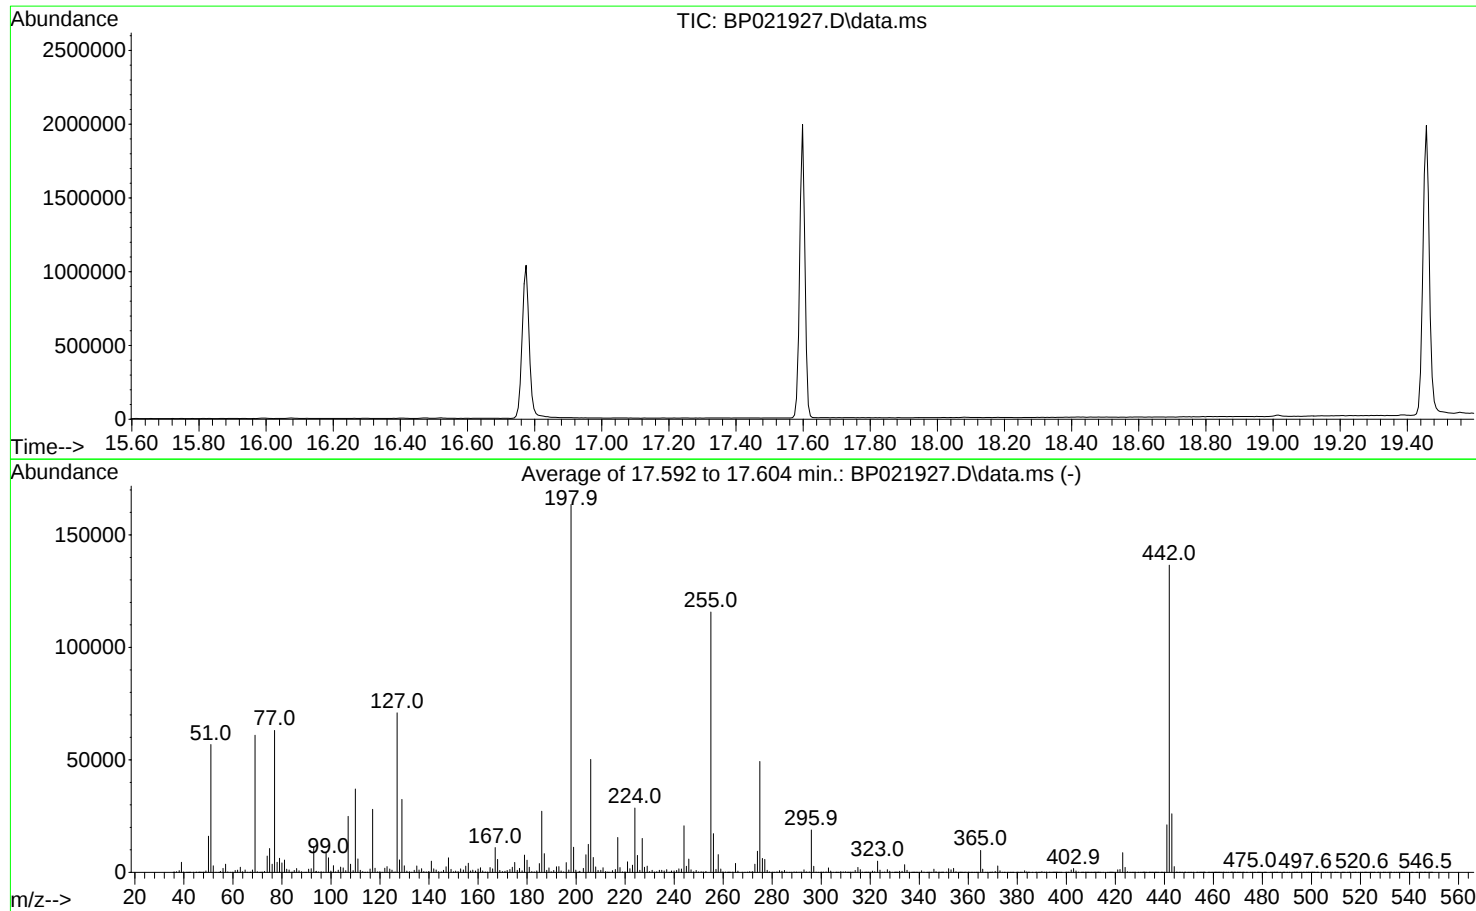




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2475

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	34.8	56852	PASS
68	69	0.00	2	1.8	1099	PASS
69	198	0.00	100	37.3	60989	PASS
70	69	0.00	2	0.5	303	PASS
127	198	10	80	43.4	70944	PASS
197	198	0.00	2	0.7	1075	PASS
198	198	100	100	100.0	163517	PASS
199	198	5	9	6.8	11164	PASS
275	198	10	60	30.1	49292	PASS
365	198	1	100	6.0	9772	PASS
441	198	0.01	100	12.9	21167	PASS
442	442	100	100	100.0	136533	PASS
443	442	15	24	19.1	26035	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091624\
Data File : BP021927.D
Acq On : 16 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 16:49:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 16 16:26:06 2024
Response via : Initial Calibration

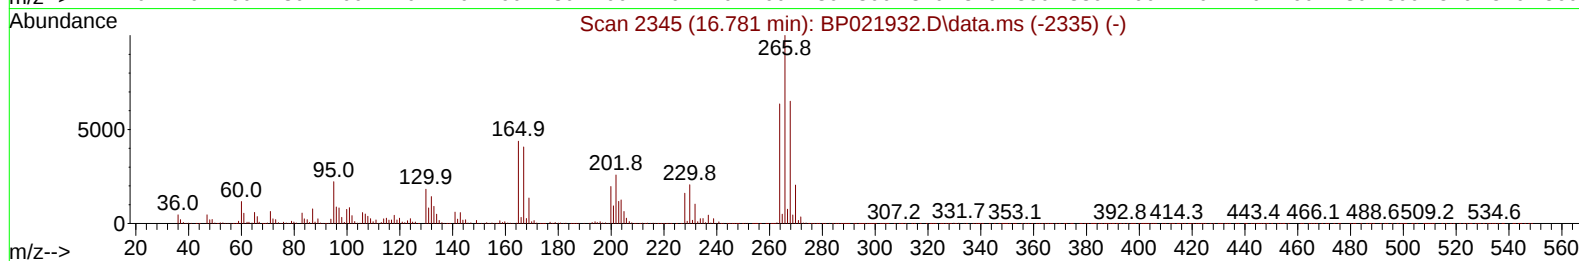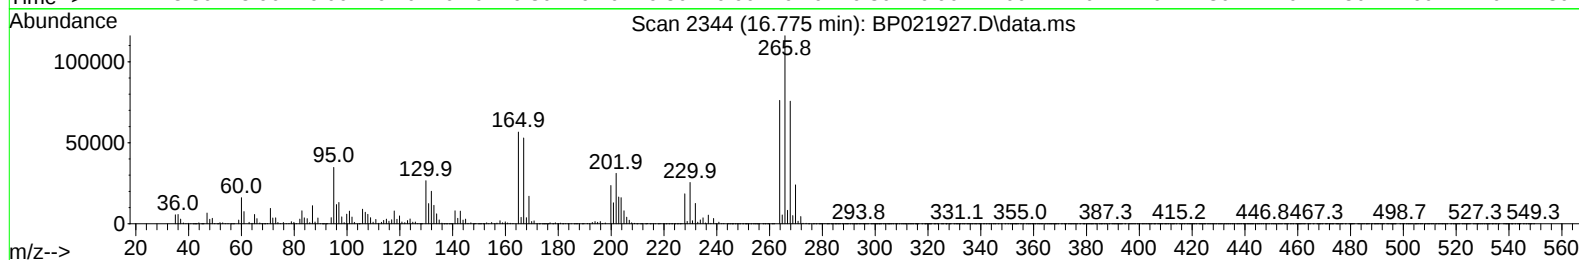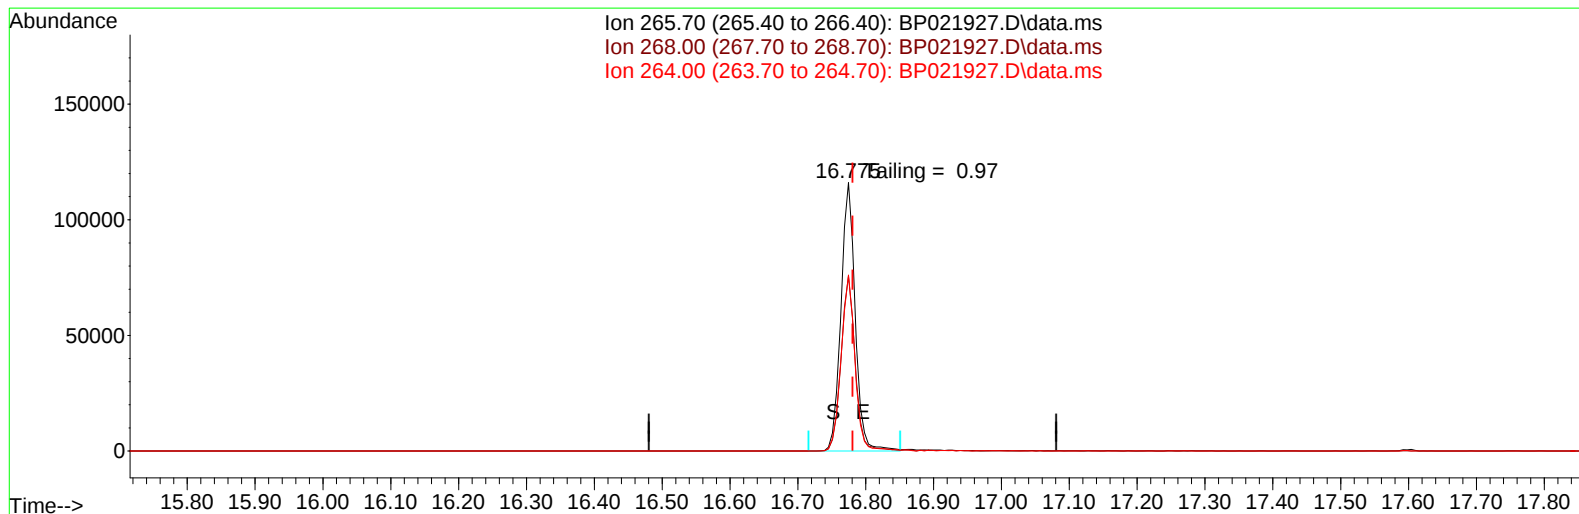

TIC: BP021927.D\data.ms

(70) Pentachlorophenol (C)

16.775min (-0.006) 2589960.09 ng




response 169375

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	65.19
264.00	63.60	65.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091624\
Data File : BP021927.D
Acq On : 16 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 16:49:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 16 16:26:06 2024
Response via : Initial Calibration

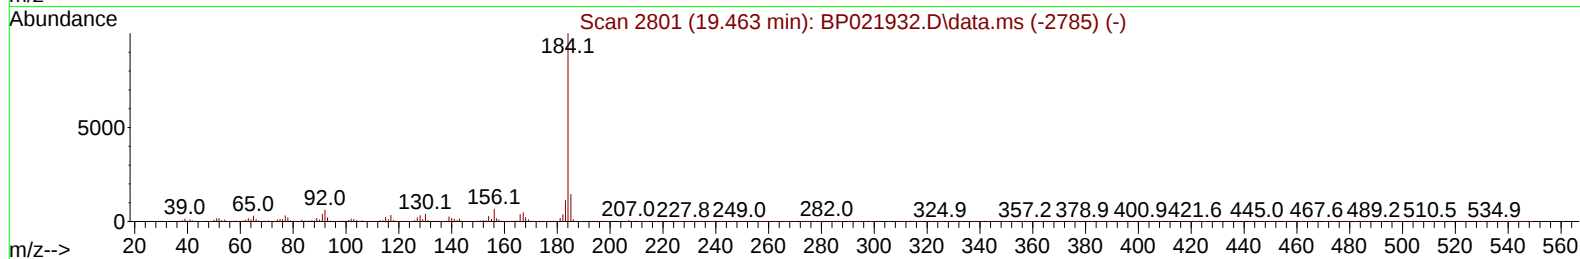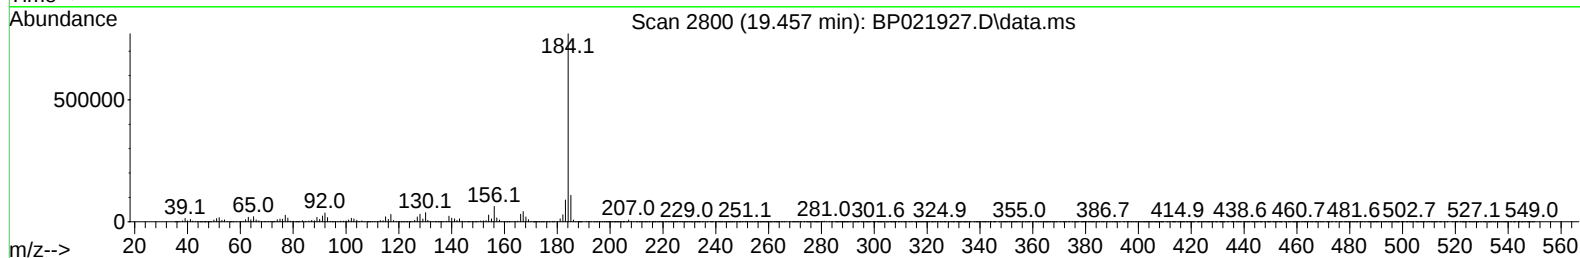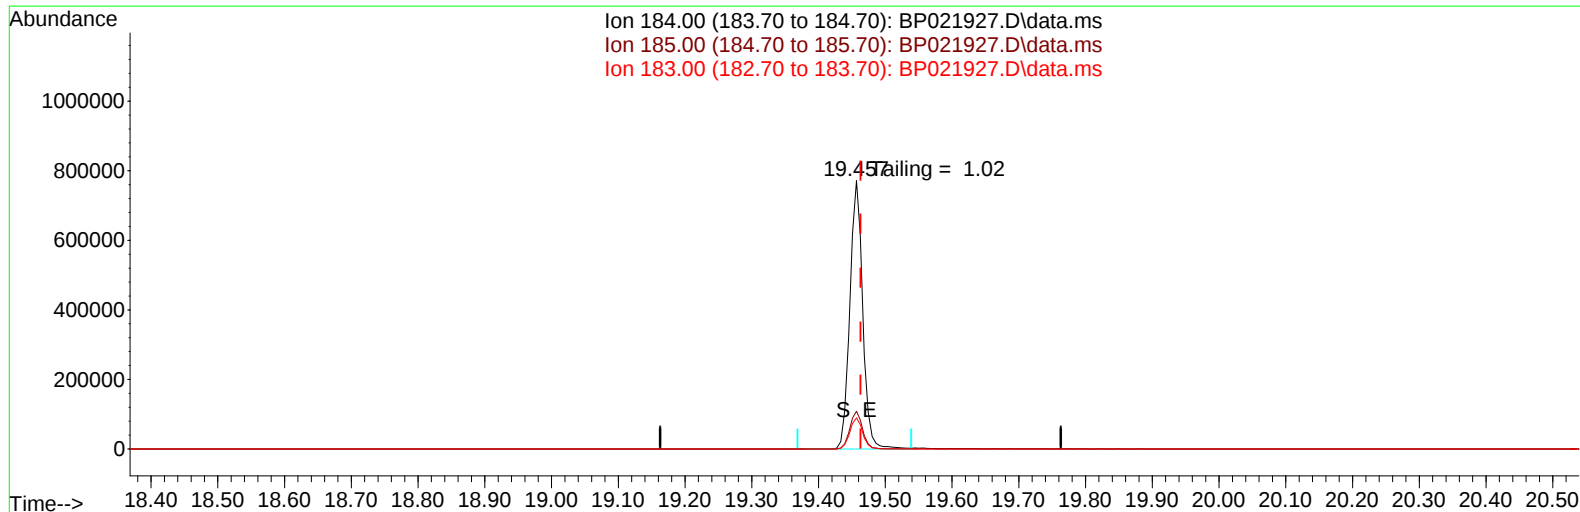

TIC: BP021927.D\data.ms

(77) Benzidine

19.457min (-0.006) 8876393.78 ng

response 1033431

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.06
183.00	11.20	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/16/2024	BNA_P	<u>BP021927.D</u>
Compound Name	Response	Retention Time
DDT	584101	20.751
DDD	7756	20.345
DDE	0	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7756	591857	1.31

Instrument :
BNA_P
ClientSampleId :
DFTPP