
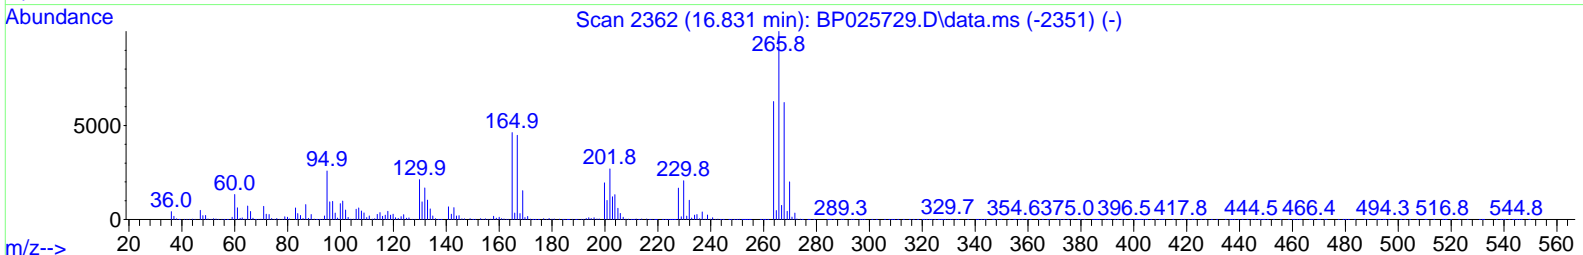
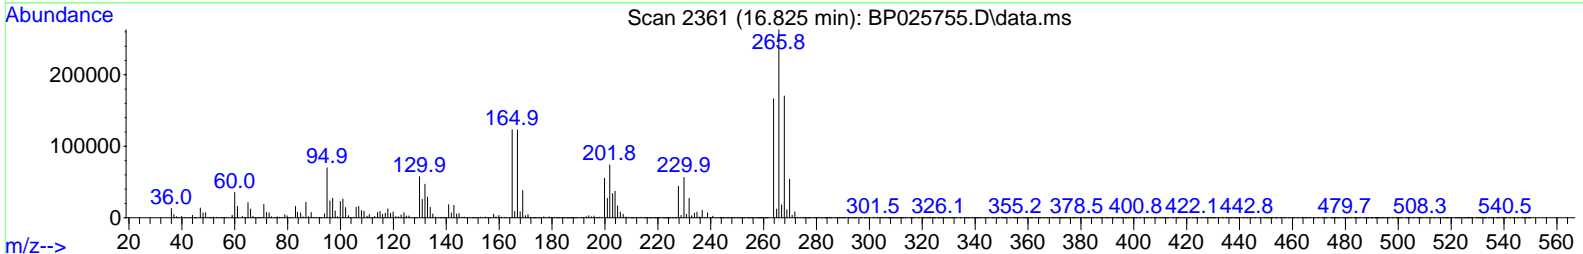


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091625\
 Data File : BP025755.D
 Acq On : 16 Sep 2025 12:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 13:17:17 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 16:45:04 2025
 Response via : Initial Calibration

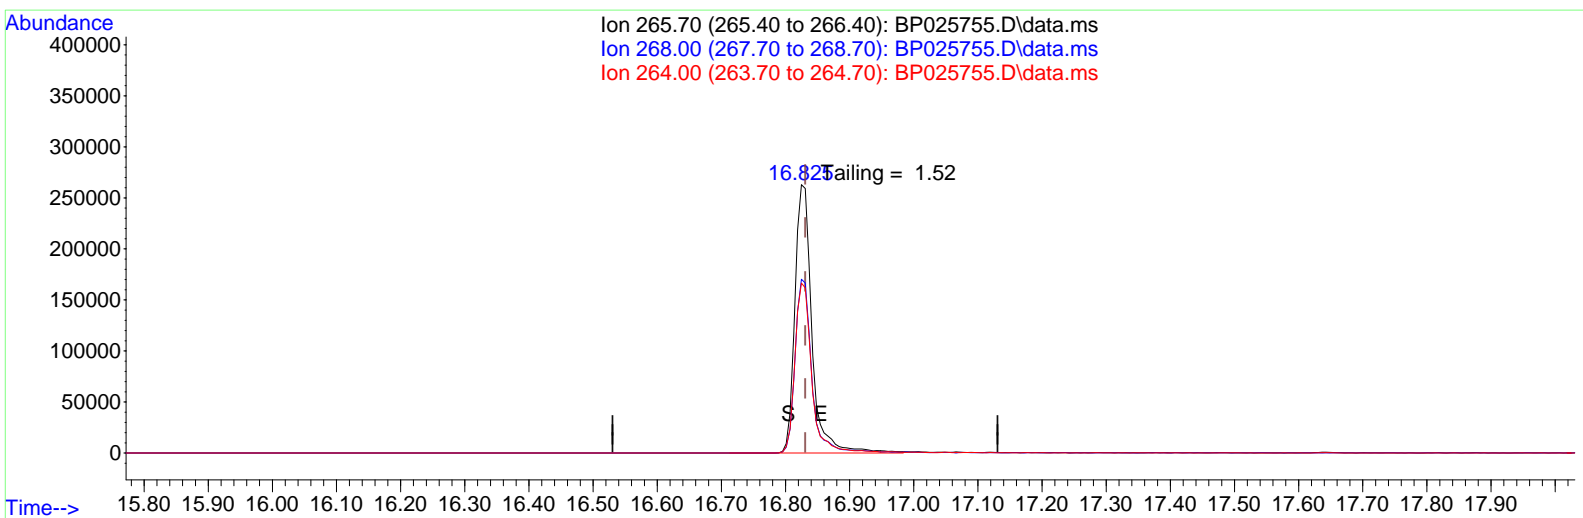

TIC: BP025755.D\data.ms




(70) Pentachlorophenol (C)

16.825min (-0.006) 2241284.43 ng

response	489303
Ion	Exp% Act%
265.70	100.00 100.00
268.00	62.30 64.78
264.00	62.70 63.35
0.00	0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091625\
 Data File : BP025755.D
 Acq On : 16 Sep 2025 12:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 13:17:17 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 16:45:04 2025
 Response via : Initial Calibration

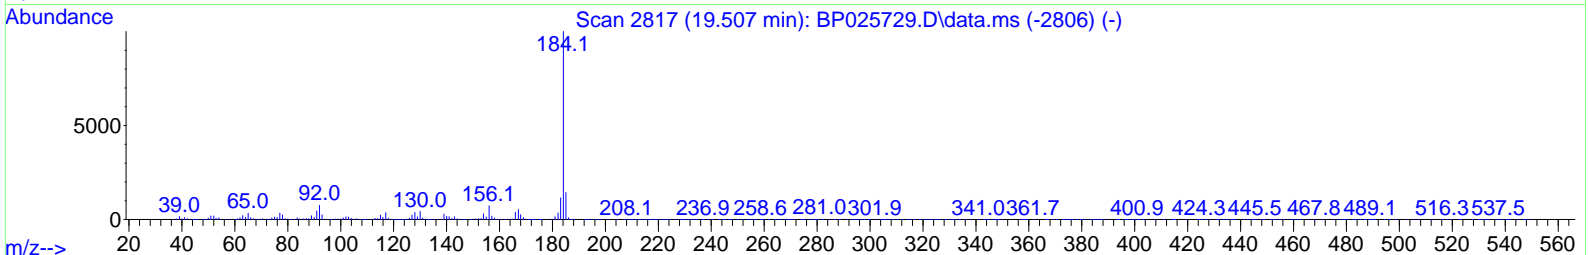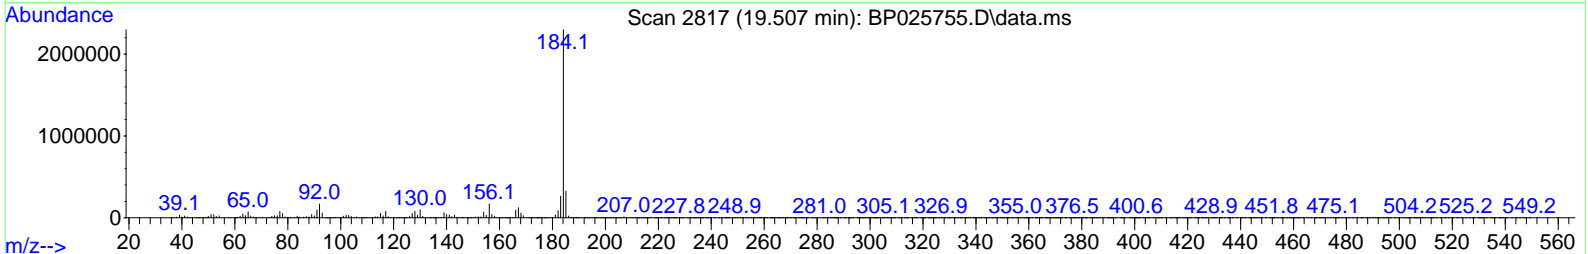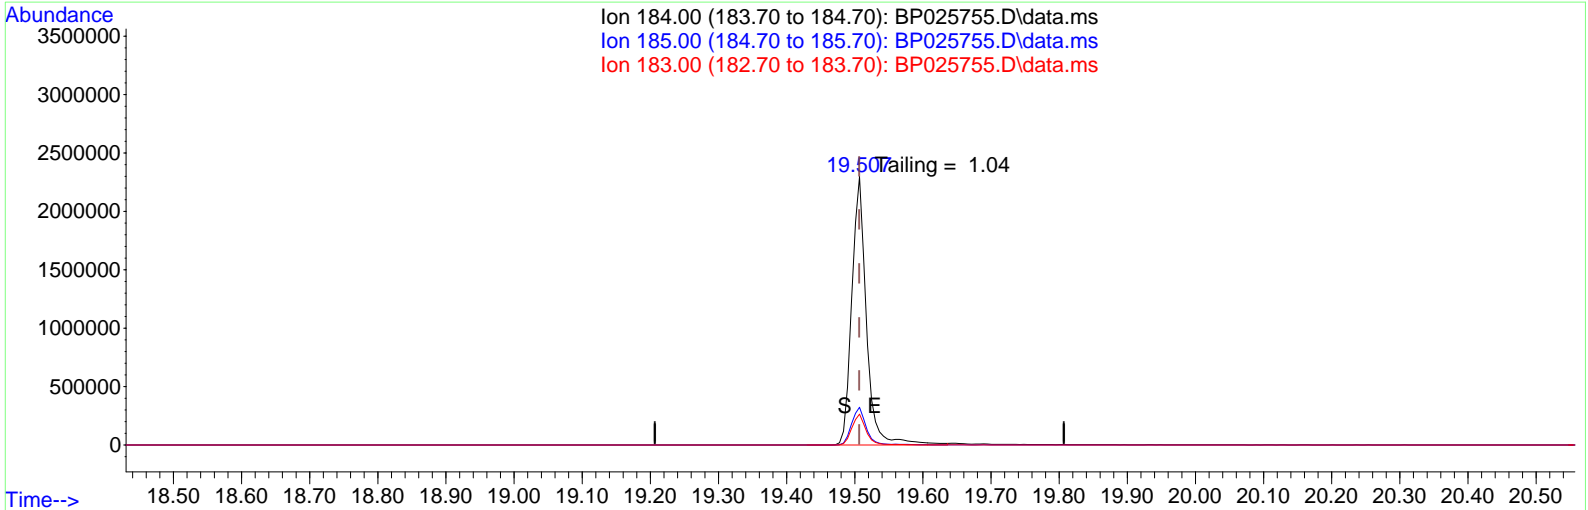

TIC: BP025755.D\data.ms

(77) Benzidine

19.507min (+ 0.000) 744639.67 ng

response 3324689

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.10
183.00	11.50	11.53
0.00	0.00	0.00