


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091719\
 Data File : BP000261.D
 Acq On : 17 Sep 2019 10:29
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 16 18:59:05 2019

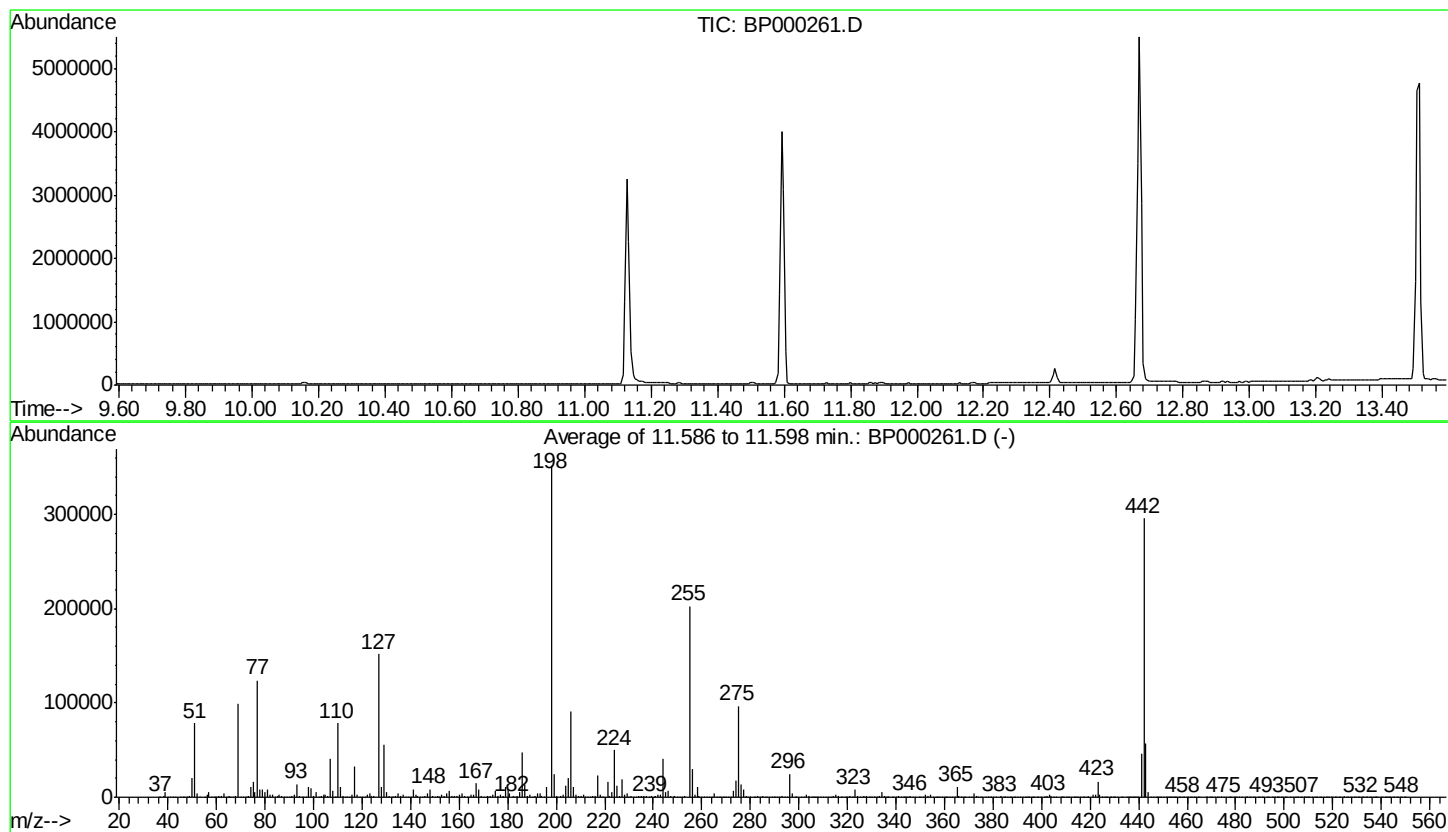

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	78757	PASS
68	69	0.00	2	2.0	1958	PASS
69	198	0.00	100	28.2	99037	PASS
70	69	0.00	2	0.5	541	PASS
127	198	10	80	43.1	151647	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	351809	PASS
199	198	5	9	6.8	23950	PASS
275	198	10	60	27.5	96821	PASS
365	198	1	100	3.2	11422	PASS
441	198	0.01	100	13.1	46045	PASS
442	198	50	100	84.1	296024	PASS
443	442	15	24	19.4	57500	PASS