
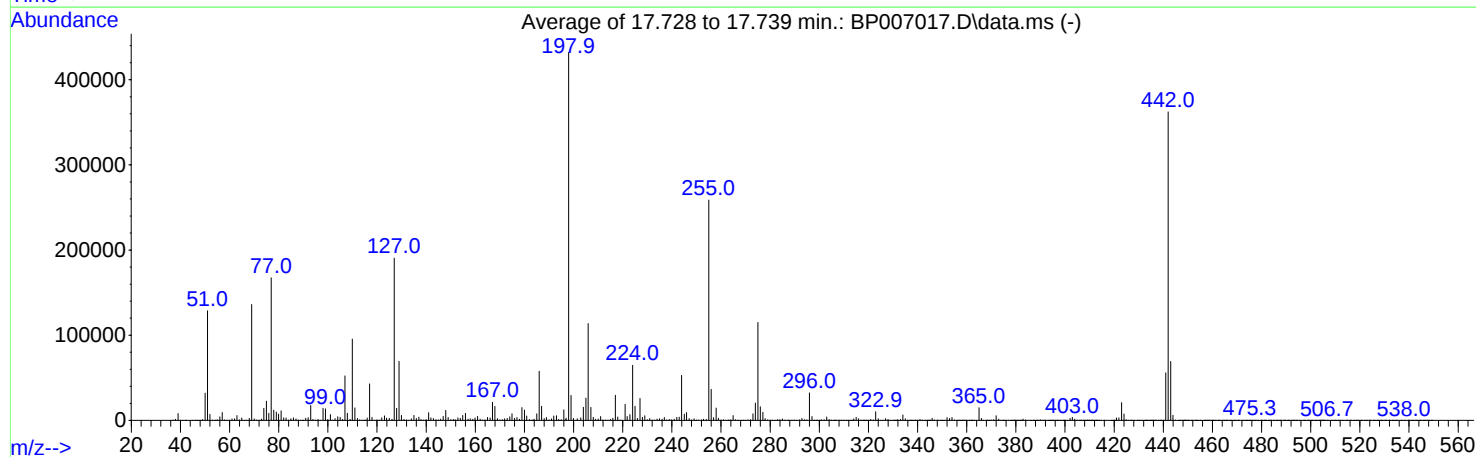


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091721\
 Data File : BP007017.D
 Acq On : 17 Sep 2021 09:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 17 10:50:16 2021

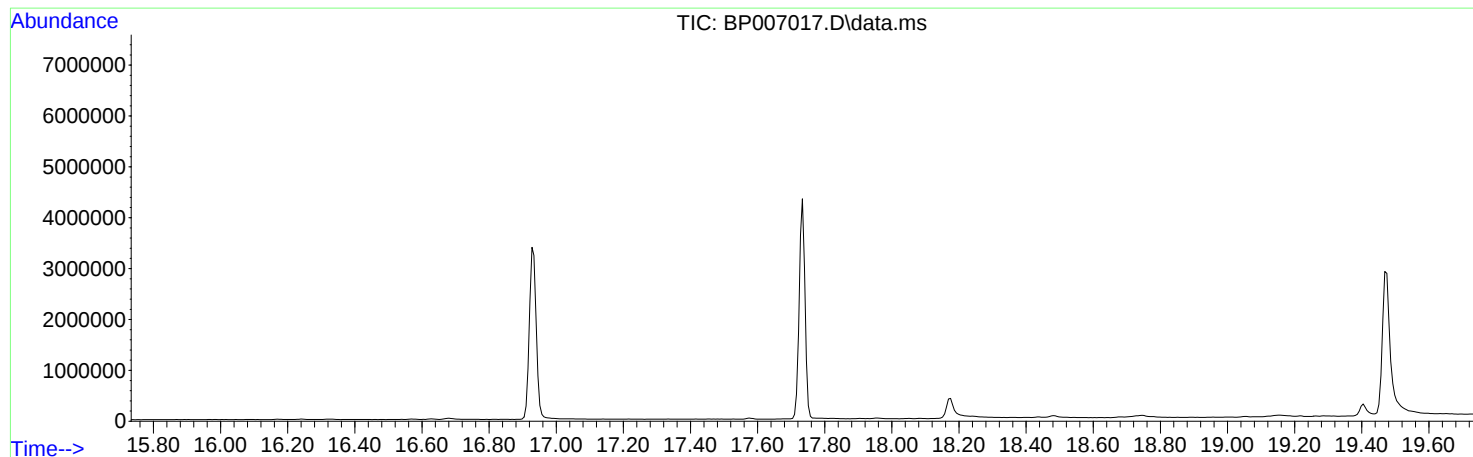




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	128767	PASS
68	69	0.00	2	1.8	2404	PASS
69	198	0.00	100	31.5	136034	PASS
70	69	0.00	2	1.2	1641	PASS
127	198	10	80	44.1	190582	PASS
197	198	0.00	2	0.6	2655	PASS
198	198	100	100	100.0	431988	PASS
199	198	5	9	6.8	29400	PASS
275	198	10	60	26.6	114989	PASS
365	198	1	100	3.4	14814	PASS
441	198	0.01	100	12.9	55832	PASS
442	442	100	100	100.0	362304	PASS
443	442	15	24	19.1	69221	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091721\
 Data File : BP007017.D
 Acq On : 17 Sep 2021 09:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 17 10:45:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 16 15:16:52 2021
 Response via : Initial Calibration

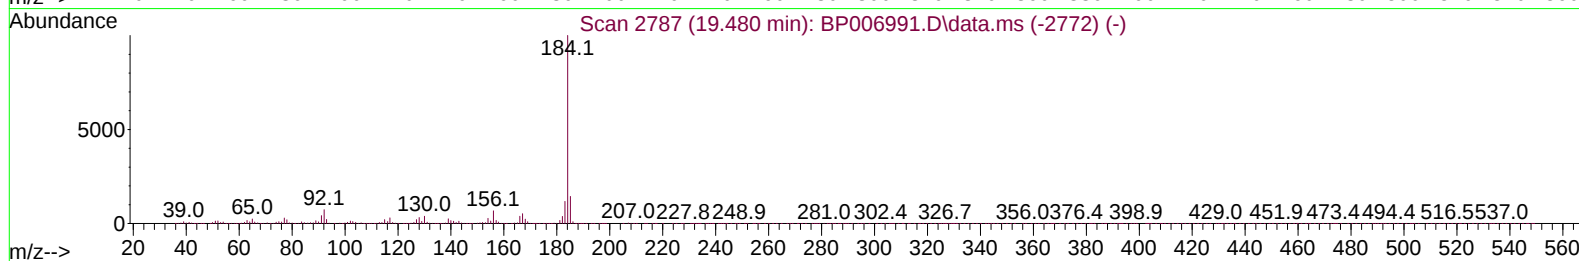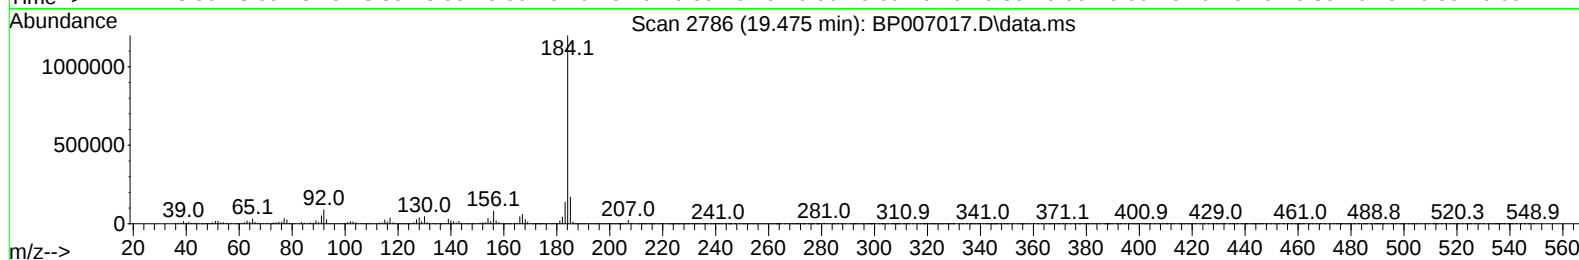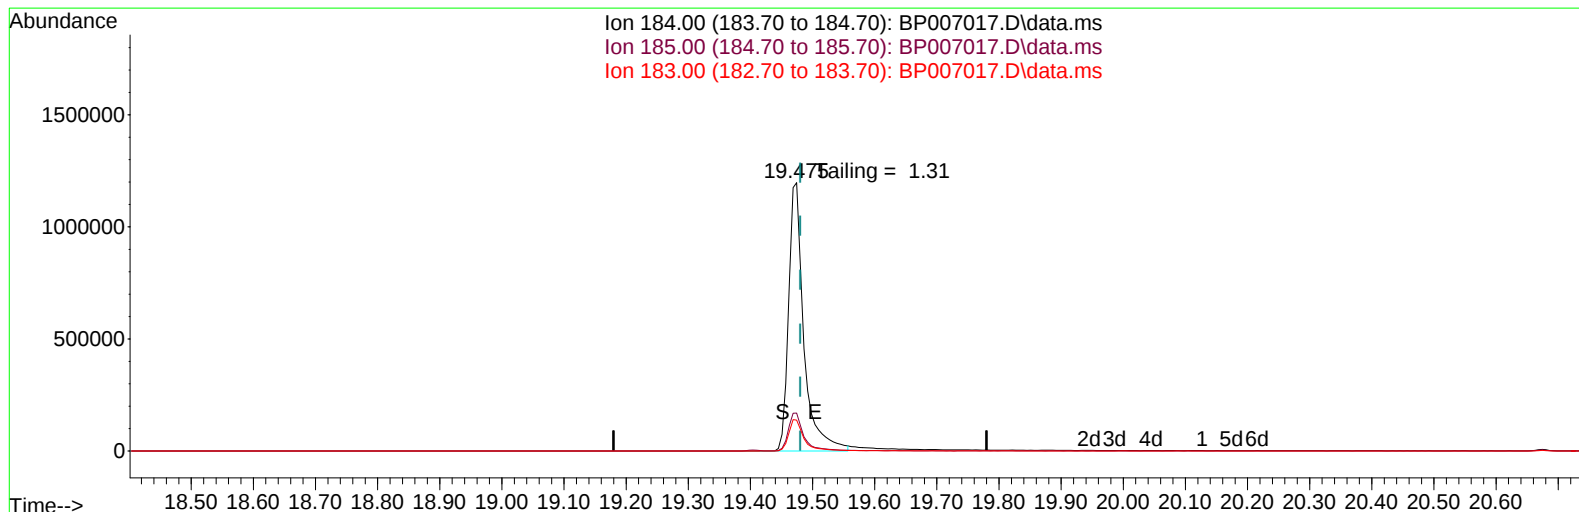

TIC: BP007017.D\data.ms

(77) Benzidine

19.475min (-0.005) -20.00 ng m




response 2141525

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.16
183.00	11.90	11.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091721\
 Data File : BP007017.D
 Acq On : 17 Sep 2021 09:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 17 10:45:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 16 15:16:52 2021
 Response via : Initial Calibration

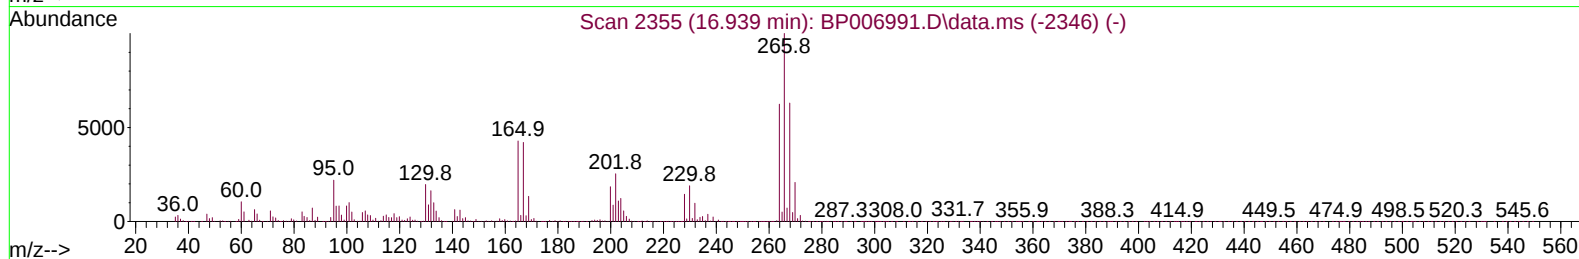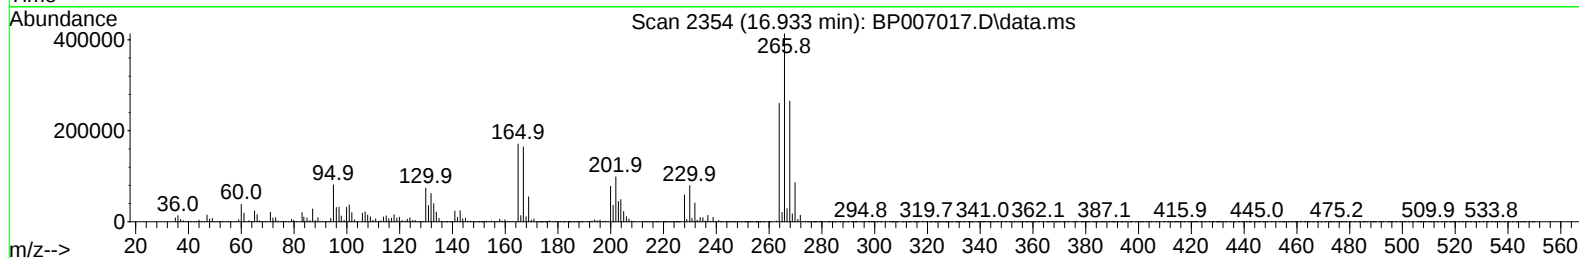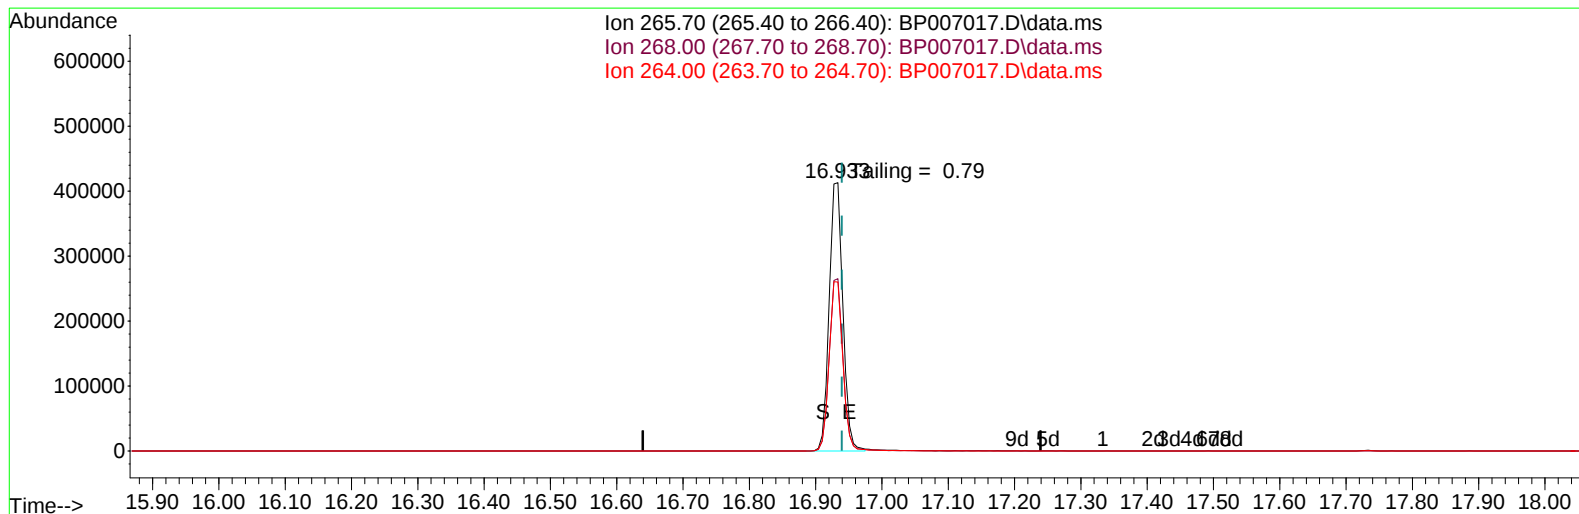

TIC: BP007017.D\data.ms

(70) Pentachlorophenol (C)

16.933min (-0.006) 24912.63 ng m

response 591789

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.20
264.00	62.90	62.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/17/2021	BNA_P	<u>BP007017.D</u>
Compound Name	Response	Retention Time
DDT	1612011	20.67
DDD	6699	20.24
DDE	1963	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8662	1620673	0.53