
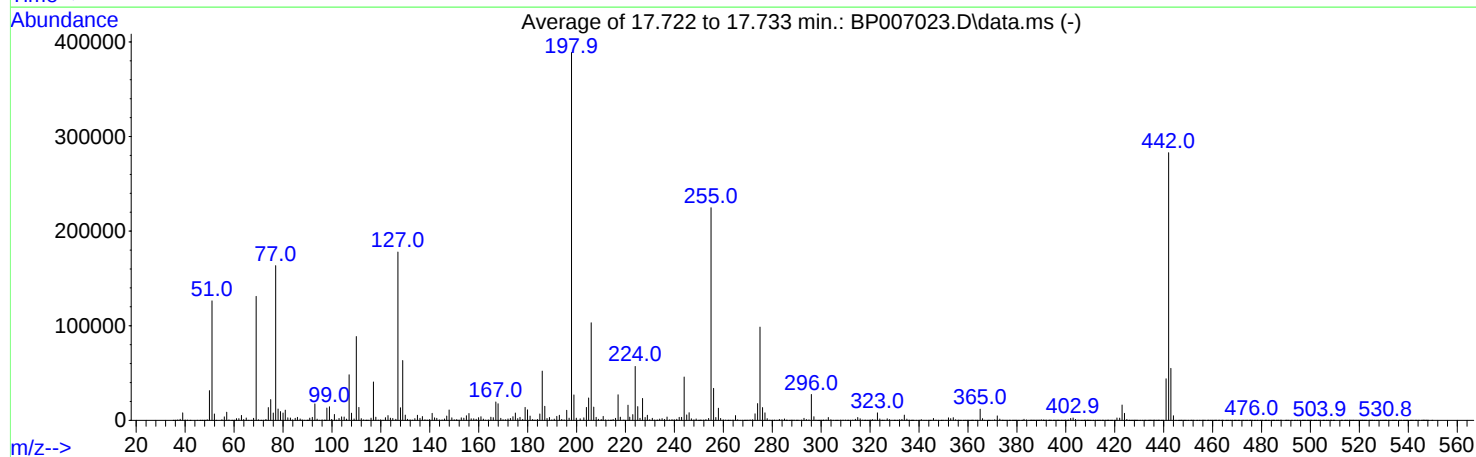


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091721\
 Data File : BP007023.D
 Acq On : 17 Sep 2021 12:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 17 10:50:16 2021

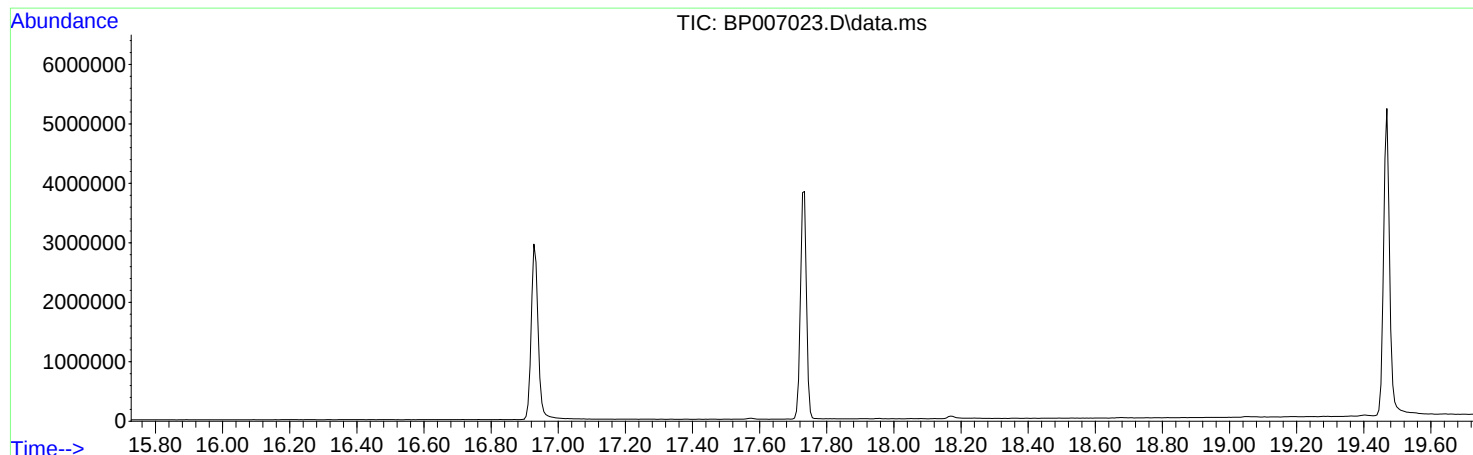




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	126394	PASS
68	69	0.00	2	1.7	2273	PASS
69	198	0.00	100	33.7	131118	PASS
70	69	0.00	2	0.5	689	PASS
127	198	10	80	45.8	177936	PASS
197	198	0.00	2	0.6	2343	PASS
198	198	100	100	100.0	388806	PASS
199	198	5	9	6.9	26816	PASS
275	198	10	60	25.4	98566	PASS
365	198	1	100	3.1	11907	PASS
441	198	0.01	100	11.3	43923	PASS
442	442	100	100	100.0	282976	PASS
443	442	15	24	19.4	54905	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091721\
 Data File : BP007023.D
 Acq On : 17 Sep 2021 12:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 17 13:15:05 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 10:50:16 2021
 Response via : Initial Calibration

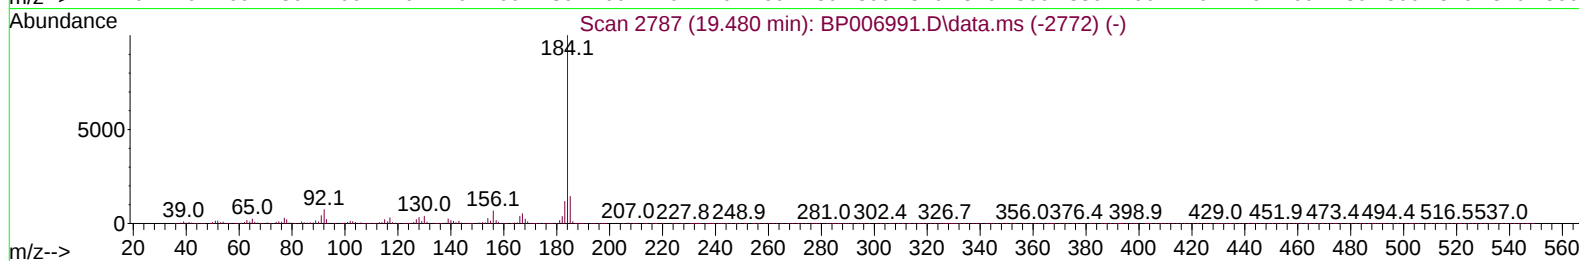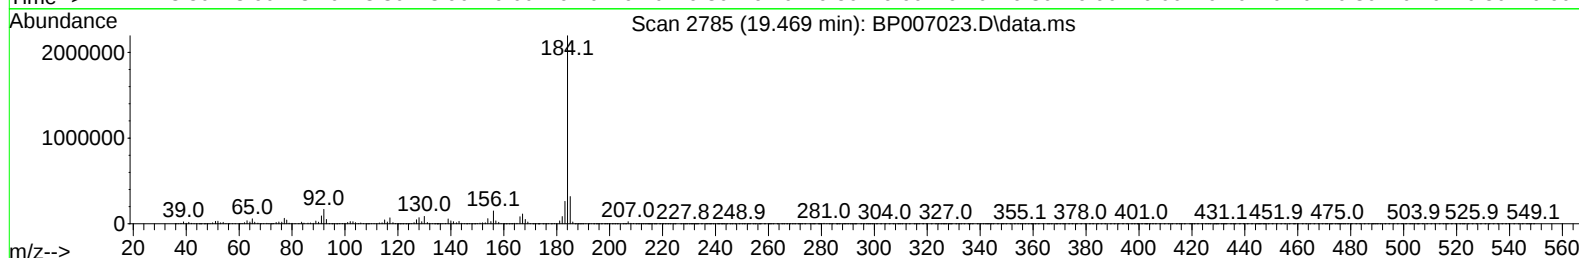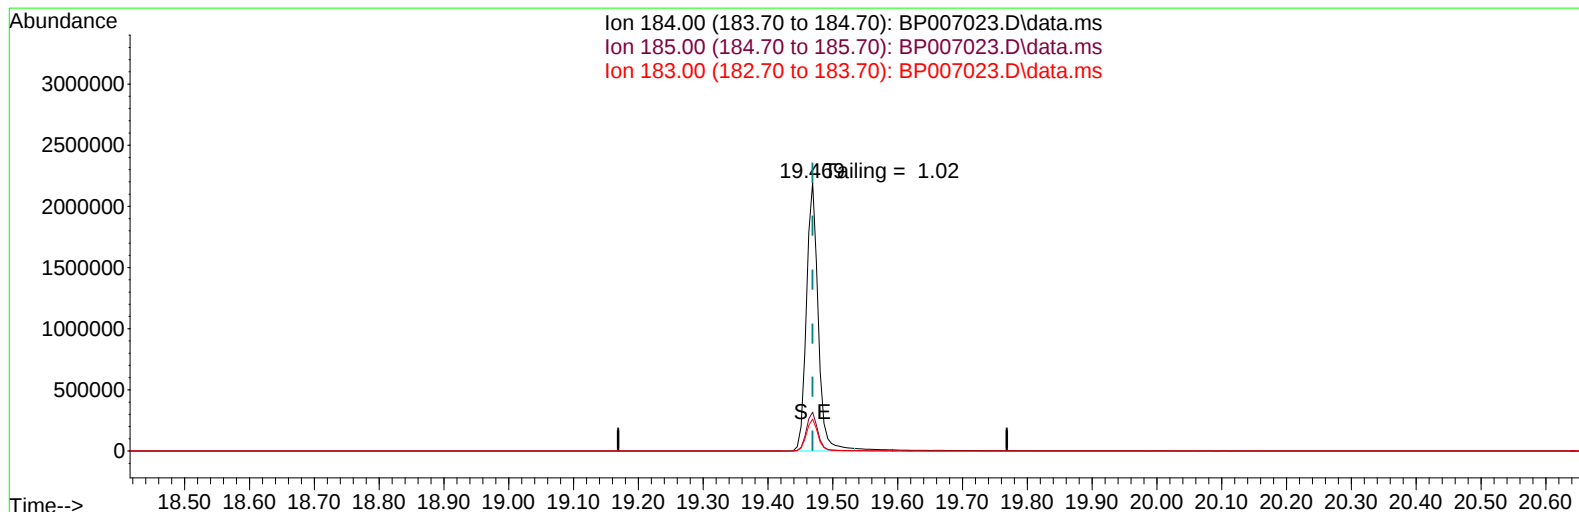

TIC: BP007023.D\data.ms

(77) Benzidine

19.469min (-0.000) -20.00 ng




response 2821562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.50
183.00	11.90	11.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091721\
 Data File : BP007023.D
 Acq On : 17 Sep 2021 12:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 17 13:15:05 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 10:50:16 2021
 Response via : Initial Calibration

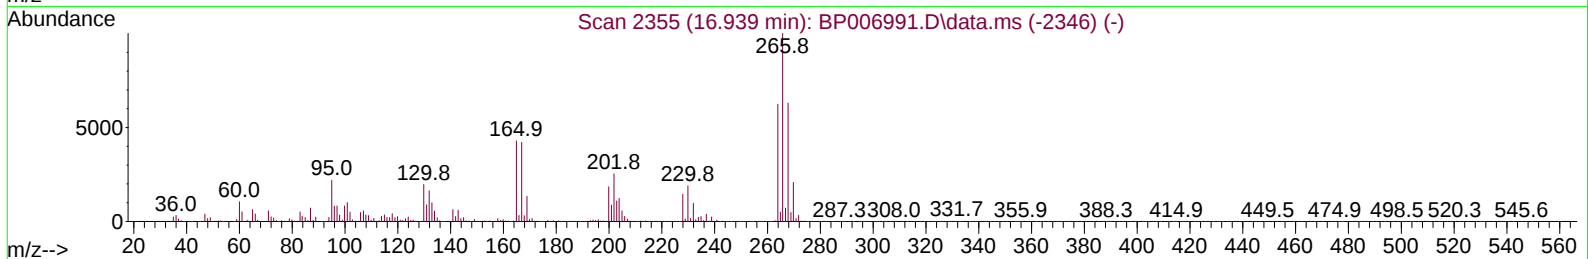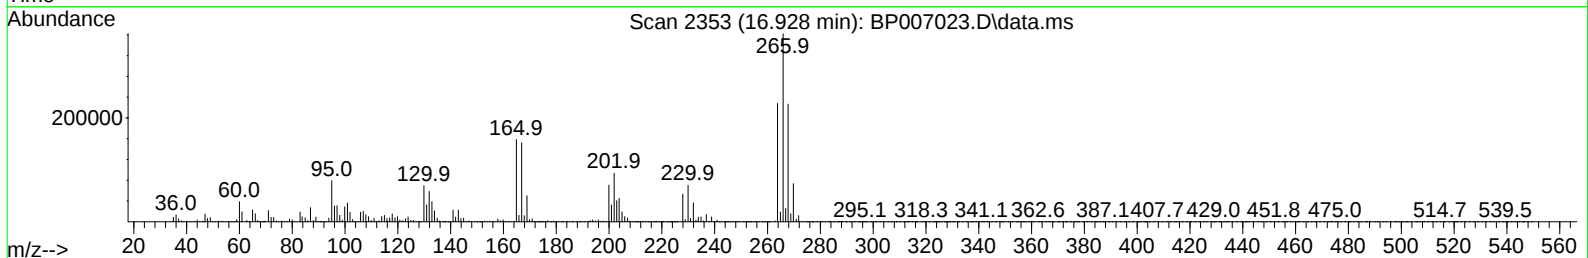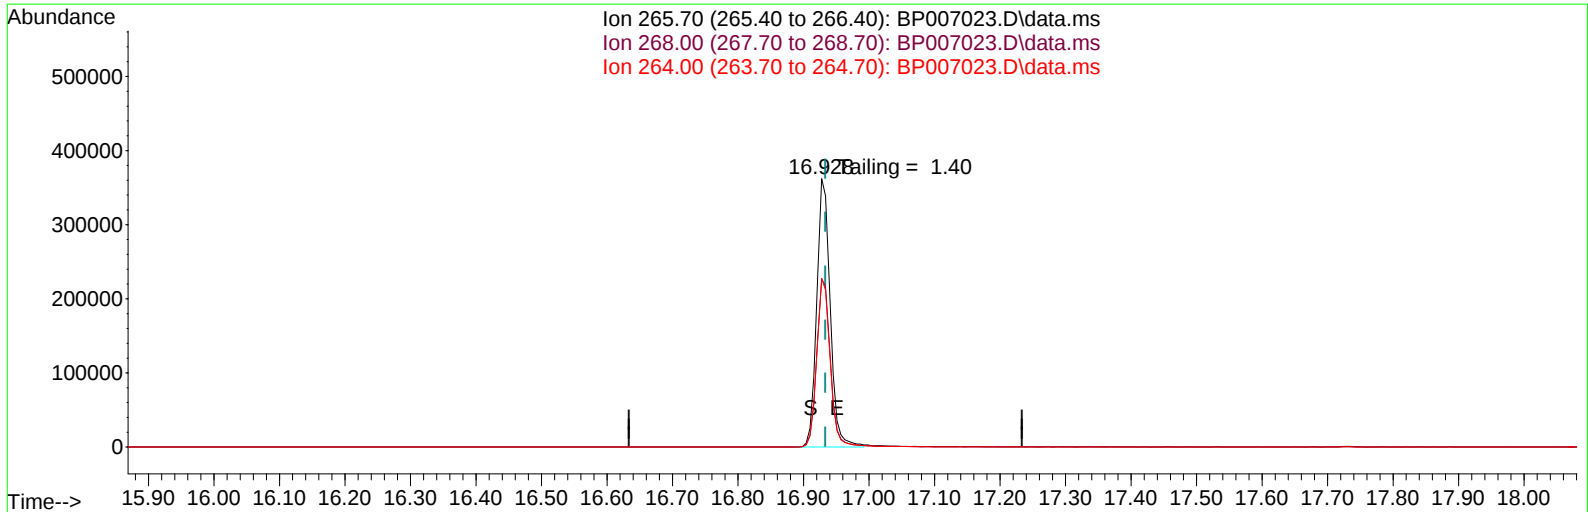

TIC: BP007023.D\data.ms

(70) Pentachlorophenol (C)

16.928min (-0.006) 101511.85 ng

response 524244

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.54
264.00	62.90	62.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/17/2021	BNA_P	<u>BP007023.D</u>
Compound Name	Response	Retention Time
DDT	1460567	20.67
DDD	7647	20.24
DDE	2534	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10181	1470748	0.69