
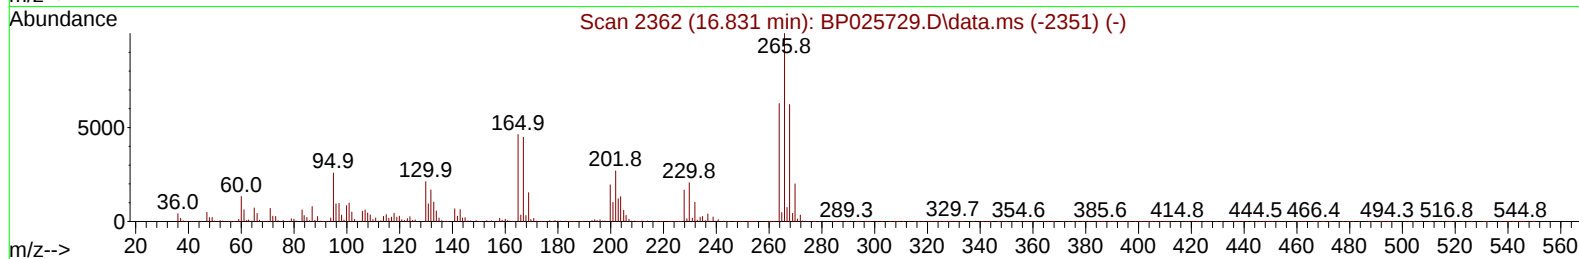
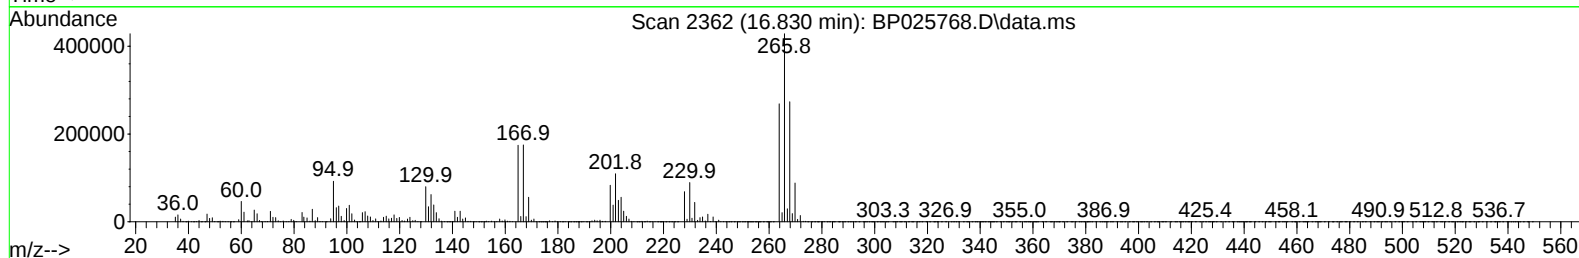


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091725\
Data File : BP025768.D
Acq On : 17 Sep 2025 11:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 13:24:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

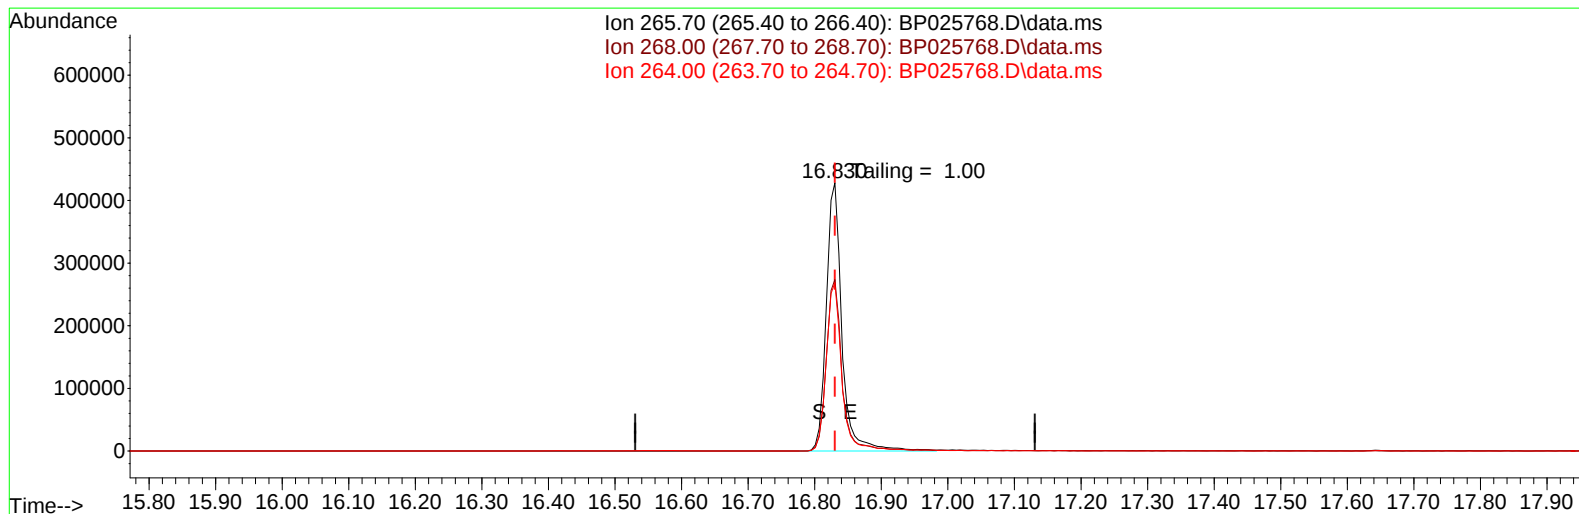

TIC: BP025768.D\data.ms

(70) Pentachlorophenol (C)




16.830min (-0.000) 1245628.62 ng

response 694952

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.86
264.00	62.70	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091725\
Data File : BP025768.D
Acq On : 17 Sep 2025 11:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 13:24:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

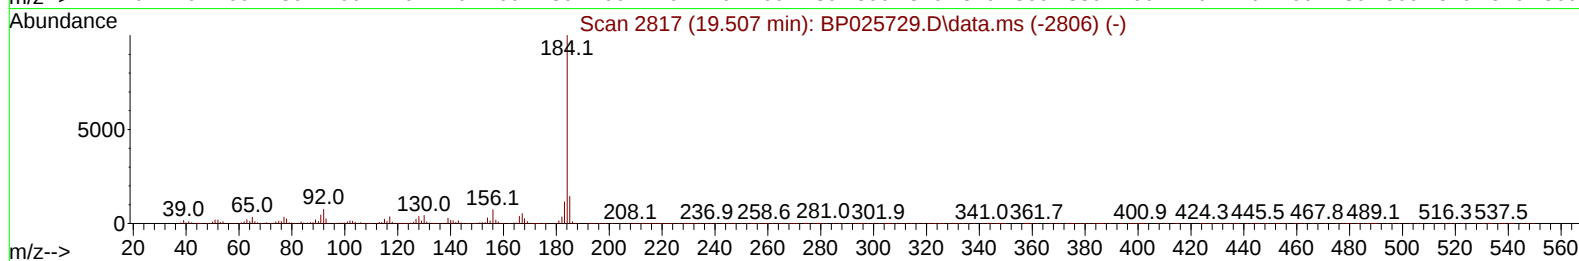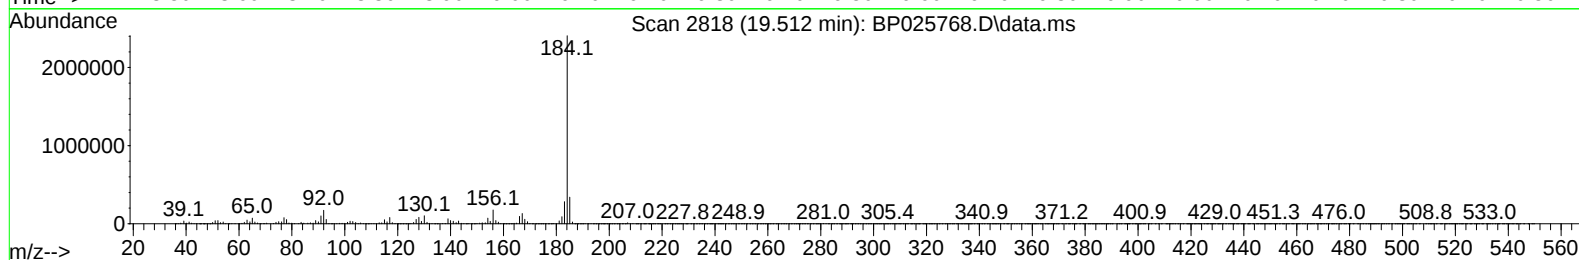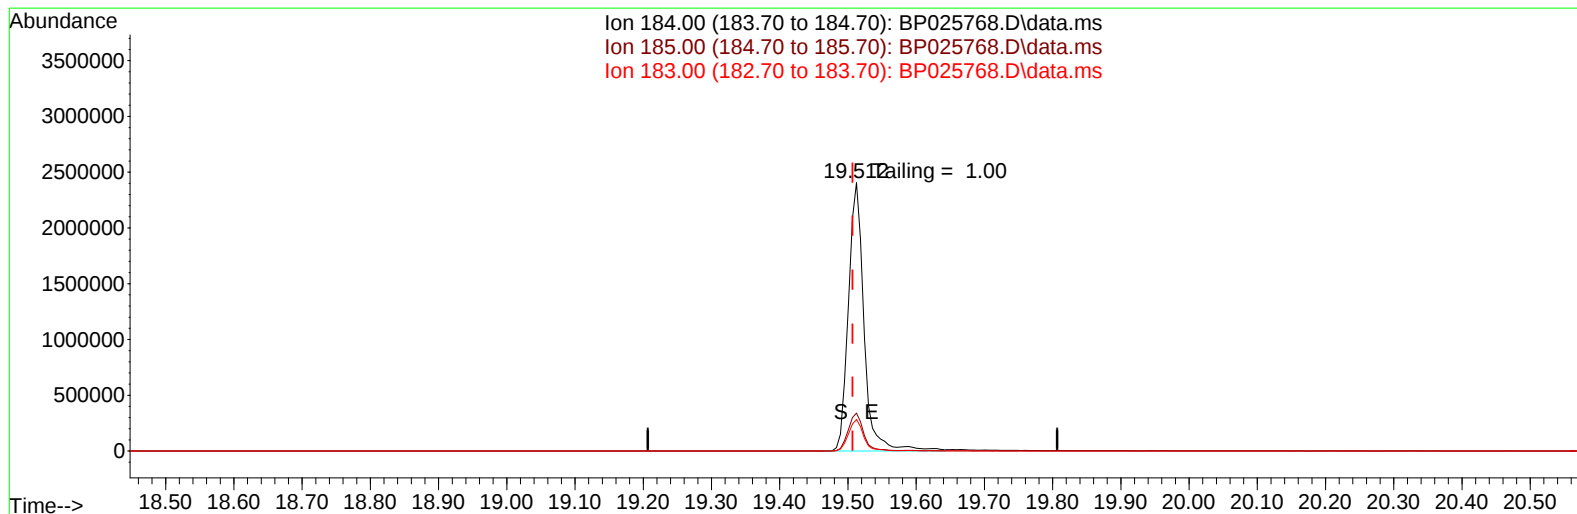

TIC: BP025768.D\data.ms

(77) Benzidine

19.512min (+ 0.006) 1057543.21 ng

response 3746937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	11.50	11.77
0.00	0.00	0.00