
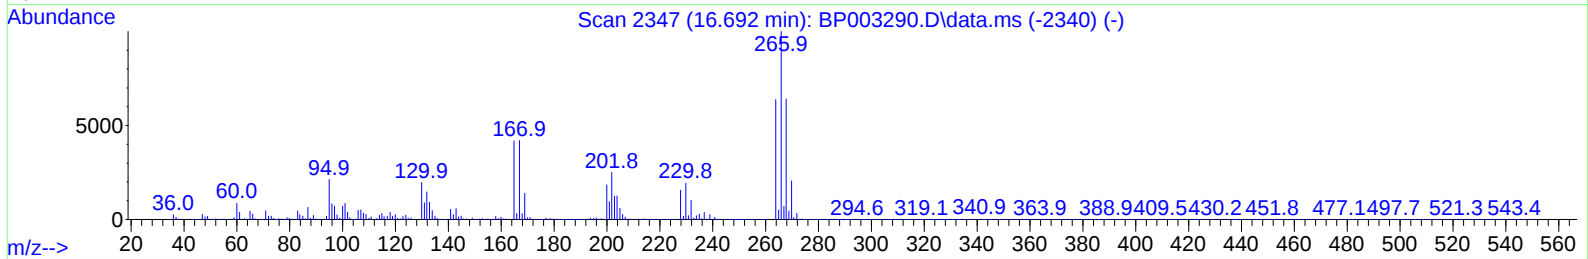
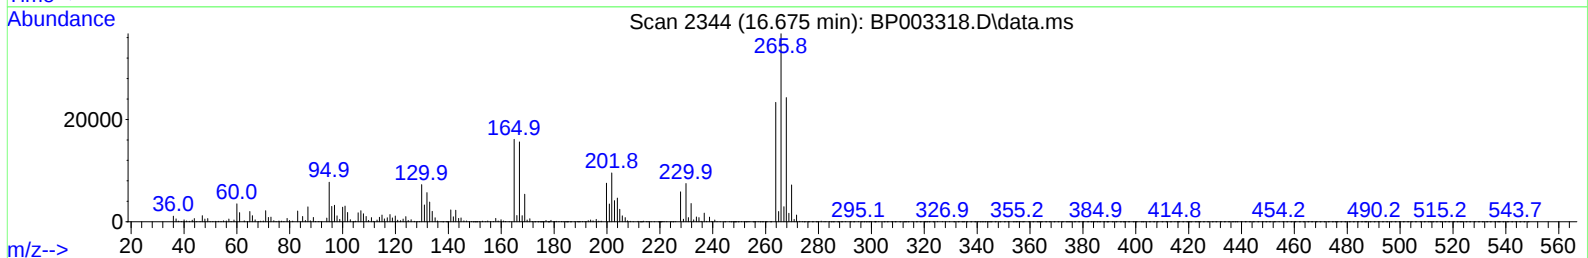


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091820\
Data File : BP003318.D
Acq On : 18 Sep 2020 12:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 13:56:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 16 13:18:39 2020
Response via : Initial Calibration

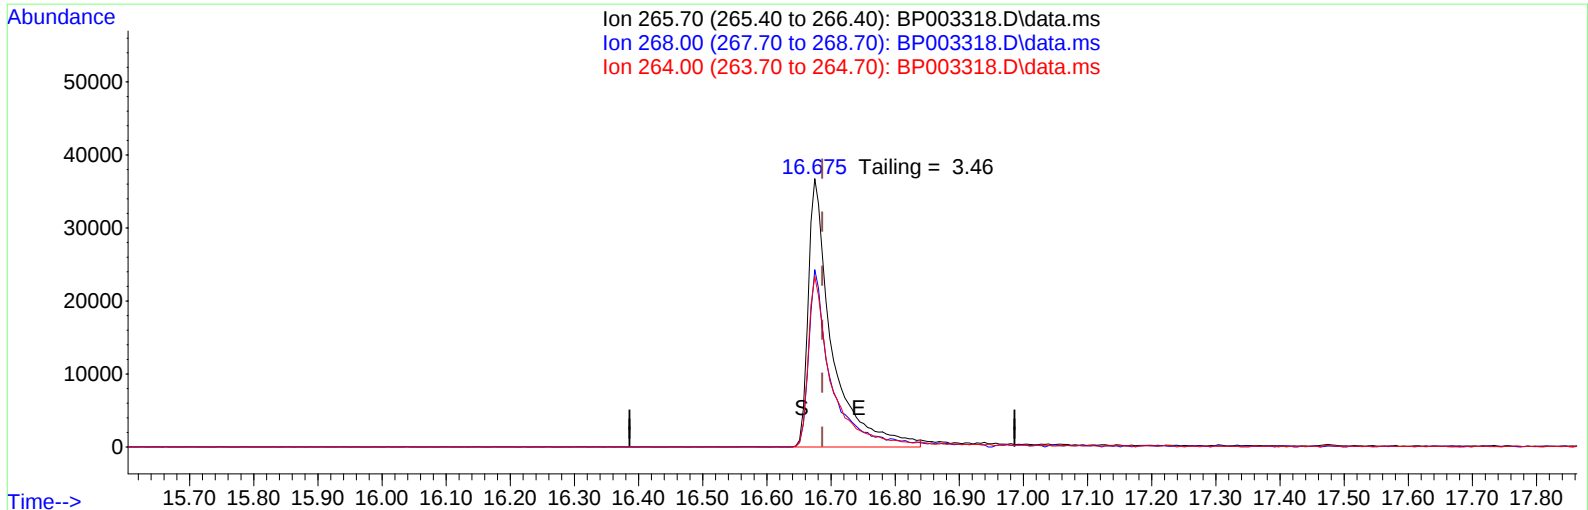

TIC: BP003318.D\data.ms

(70) Pentachlorophenol (C)




16.675min (-0.012) 457989.03 ng

response 95603

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	66.07
264.00	63.30	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091820\
Data File : BP003318.D
Acq On : 18 Sep 2020 12:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 13:56:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 16 13:18:39 2020
Response via : Initial Calibration

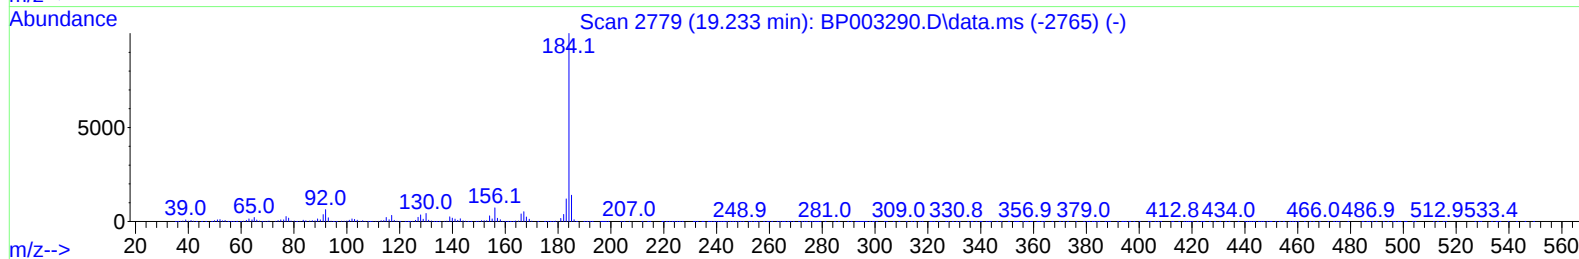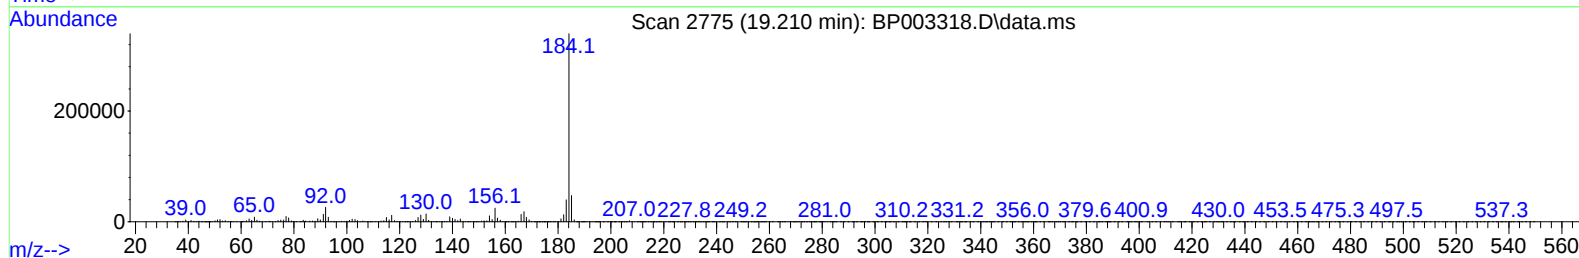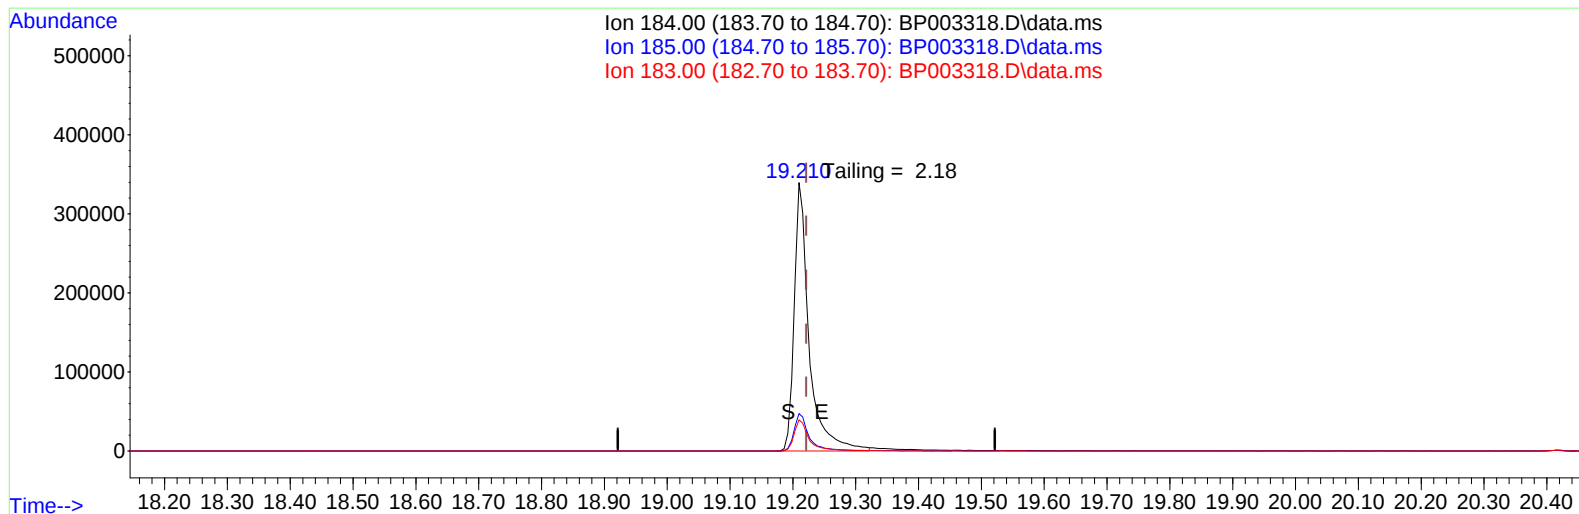

TIC: BP003318.D\data.ms

(77) Benzidine**19.210min (-0.012) 1030715.88 ng****response 575303**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	12.00	11.63
0.00	0.00	0.00