
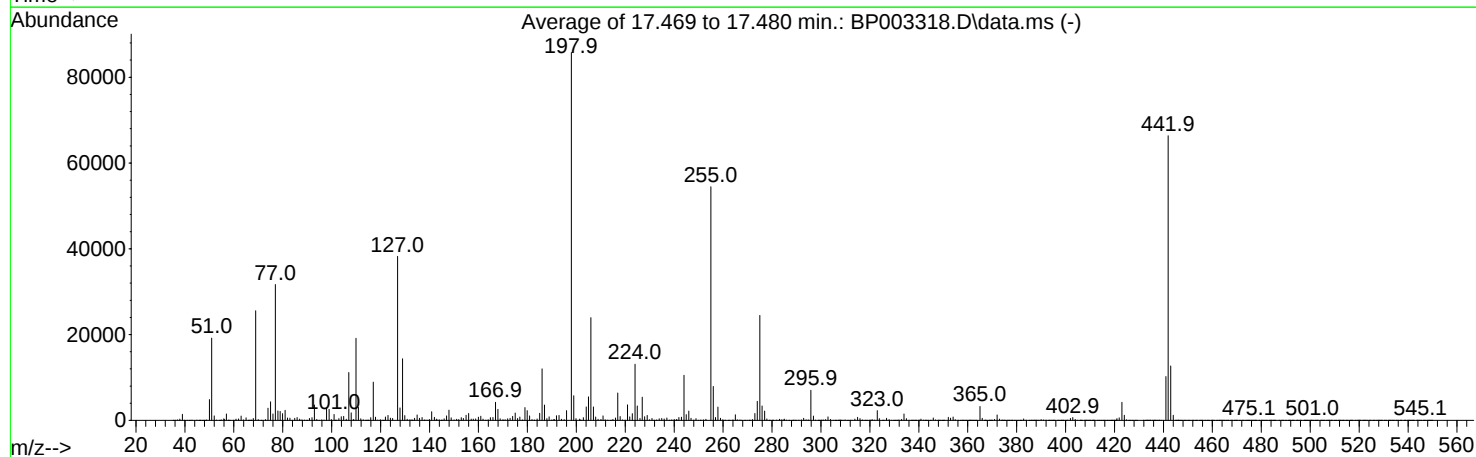


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091820\
 Data File : BP003318.D
 Acq On : 18 Sep 2020 12:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 18 14:13:41 2020

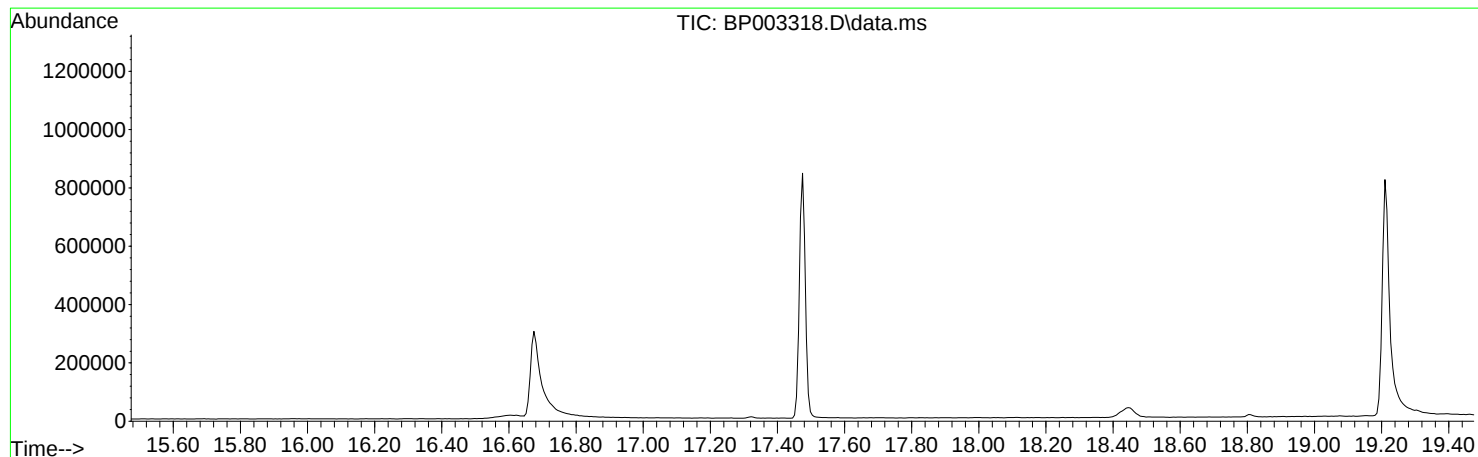

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	19189	PASS
68	69	0.00	2	1.8	453	PASS
69	198	0.00	100	29.8	25542	PASS
70	69	0.00	2	0.8	204	PASS
127	198	10	80	44.6	38229	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85771	PASS
199	198	5	9	6.7	5758	PASS
275	198	10	60	28.6	24488	PASS
365	198	1	100	3.8	3263	PASS
441	198	0.01	100	11.9	10218	PASS
442	198	50	100	77.4	66360	PASS
443	442	15	24	19.1	12681	PASS