
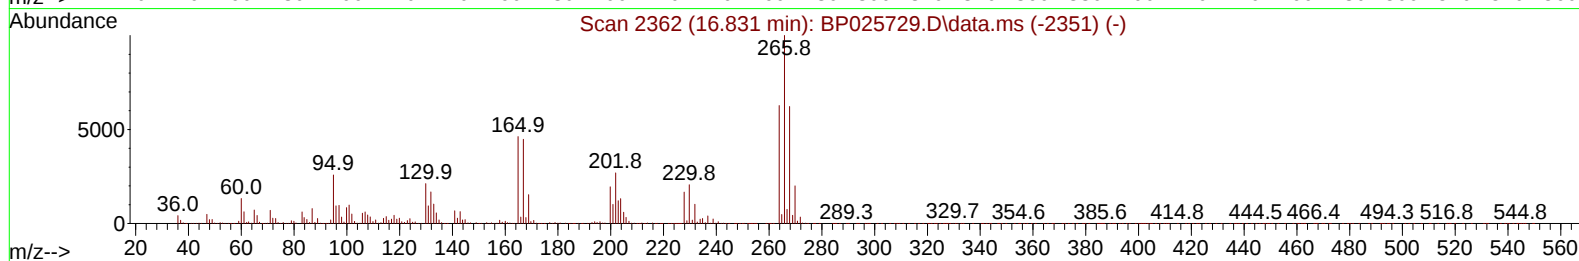
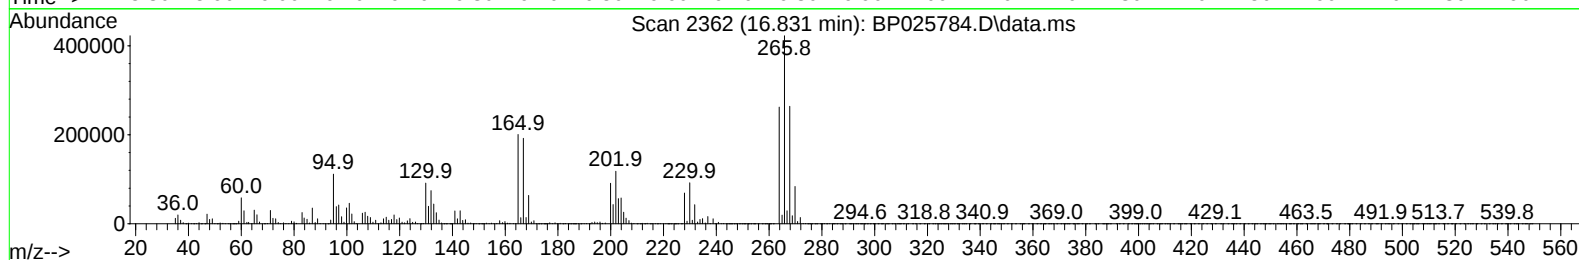


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025784.D
Acq On : 18 Sep 2025 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 18:21:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

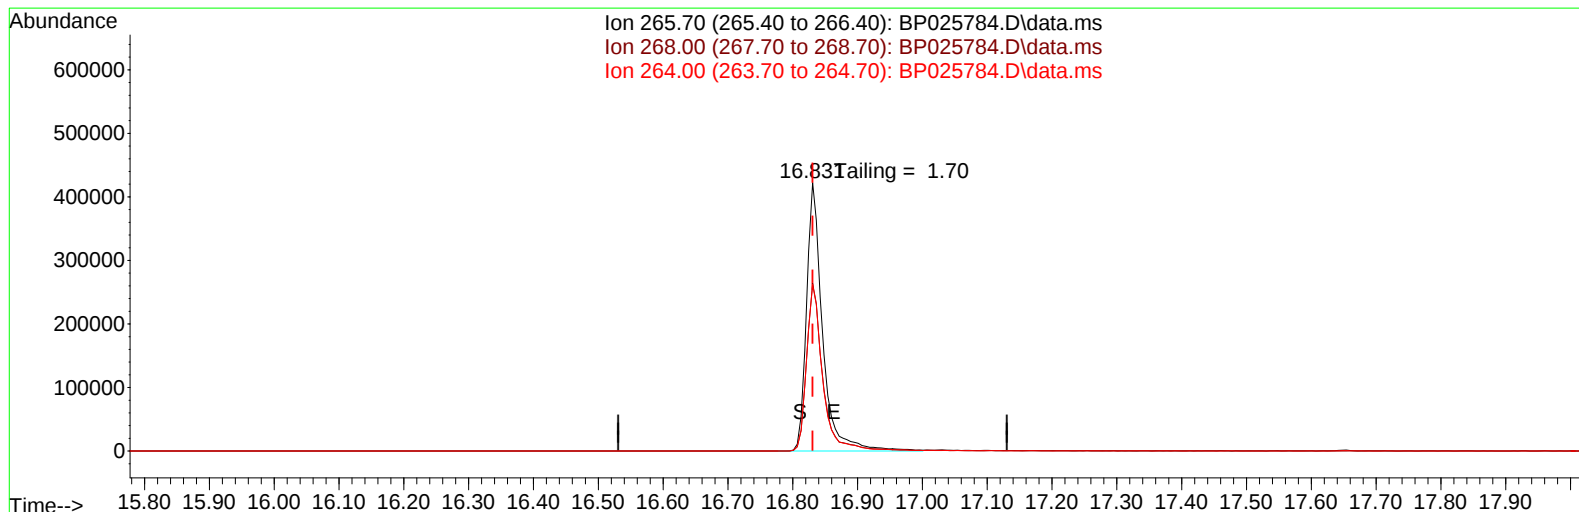

TIC: BP025784.D\data.ms

(70) Pentachlorophenol (C)




16.831min (-0.000) 11114.00 ng

response 729339

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.43
264.00	62.70	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025784.D
Acq On : 18 Sep 2025 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 18:21:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

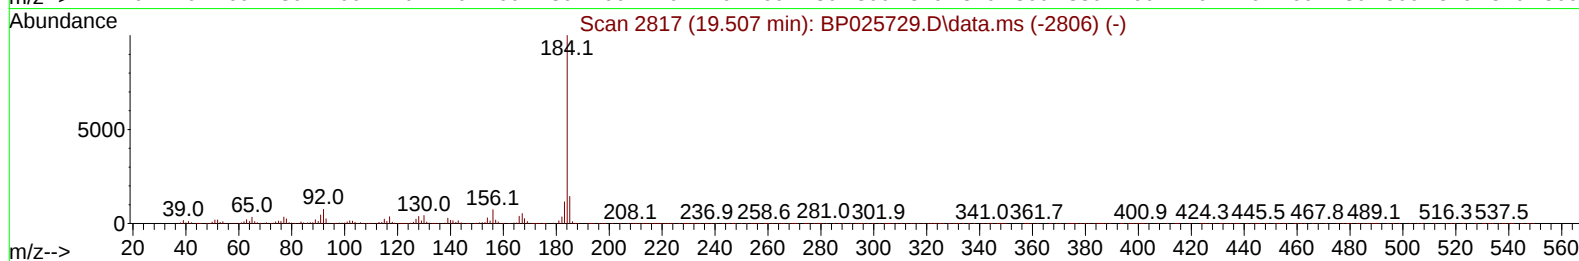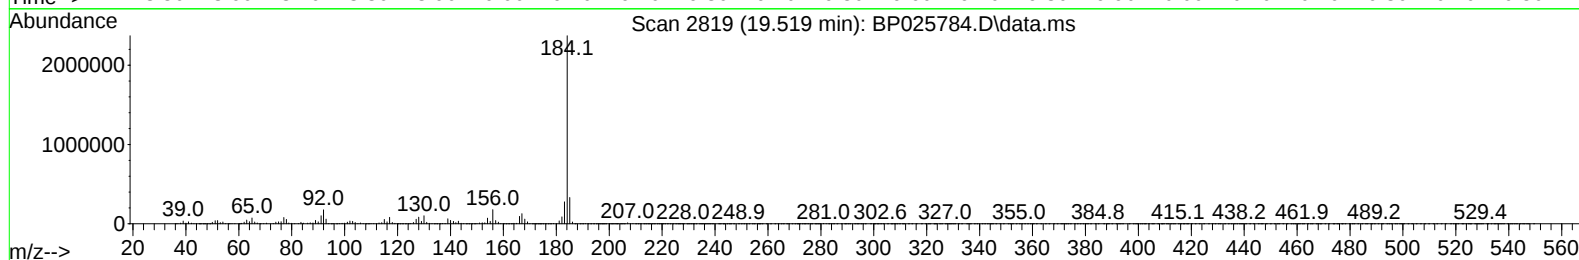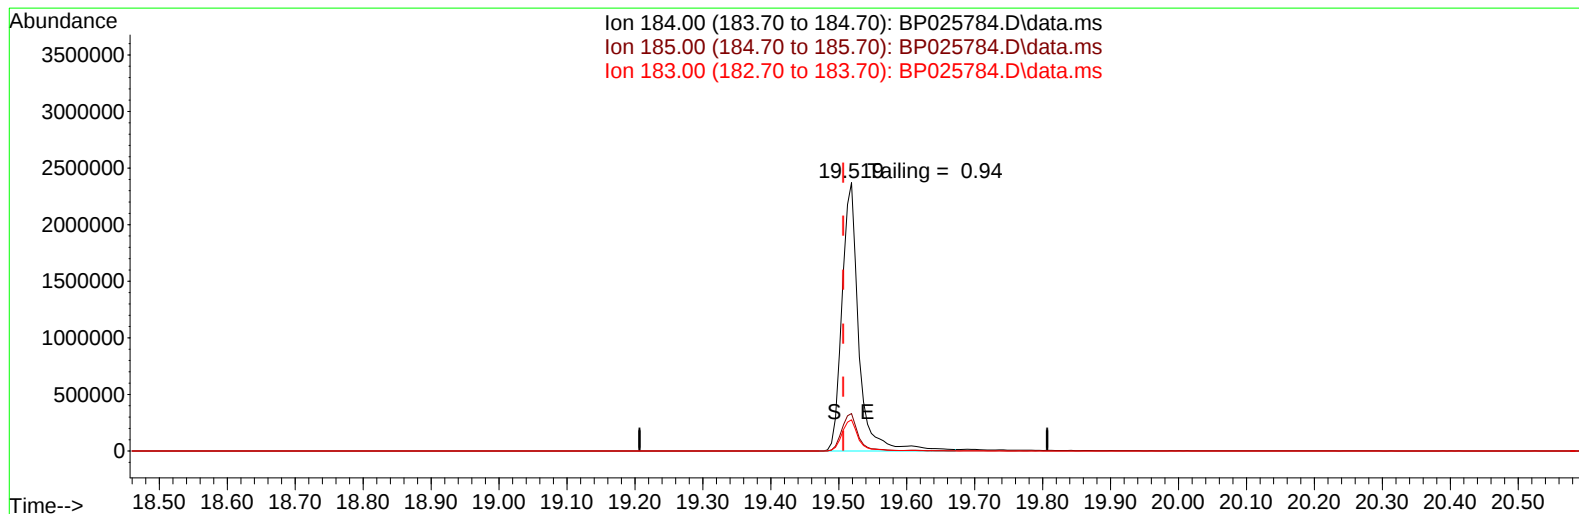

TIC: BP025784.D\data.ms

(77) Benzidine**19.519min (+ 0.012) 12920.41 ng****response 3968149**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	11.50	11.62
0.00	0.00	0.00