

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025788.D
Acq On : 18 Sep 2025 19:28
Operator : CG/JU
Sample : PB169718BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169718BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.378	409	415	434	rBV	1949203	3121997	31.88%	8.199%
2	6.943	671	681	718	rBV	1578109	3065408	31.30%	8.050%
3	7.748	811	818	832	rBV	556261	947940	9.68%	2.490%
4	8.895	1005	1013	1033	rBV	1542811	3041294	31.05%	7.987%
5	10.519	1282	1289	1311	rBV	526796	1226929	12.53%	3.222%
6	12.989	1700	1709	1735	rBV	3841795	6476916	66.13%	17.010%
7	14.383	1939	1946	1968	rBV	785415	1566370	15.99%	4.114%
8	15.901	2197	2204	2227	rBV2	1383507	2974201	30.37%	7.811%
9	17.189	2414	2423	2436	rBV2	974816	1820790	18.59%	4.782%
10	19.907	2878	2885	2897	rBV	6945296	9793697	100.00%	25.721%
11	21.642	3173	3180	3192	rBV2	1068477	2152532	21.98%	5.653%
12	25.000	3743	3751	3769	rVB2	588295	1889225	19.29%	4.962%




Sum of corrected areas: 38077299

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025788.D
Acq On : 18 Sep 2025 19:28
Operator : CG/JU
Sample : PB169718BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169718BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

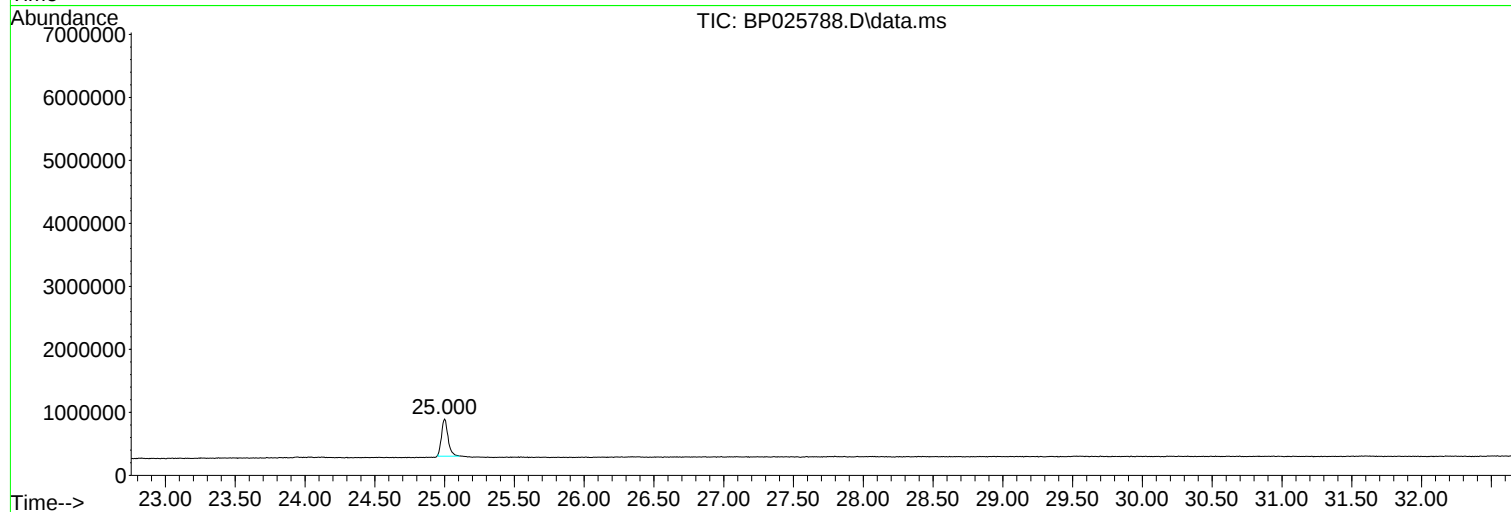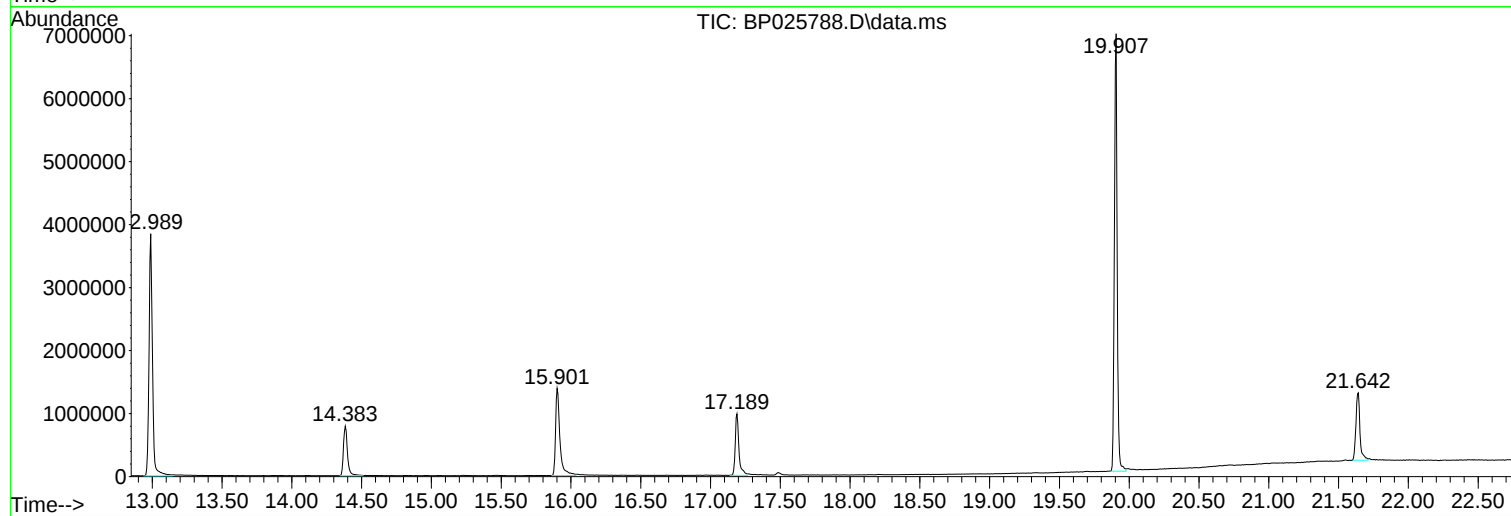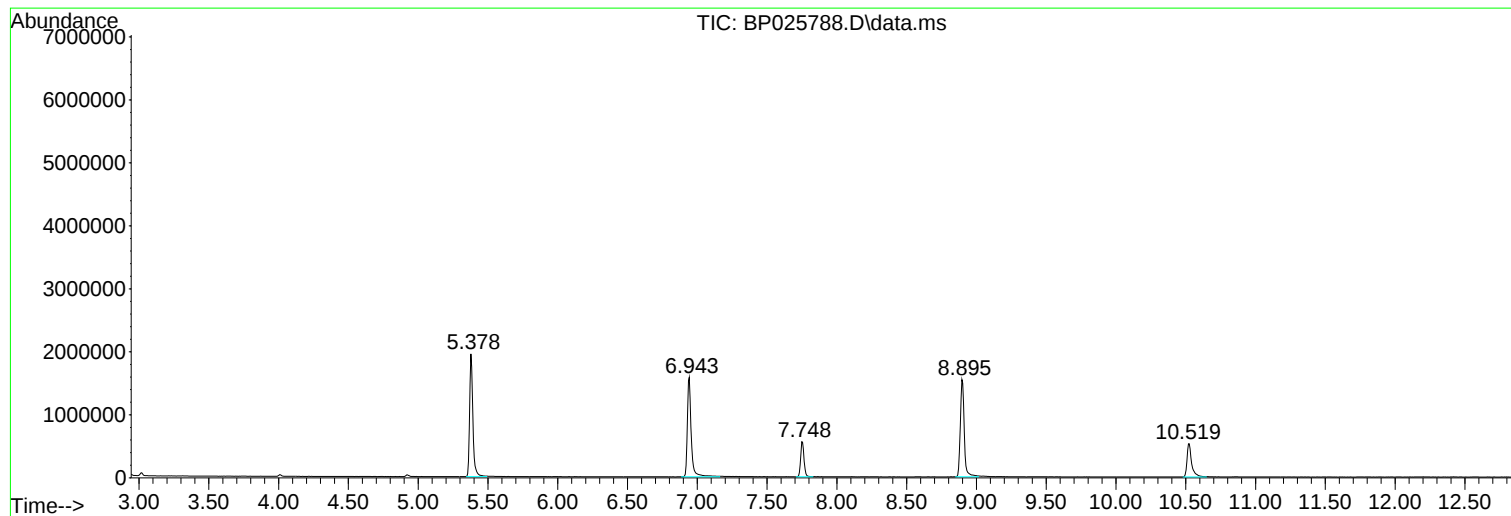

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025788.D
Acq On : 18 Sep 2025 19:28
Operator : CG/JU
Sample : PB169718BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169718BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025788.D
Acq On : 18 Sep 2025 19:28
Operator : CG/JU
Sample : PB169718BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169718BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------