
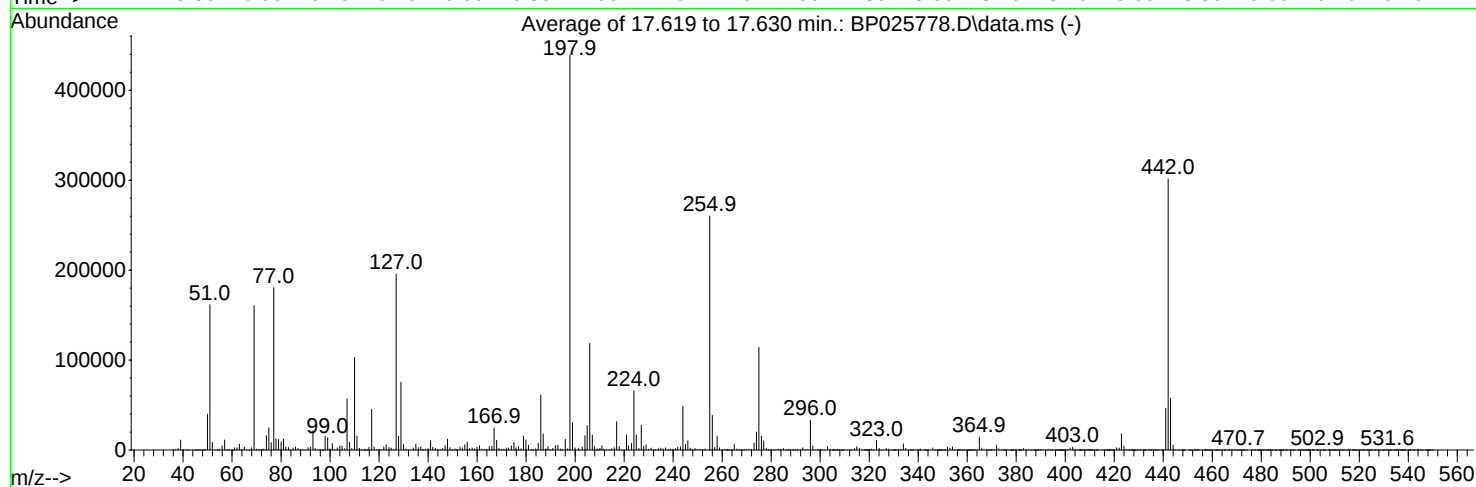


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025778.D
Acq On : 18 Sep 2025 08:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

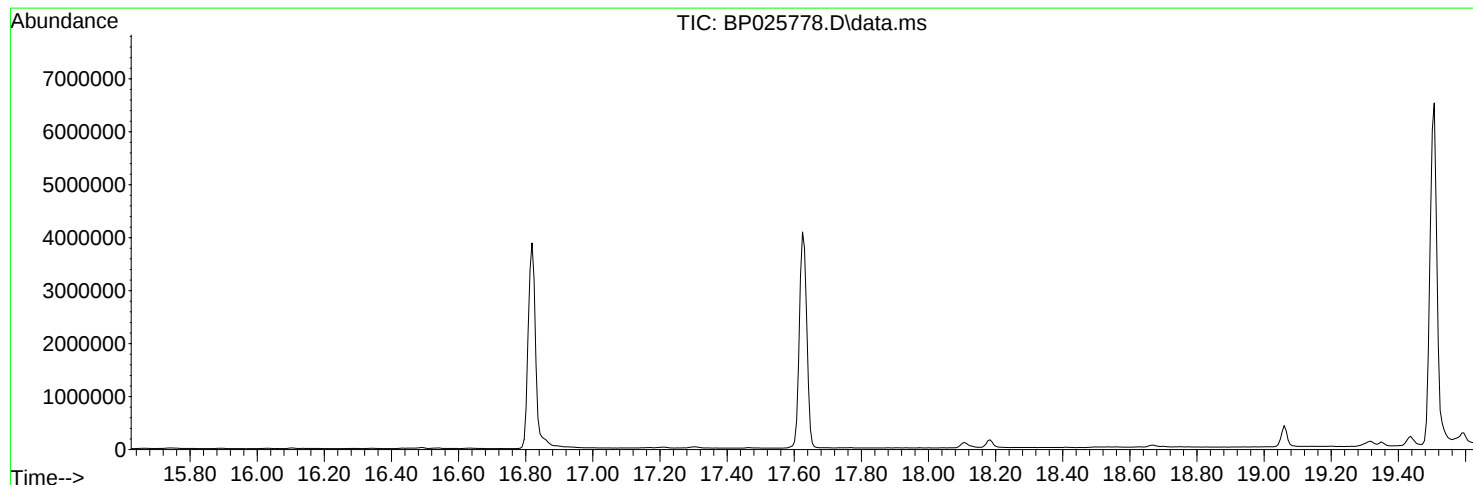




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2540	PASS
69	69	100	100	100.0	160686	PASS
70	69	0.00	2	0.5	874	PASS
197	198	0.00	2	0.3	1514	PASS
198	198	100	100	100.0	438981	PASS
199	198	5	9	6.9	30400	PASS
365	198	1	100	3.3	14496	PASS
441	443	0.01	150	80.4	46240	PASS
442	442	100	100	100.0	301480	PASS
443	442	15	24	19.1	57499	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025778.D
Acq On : 18 Sep 2025 08:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 18 11:27:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

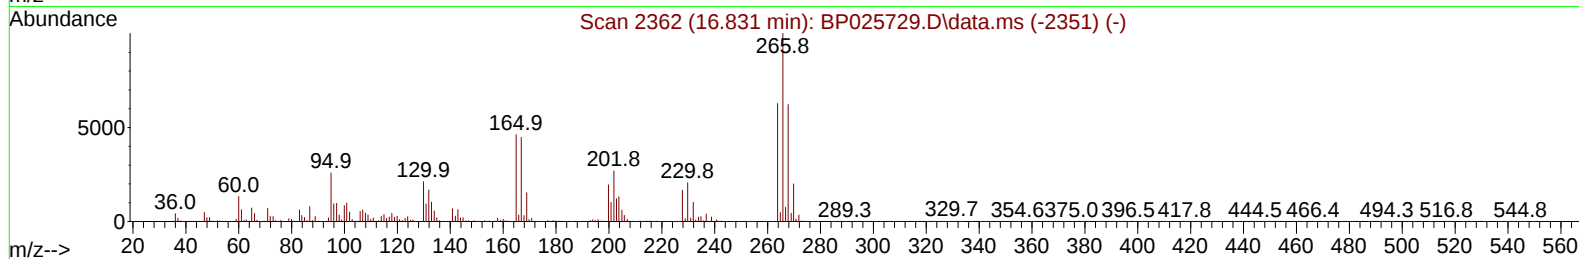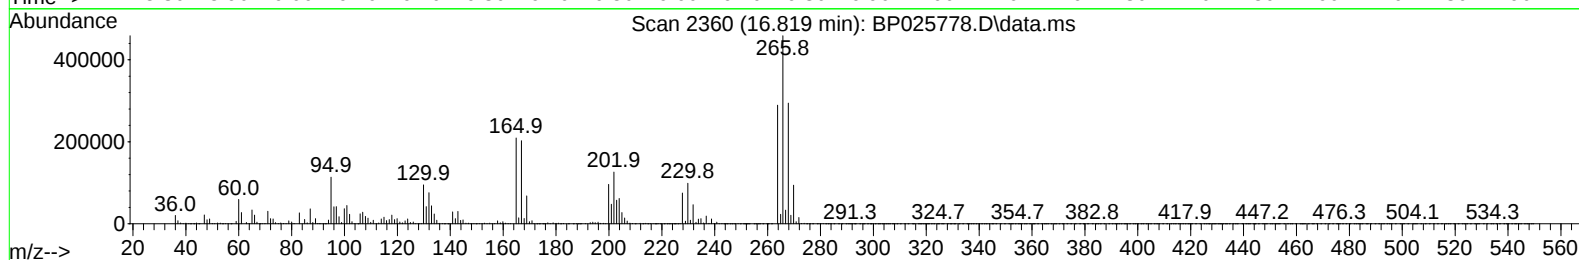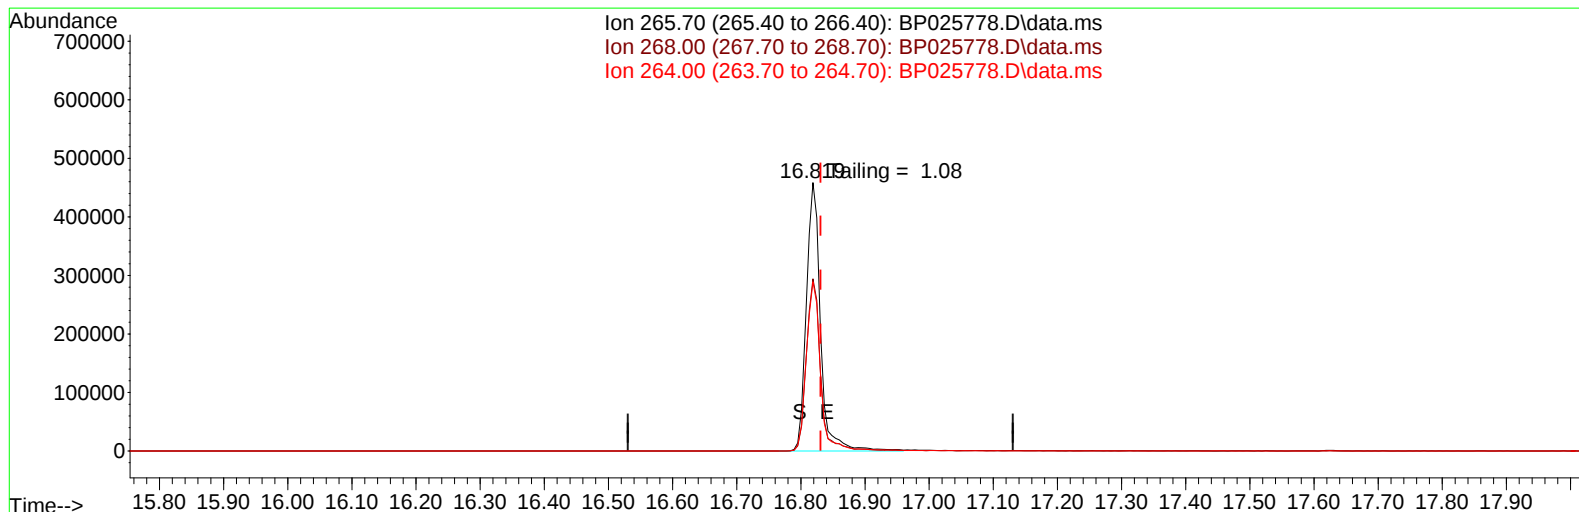

TIC: BP025778.D\data.ms

(70) Pentachlorophenol (C)

16.819min (-0.012) 11531.73 ng




response 710131

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.16
264.00	62.70	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025778.D
Acq On : 18 Sep 2025 08:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 18 11:27:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

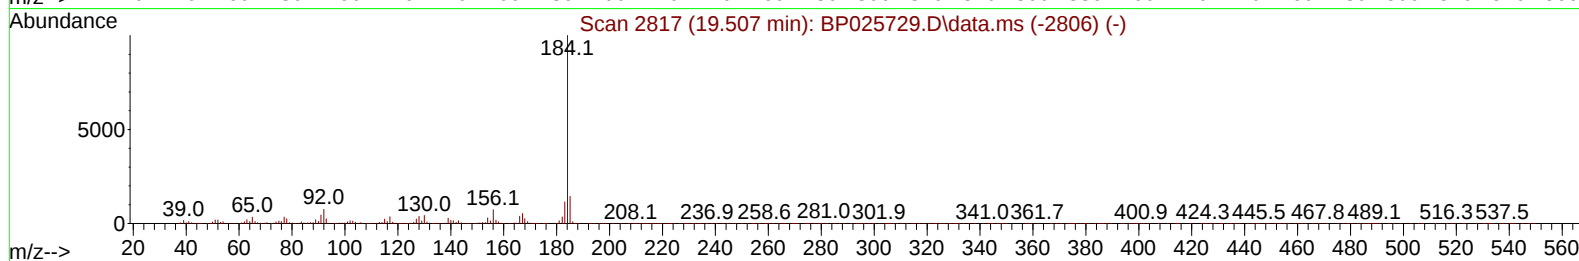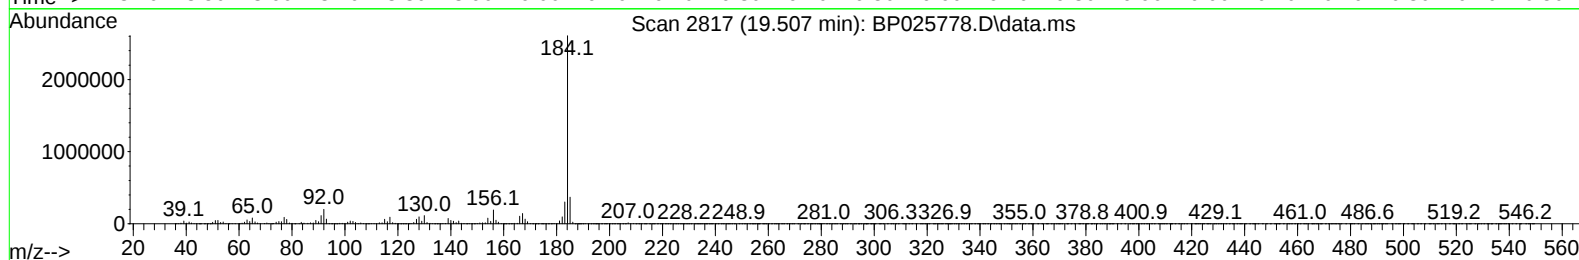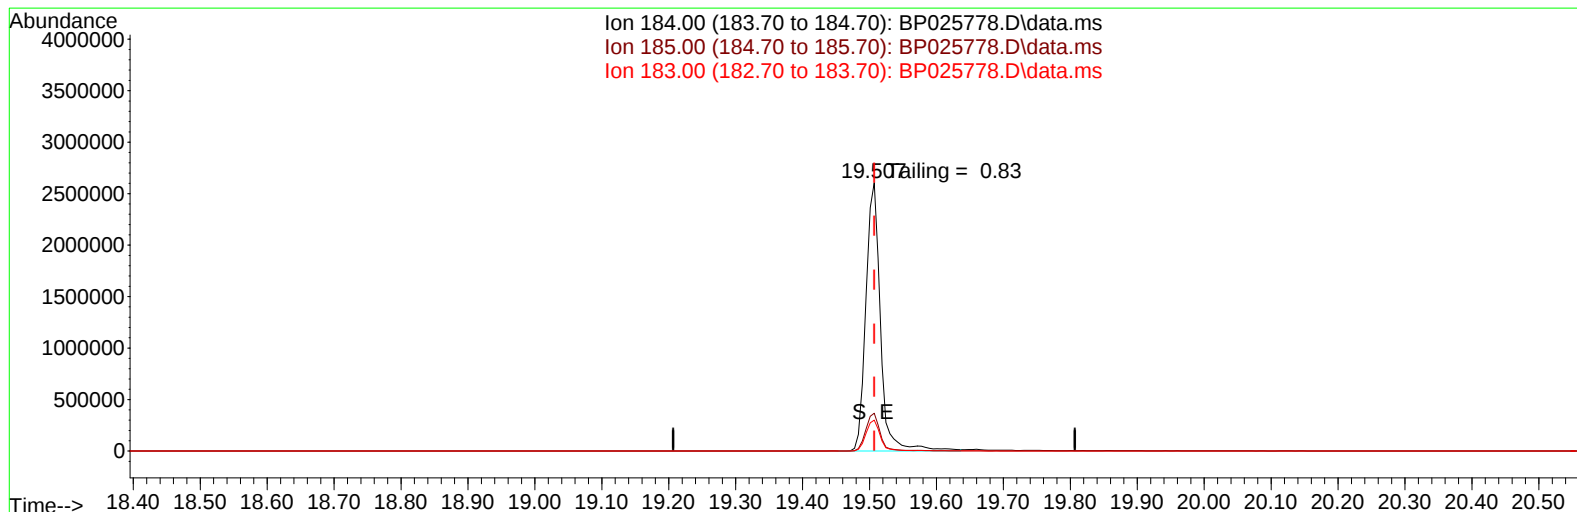

TIC: BP025778.D\data.ms

(77) Benzidine

19.507min (-0.000) 3522.69 ng

response 3834137

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.09
183.00	11.50	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2025	BNA_P	<u>BP025778.D</u>
Compound Name	Response	Retention Time
DDT	2077125	20.795
DDD	37894	20.336
DDE	5667	19.801
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43561	2120686	2.05

Instrument :
BNA_P
ClientSampleId :
DFTPP