
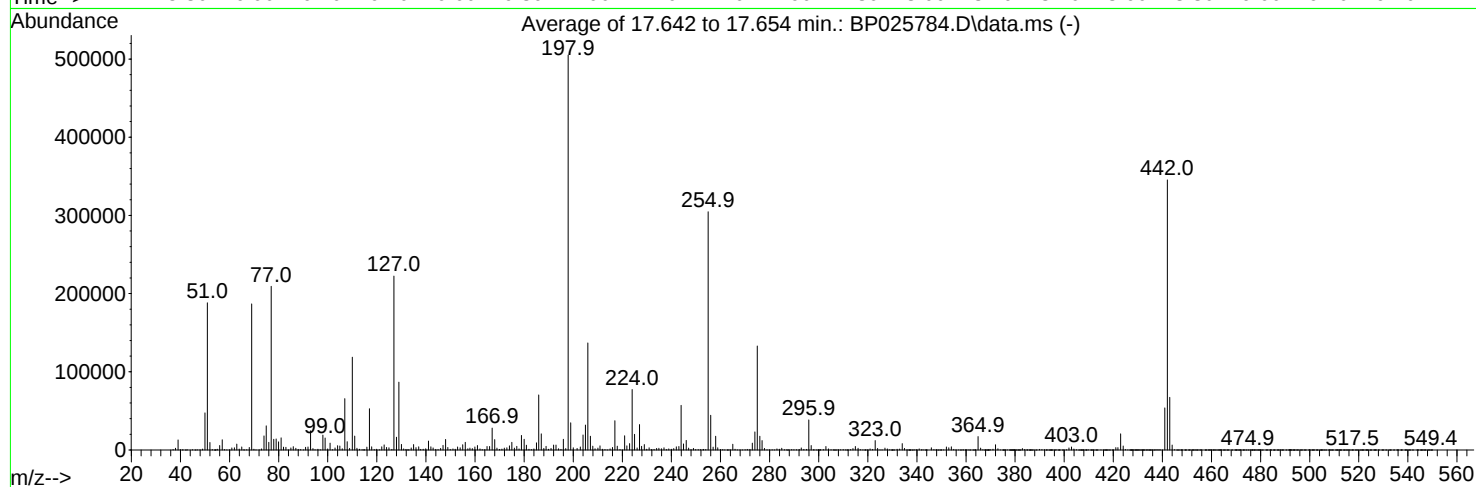


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025784.D
Acq On : 18 Sep 2025 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

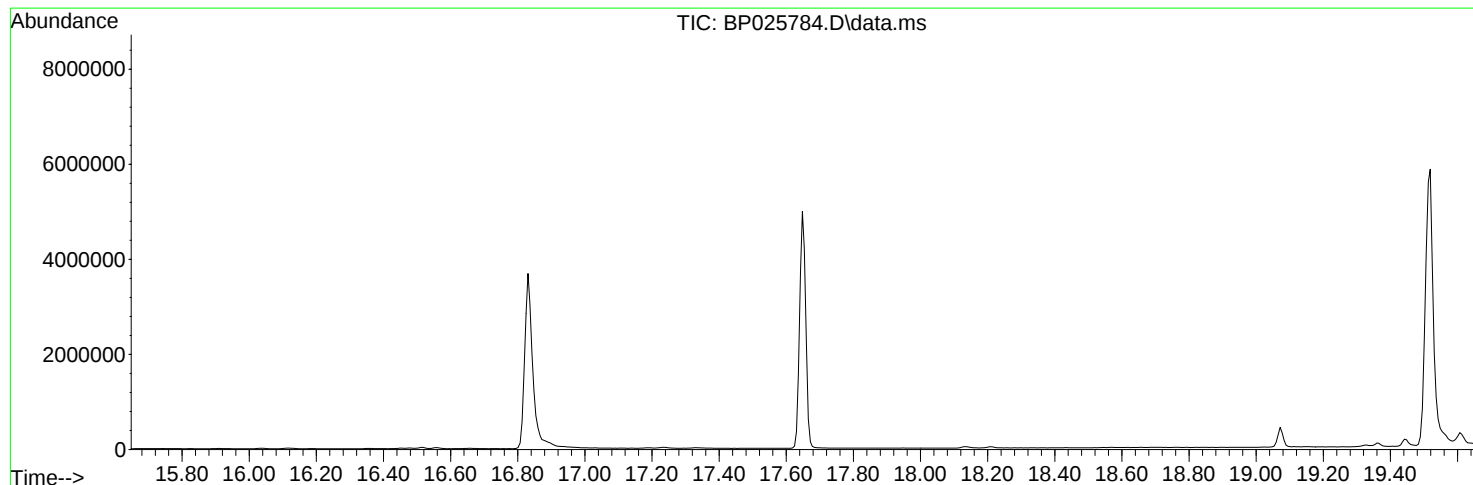




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2488

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3125	PASS
69	69	100	100	100.0	186779	PASS
70	69	0.00	2	0.5	918	PASS
197	198	0.00	2	0.4	1837	PASS
198	198	100	100	100.0	505058	PASS
199	198	5	9	6.9	34667	PASS
365	198	1	100	3.4	17024	PASS
441	443	0.01	150	79.8	53688	PASS
442	442	100	100	100.0	345451	PASS
443	442	15	24	19.5	67317	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025784.D
Acq On : 18 Sep 2025 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 18 18:21:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

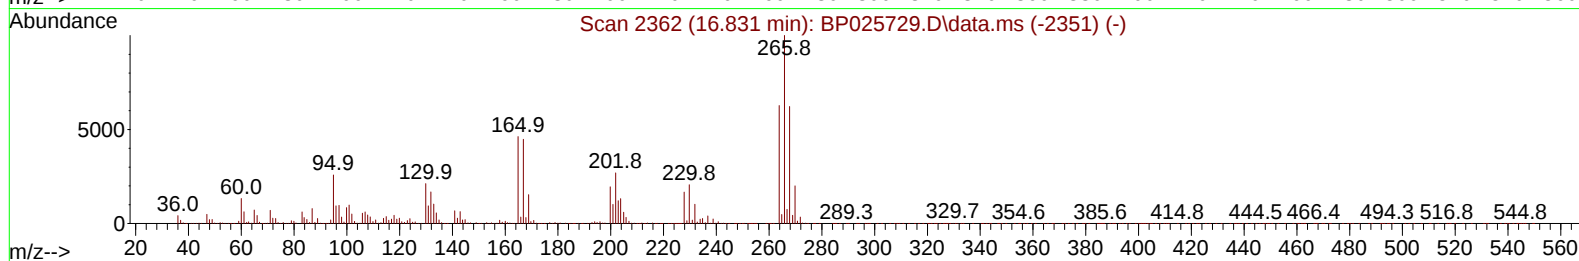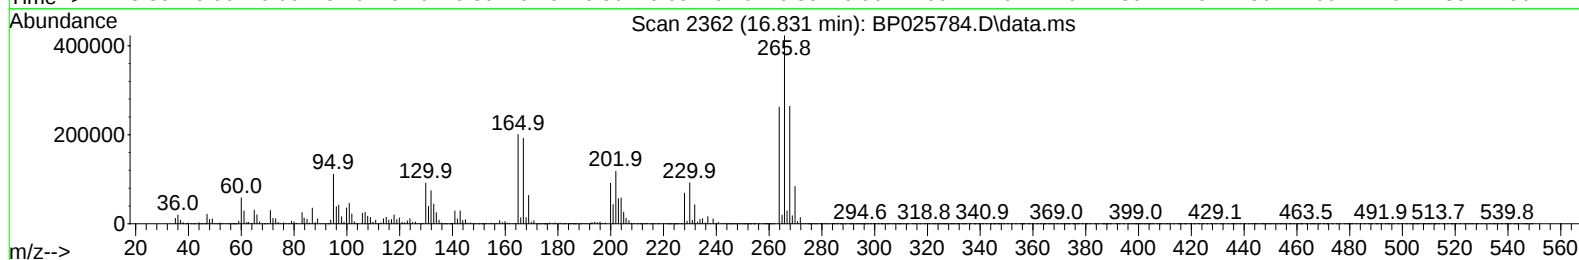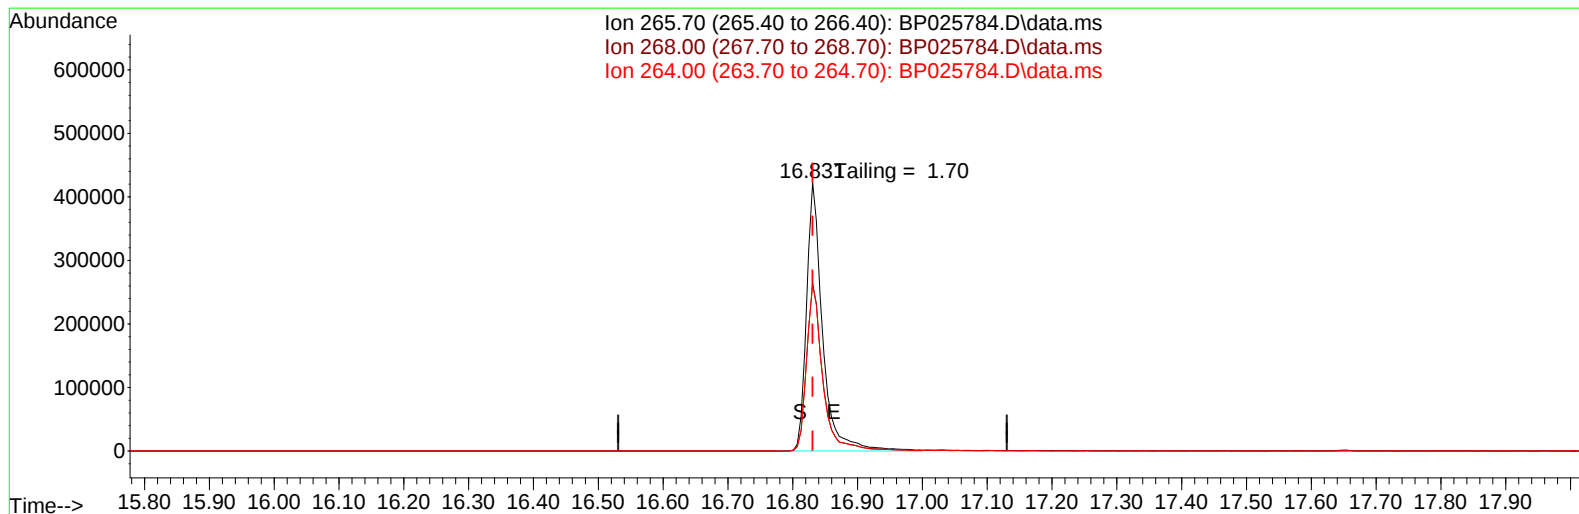

TIC: BP025784.D\data.ms

(70) Pentachlorophenol (C)

16.831min (-0.000) 11114.00 ng




response 729339

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.43
264.00	62.70	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091825\
Data File : BP025784.D
Acq On : 18 Sep 2025 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 18 18:21:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

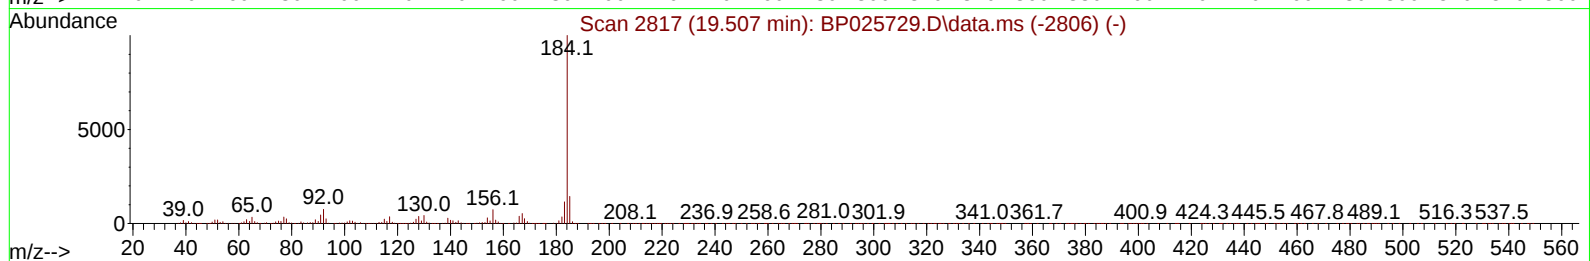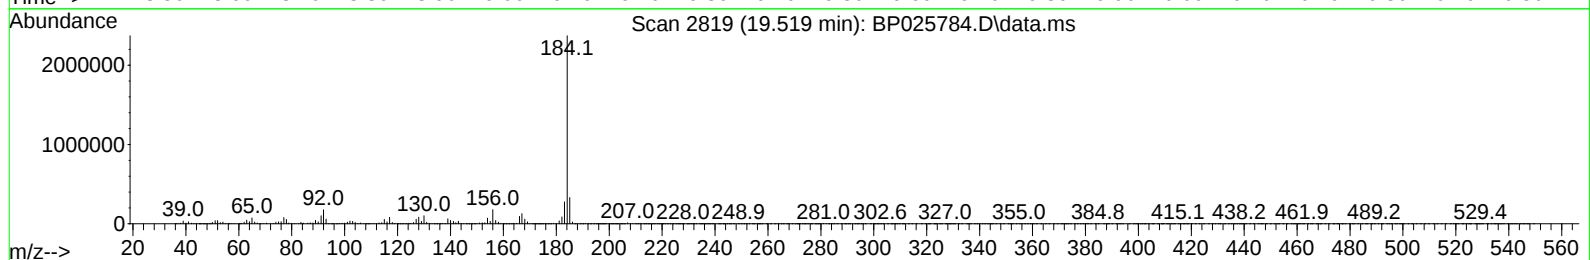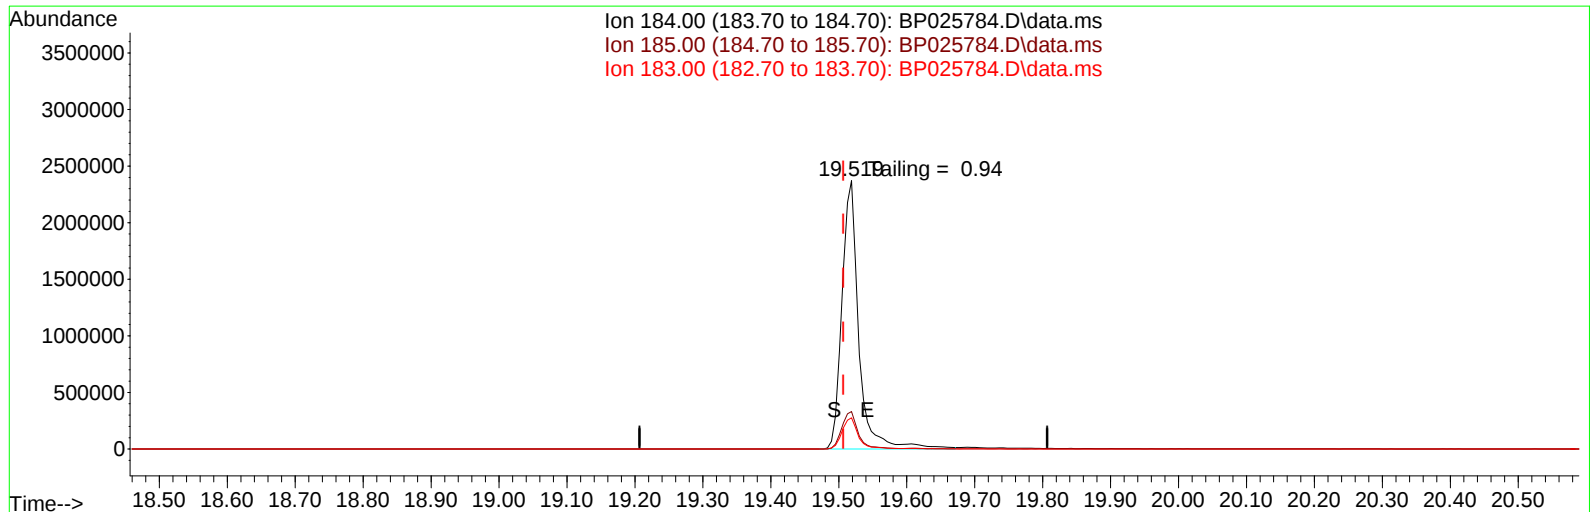

TIC: BP025784.D\data.ms

(77) Benzidine

19.519min (+ 0.012) 12920.41 ng

response 3968149

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	11.50	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2025	BNA_P	<u>BP025784.D</u>
Compound Name	Response	Retention Time
DDT	2084306	20.807
DDD	38082	20.348
DDE	1142	19.072
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39224	2123530	1.85

Instrument :
BNA_P
ClientSampleId :
DFTPP