
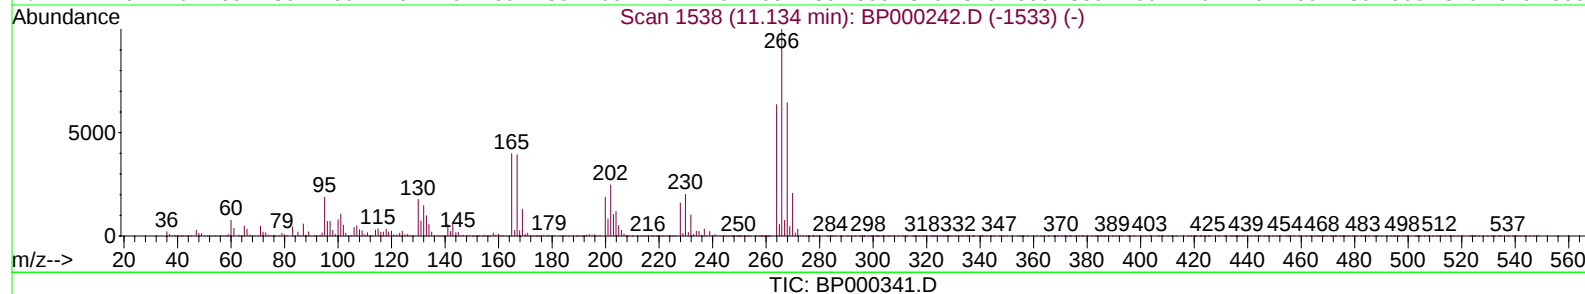
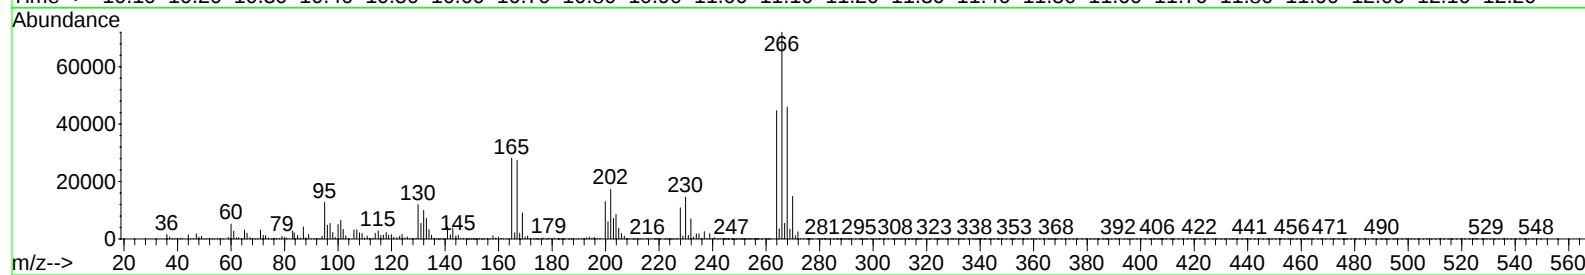


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP092019\
Data File : BP000341.D
Acq On : 20 Sep 2019 08:22
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 19:11:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 19 14:44:51 2019
Response via : Initial Calibration

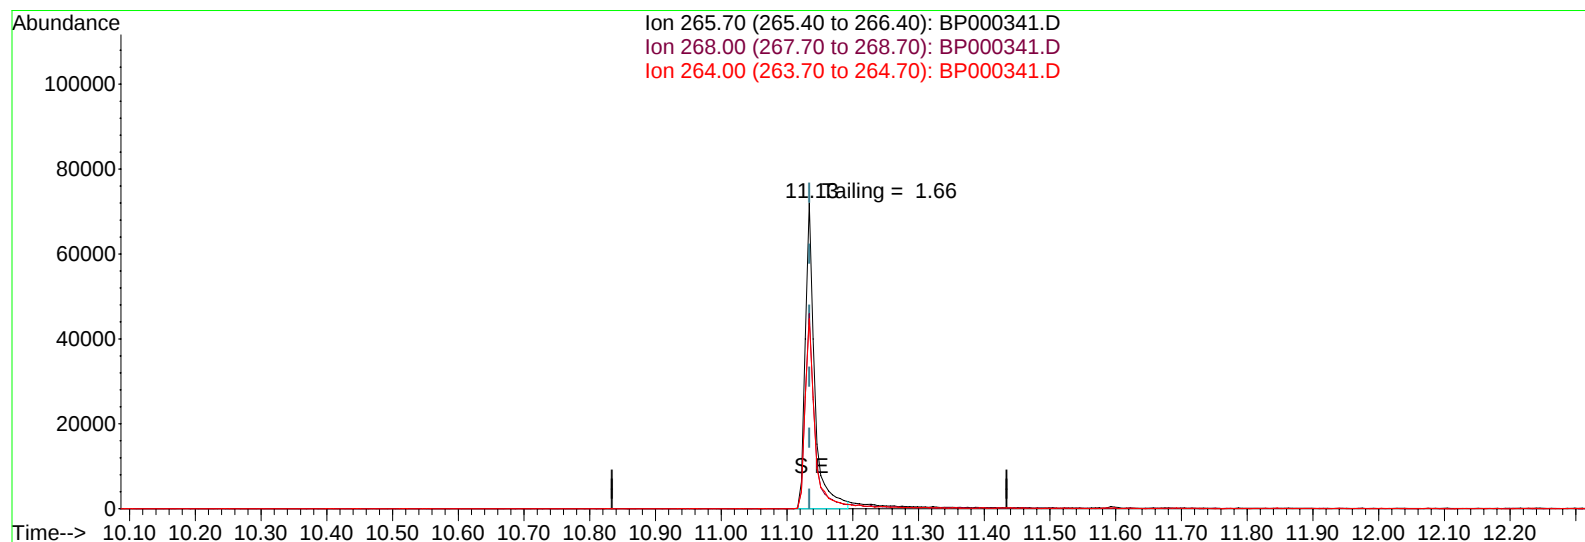

(70) Pentachlorophenol (C)




11.134min (-0.000) 66548.38ng

response 77069

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	63.77
264.00	63.50	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP092019\
 Data File : BP000341.D
 Acq On : 20 Sep 2019 08:22
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 19:11:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 19 14:44:51 2019
 Response via : Initial Calibration

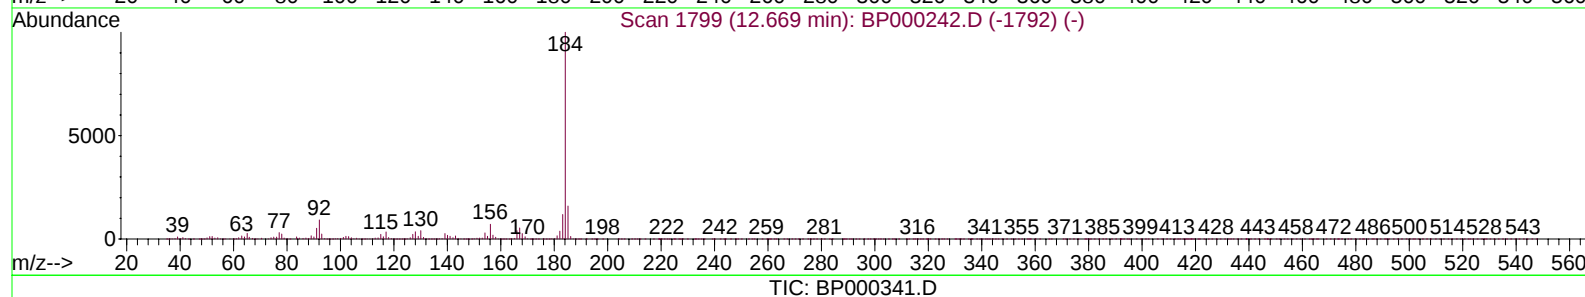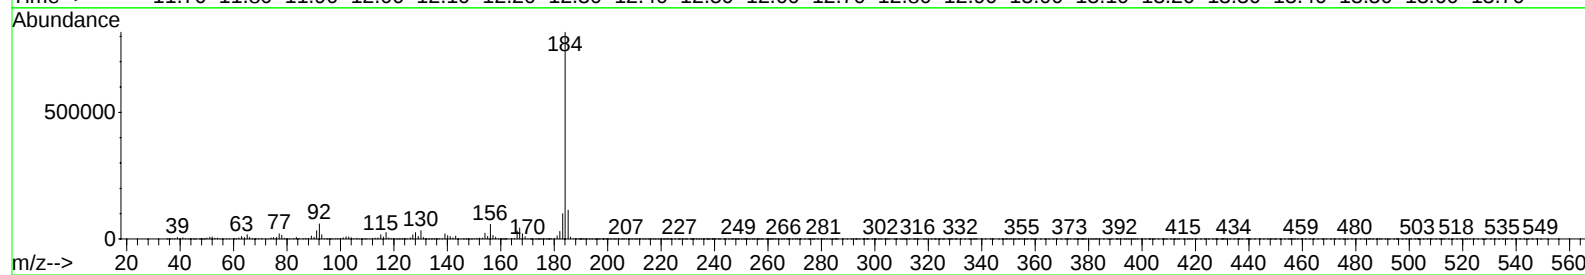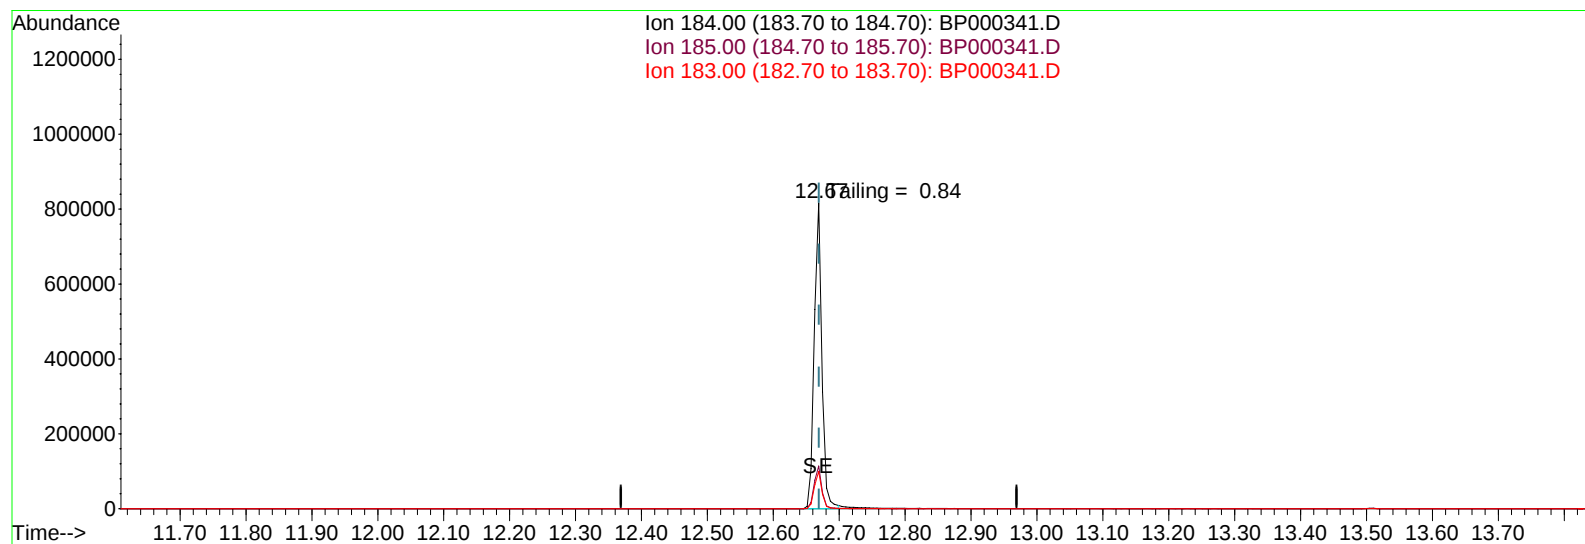

(77) Benzidine

12.669min (-0.000) 41008.05ng

response 676631

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	13.96
183.00	11.90	12.22
0.00	0.00	0.00