

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP092019\
 Data File : BP000344.D
 Acq On : 20 Sep 2019 09:52
 Operator : HP/JU
 Sample : PB123227BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB123227BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	562	567	570	rBV	4966691	4862243	53.11%	8.416%
2	6.428	733	738	741	rBV	4685481	4972734	54.32%	8.607%
3	6.563	757	761	764	rBV	5601556	5288442	57.77%	9.154%
4	6.792	796	800	803	rBV	1832234	1419856	15.51%	2.458%
5	6.951	823	827	830	rBV	5581554	4628907	50.56%	8.012%
6	7.351	890	895	898	rBV	3683693	3259434	35.61%	5.642%
7	8.075	1014	1018	1021	rBV	2292552	1800199	19.66%	3.116%
8	9.157	1197	1202	1205	rBV	8077484	7607635	83.10%	13.168%
9	9.833	1313	1317	1321	rBV	2601149	2288574	25.00%	3.961%
10	10.633	1448	1453	1456	rBV	4767300	4600391	50.25%	7.963%
11	11.333	1568	1572	1575	rBV	2522679	2286818	24.98%	3.958%
12	12.939	1840	1845	1848	rBV	9268214	9154413	100.00%	15.845%
13	13.998	2020	2025	2028	rBV	2768594	2482911	27.12%	4.298%
14	15.139	2215	2219	2229	rVB	83088	95289	1.04%	0.165%
15	15.480	2271	2277	2282	rVV	2208750	2673895	29.21%	4.628%
16	15.527	2282	2285	2294	rVB	101845	133132	1.45%	0.230%
17	15.980	2357	2362	2369	rVB	77600	123307	1.35%	0.213%
18	16.498	2445	2450	2457	rBV2	53244	96178	1.05%	0.166%


Sum of corrected areas: 57774358

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP092019\
Data File : BP000344.D
Acq On : 20 Sep 2019 09:52
Operator : HP/JU
Sample : PB123227BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123227BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

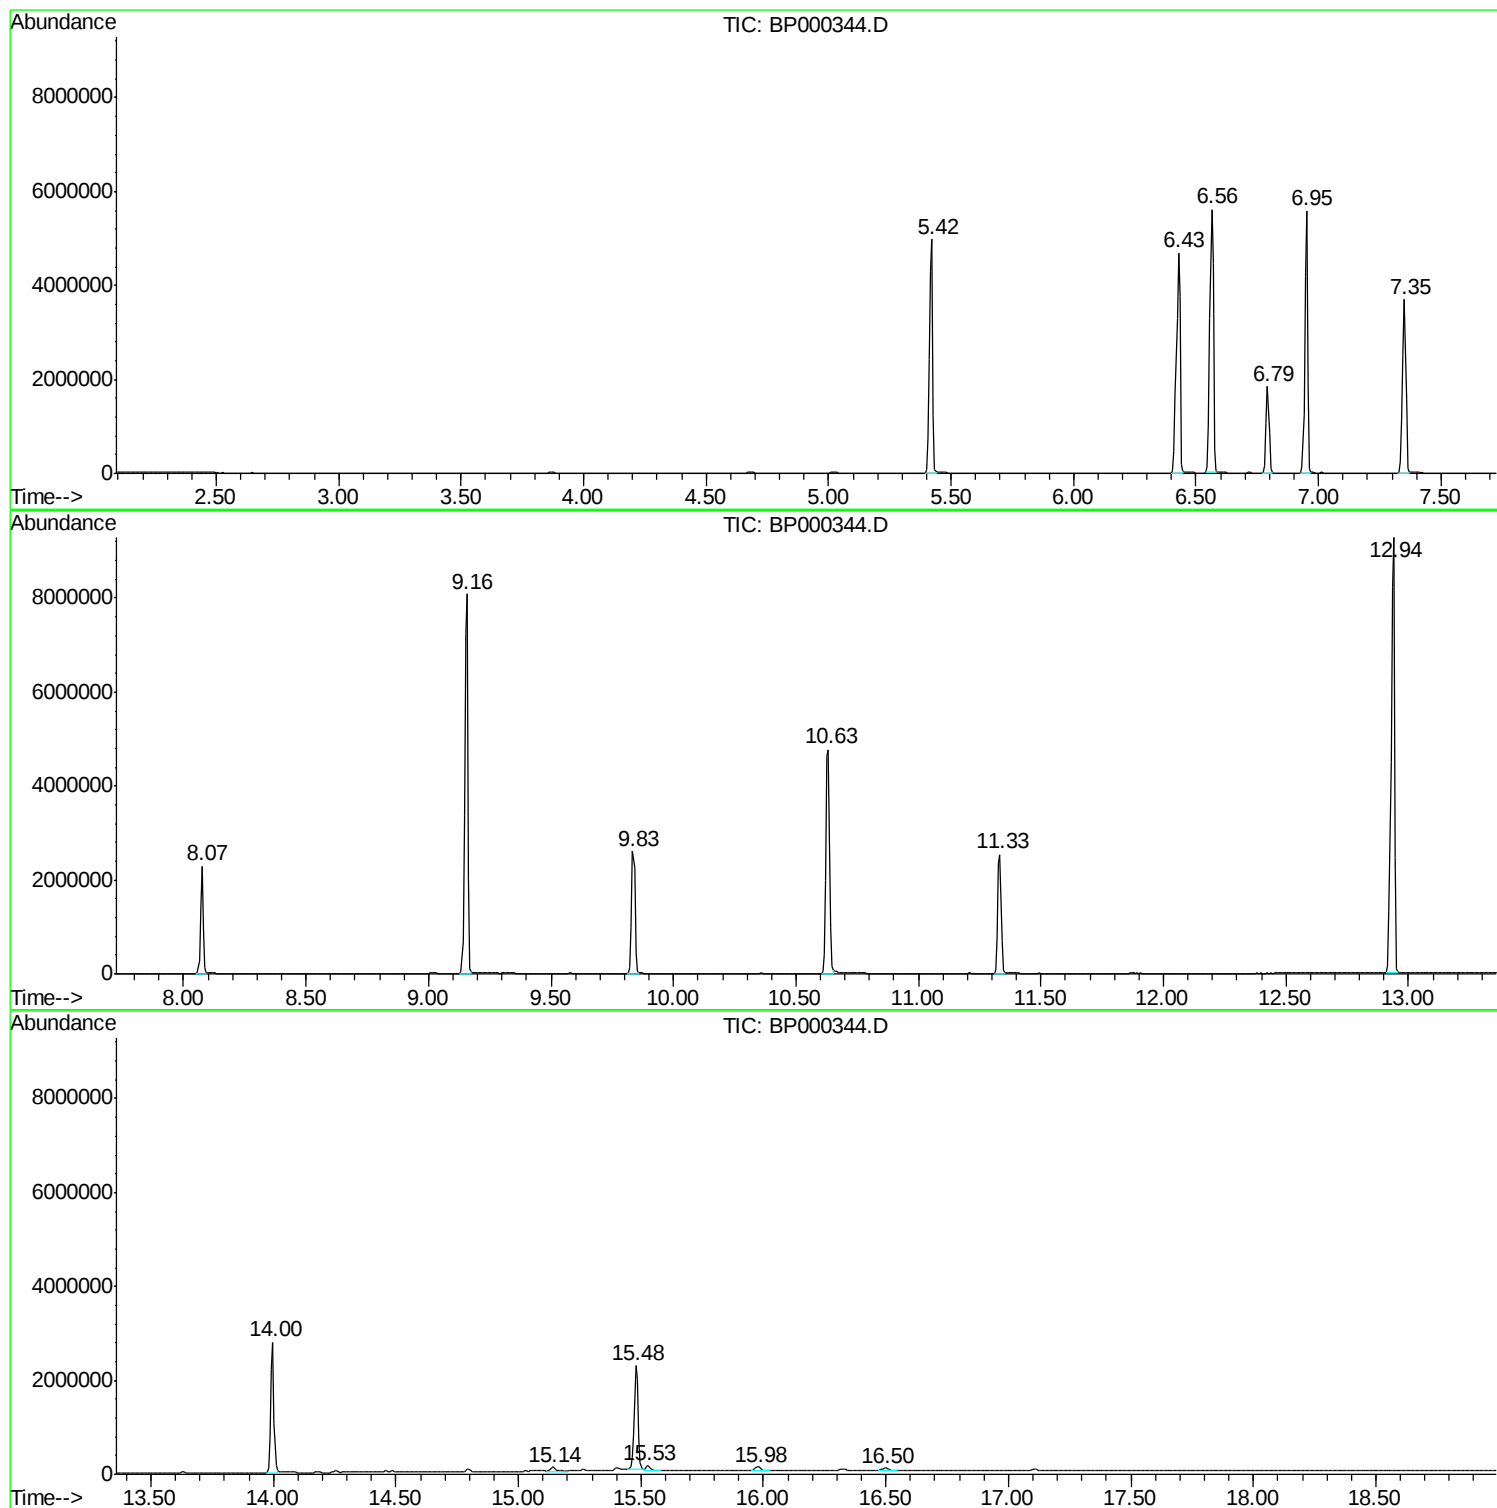

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP092019\
Data File : BP000344.D
Acq On : 20 Sep 2019 09:52
Operator : HP/JU
Sample : PB123227BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123227BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.56 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	74.49 ng	5288440	1,4-Dichlorobenzene-d4	6.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3	Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2	(E)-3	Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3	1H	Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
4	4	Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5	5	Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

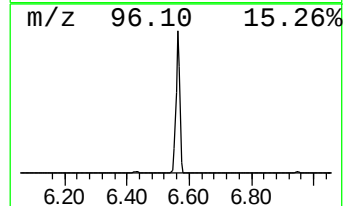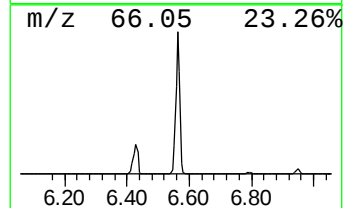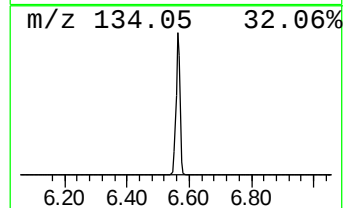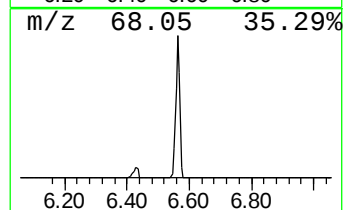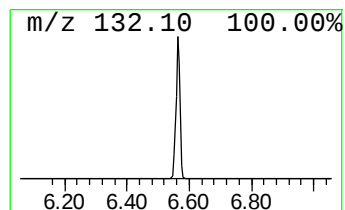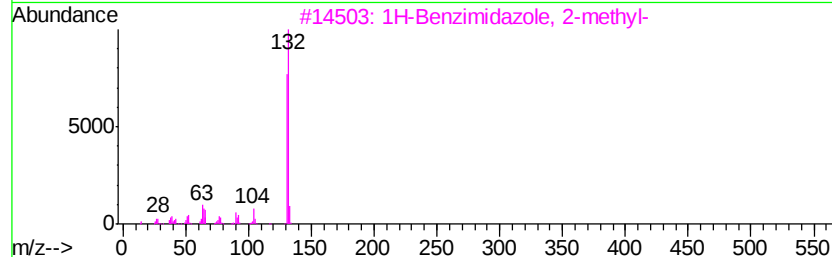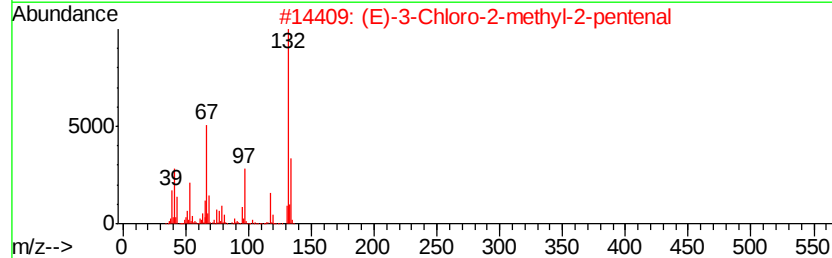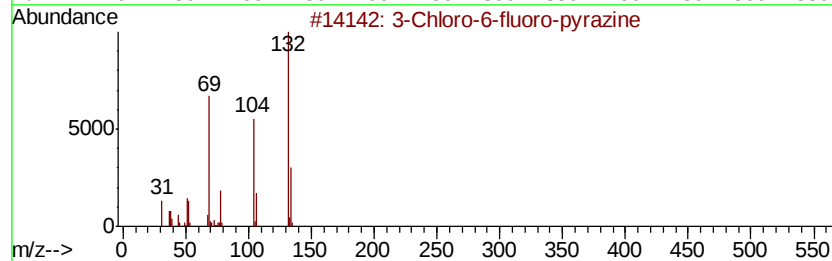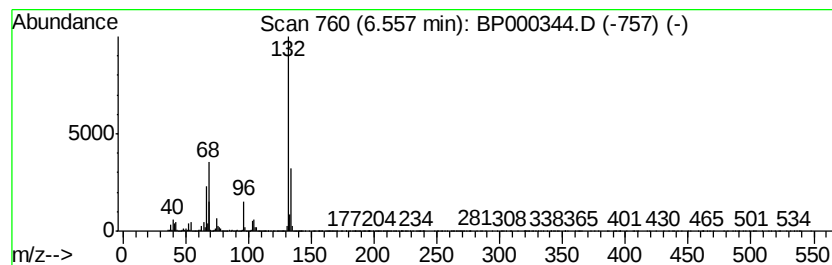

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP092019\
Data File : BP000344.D
Acq On : 20 Sep 2019 09:52
Operator : HP/JU
Sample : PB123227BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123227BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.56	6.56	74.5	ng	5288440	1	6.79	1419860	20.0