


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP092019\
 Data File : BP000341.D
 Acq On : 20 Sep 2019 08:22
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

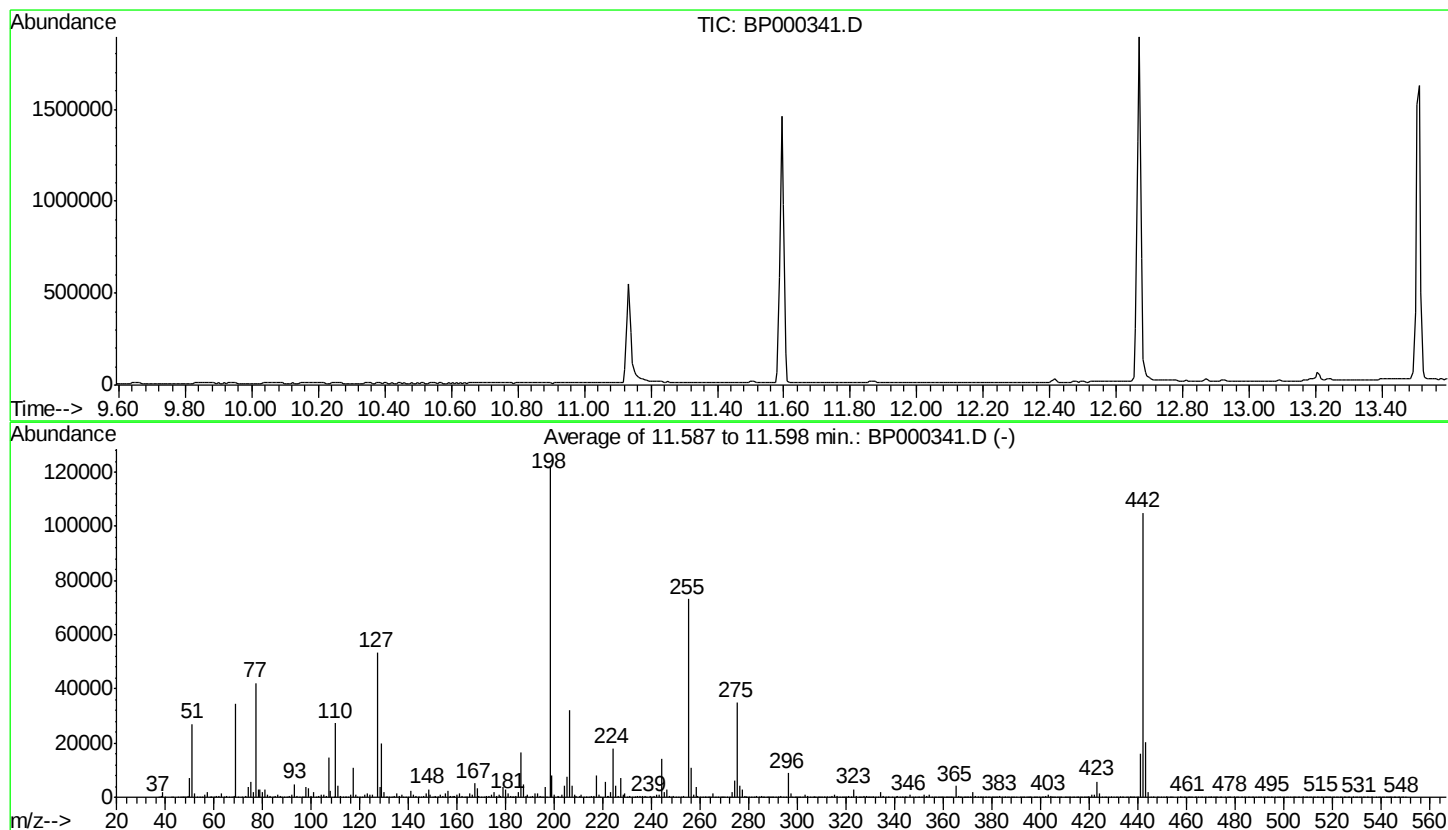

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	27125	PASS
68	69	0.00	2	0.9	321	PASS
69	198	0.00	100	28.2	34495	PASS
70	69	0.00	2	0.4	150	PASS
127	198	10	80	43.4	53200	PASS
197	198	0.00	2	0.1	170	PASS
198	198	100	100	100.0	122453	PASS
199	198	5	9	6.7	8263	PASS
275	198	10	60	28.5	34857	PASS
365	198	1	100	3.3	4081	PASS
441	198	0.01	100	13.3	16302	PASS
442	198	50	100	85.8	105065	PASS
443	442	15	24	19.4	20382	PASS