

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
 Data File : BP007056.D
 Acq On : 20 Sep 2021 18:35
 Operator : CG/JU
 Sample : M3687-36
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A002145

Quant Time: Sep 21 01:02:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 10:50:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	301584	20.000	ng	0.00
21) Naphthalene-d8	10.704	136	1146926	20.000	ng	# 0.00
39) Acenaphthene-d10	14.534	164	715079	20.000	ng	0.00
64) Phenanthrene-d10	17.281	188	1536888	20.000	ng	# 0.00
76) Chrysene-d12	21.363	240	1598138	20.000	ng	# 0.00
86) Perylene-d12	23.774	264	1654858	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	1698600	91.971	ng	0.00
7) Phenol-d6	7.069	99	2118992	84.059	ng	0.00
23) Nitrobenzene-d5	9.063	82	1219881	59.737	ng	0.00
42) 2,4,6-Tribromophenol	16.022	330	886007	103.028	ng	0.00
45) 2-Fluorobiphenyl	13.163	172	3099934	59.846	ng	0.00
79) Terphenyl-d14	19.833	244	5142741	61.740	ng	0.00
Target Compounds						
9) Benzaldehyde	7.016	77	614	Below Cal	#	41
32) Benzoic acid	9.993	122	203	6.111 ng	#	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
Data File : BP007056.D
Acq On : 20 Sep 2021 18:35
Operator : CG/JU
Sample : M3687-36
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A002145

Quant Time: Sep 21 01:02:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 17 10:50:16 2021
Response via : Initial Calibration




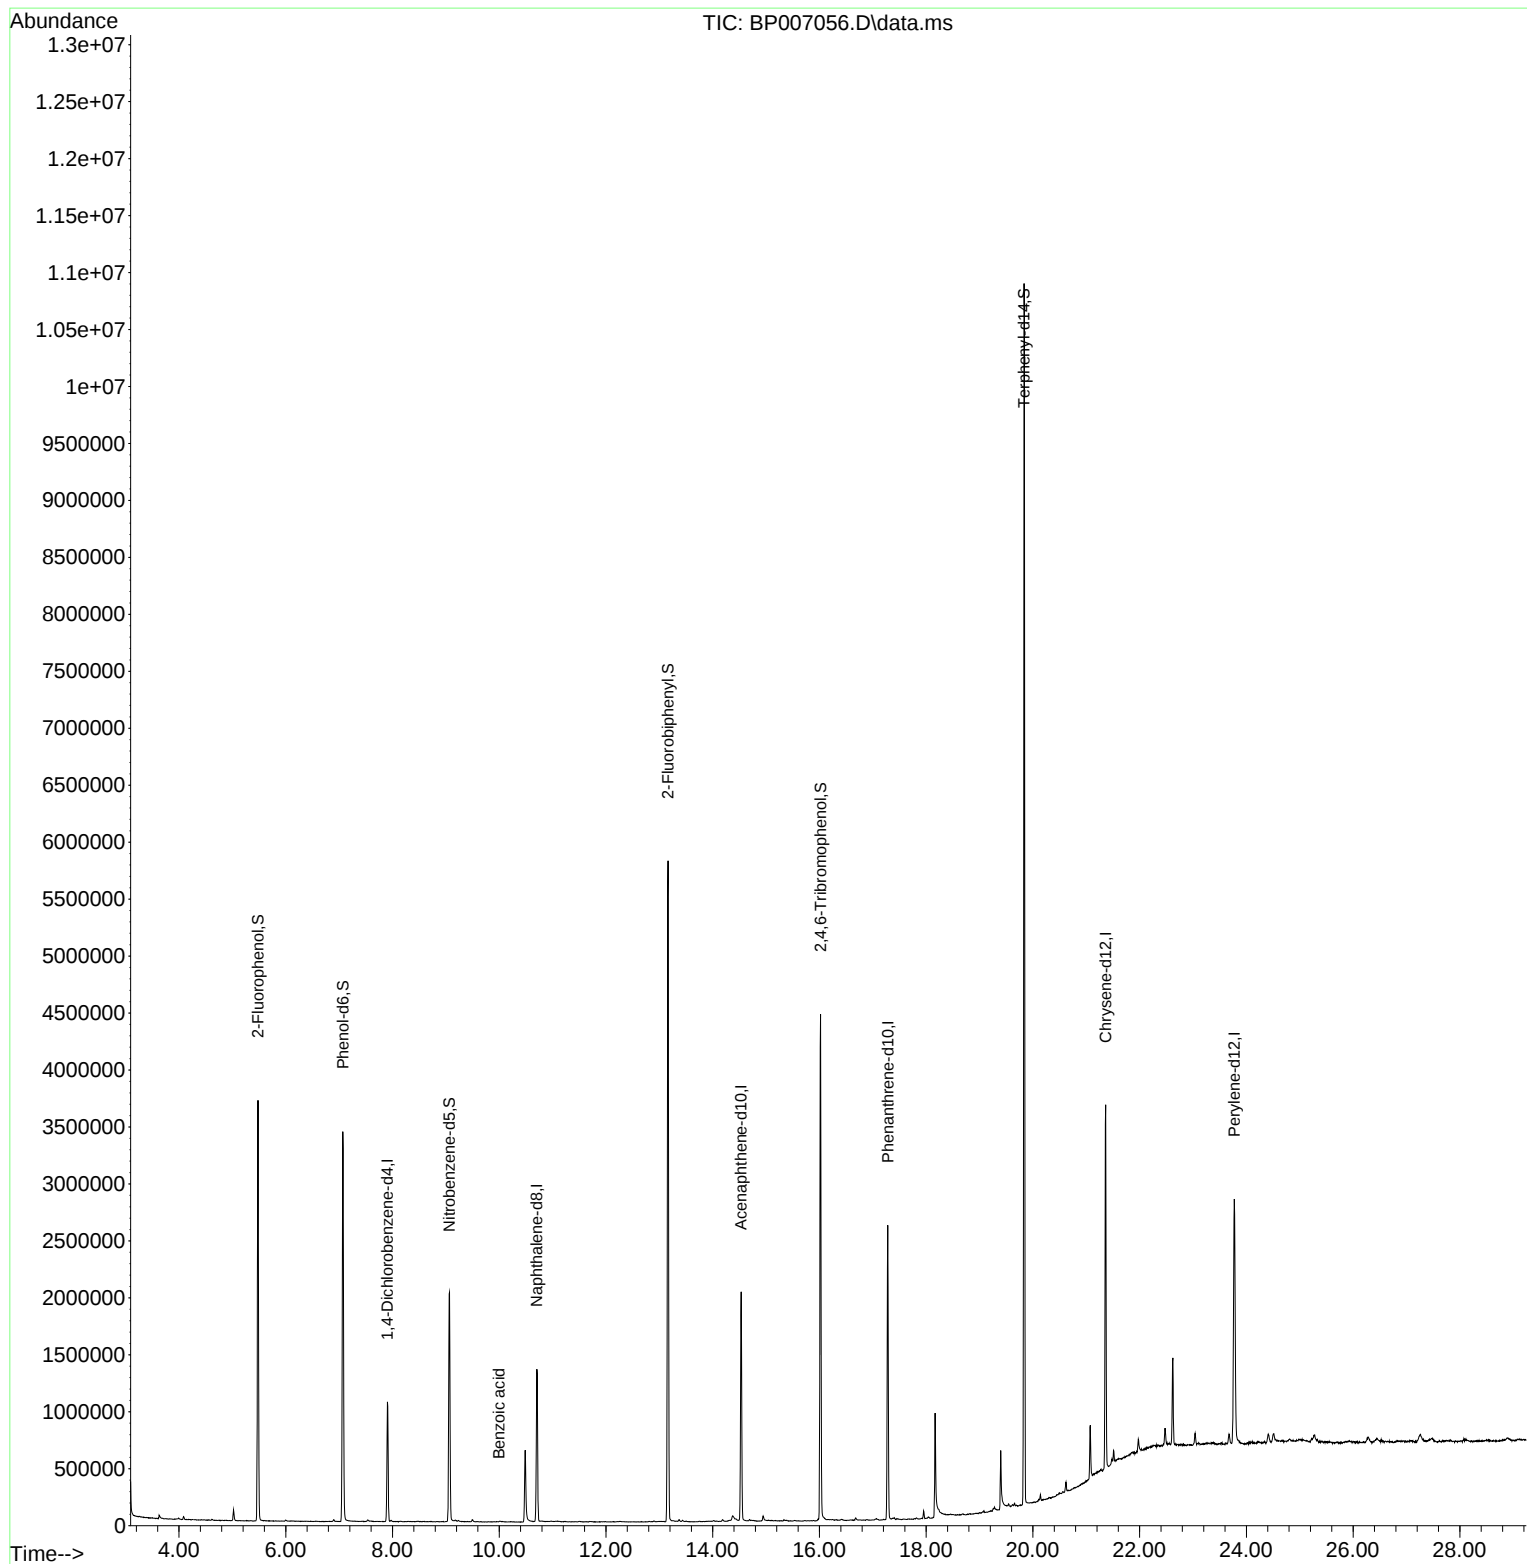




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.905 min Scan# 819
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35




Instrument :
BNA_P
ClientSampleId :
A002145


Tgt Ion:152 Resp: 301584
Ion Ratio Lower Upper
152 100
150 158.1 125.6 188.4
115 57.3 48.5 72.7

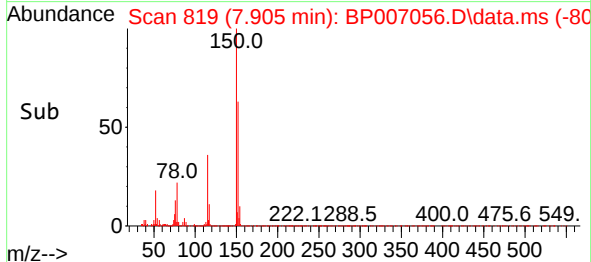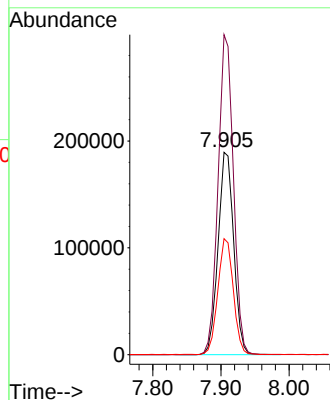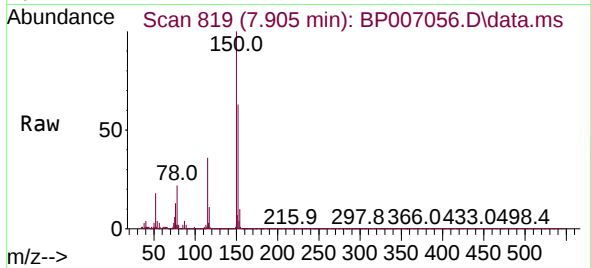

#5
2-Fluorophenol
Concen: 91.971 ng
RT: 5.481 min Scan# 407
Delta R.T. 0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Tgt Ion:112 Resp: 1698600
Ion Ratio Lower Upper
112 100
64 51.3 41.4 62.2
63 25.9 23.8 35.8


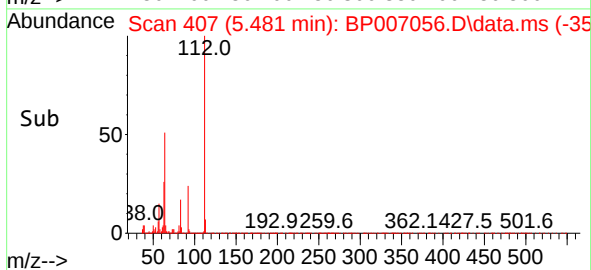
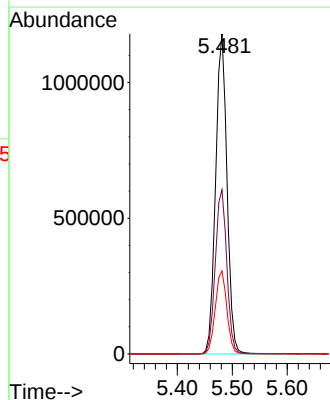
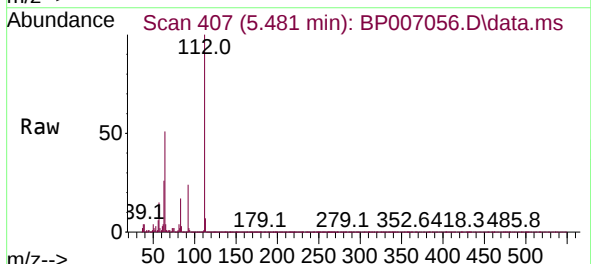


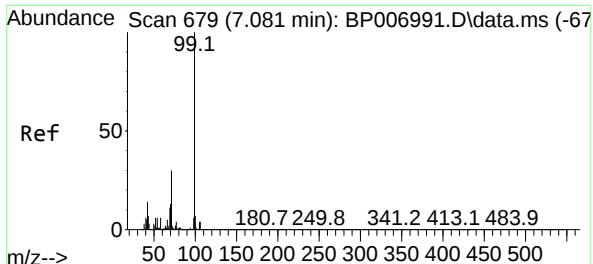

#7
Phenol-d6
Concen: 84.059 ng
RT: 7.069 min Scan# 677
Delta R.T. -0.000 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35




Instrument :
BNA_P
ClientSampleId :
A002145


Tgt Ion: 99 Resp: 2118992
Ion Ratio Lower Upper
99 100
42 13.8 13.4 20.0
71 30.1 30.6 46.0#

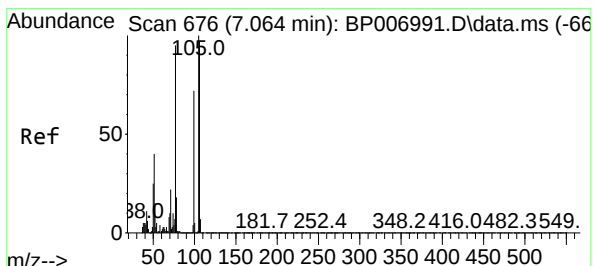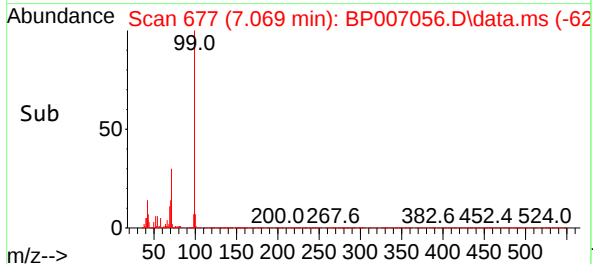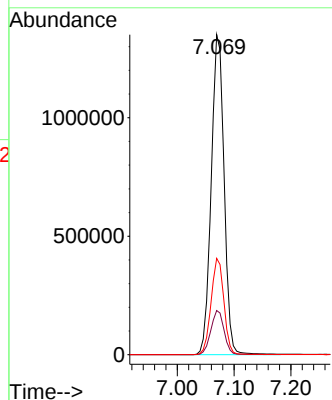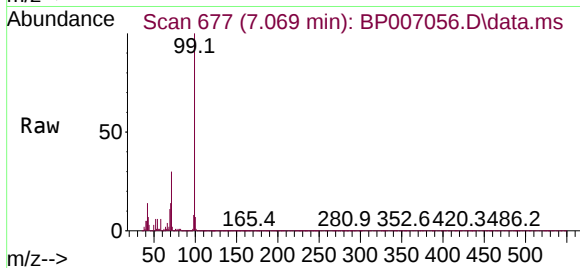

#9
Benzaldehyde
Concen: Below Cal
RT: 7.016 min Scan# 668
Delta R.T. -0.029 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Tgt Ion: 77 Resp: 614
Ion Ratio Lower Upper
77 100
105 57.9 76.7 116.7#
106 18.5 76.2 116.2#

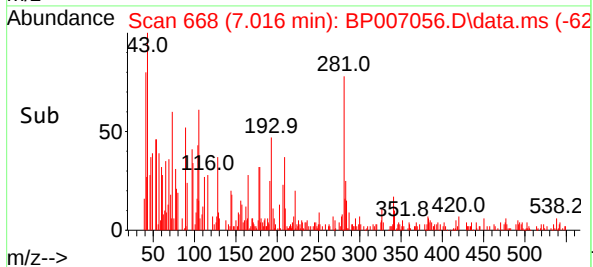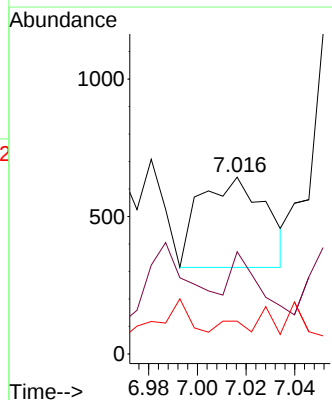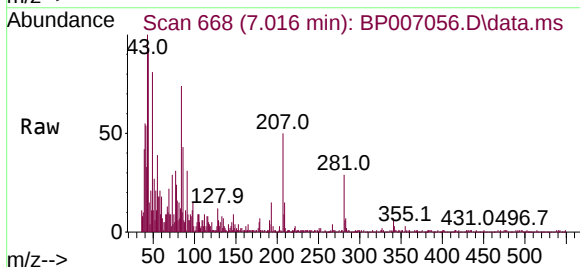







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.704 min Scan# 1295
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Instrument :
BNA_P
ClientSampleId :
A002145

Tgt Ion:136 Resp: 1146926




Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.6	12.8
54	7.4	4.6	6.8#
68	6.1	3.6	5.4#

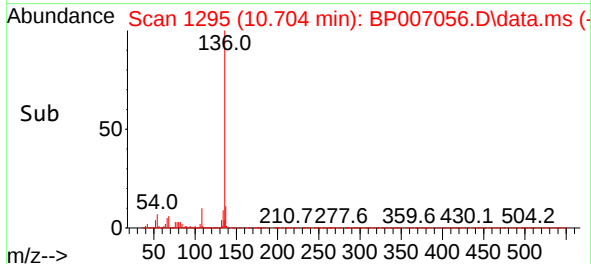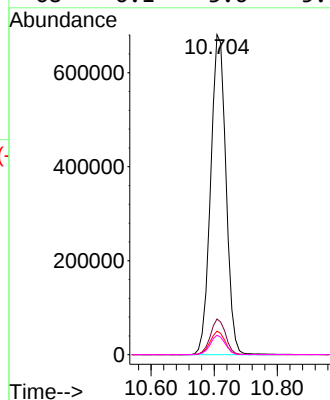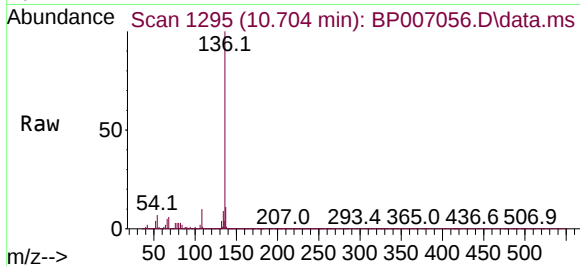


#23
Nitrobenzene-d5
Concen: 59.737 ng
RT: 9.063 min Scan# 1016
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Tgt Ion: 82 Resp: 1219881

Ion	Ratio	Lower	Upper
82	100		
128	46.1	35.7	53.5
54	45.5	35.0	52.4


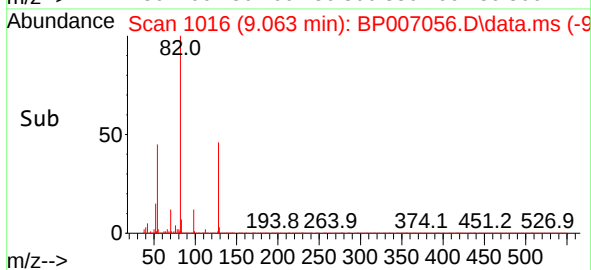
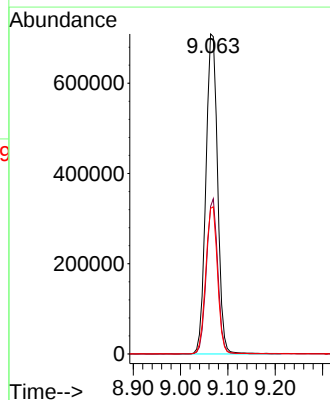
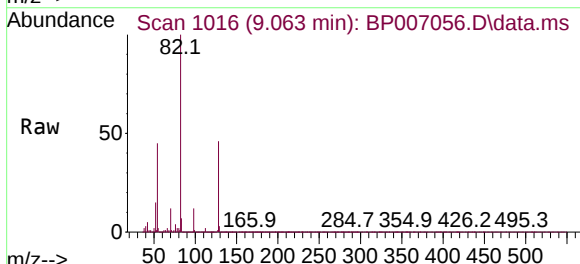




#32
Benzoic acid
Concen: 6.111 ng
RT: 9.993 min Scan# 1174
Delta R.T. -0.018 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35




Instrument :
BNA_P
ClientSampleId :
A002145


Tgt Ion:122 Resp: 203
Ion Ratio Lower Upper
122 100
105 143.4 103.2 143.2#
77 283.3 76.2 116.2#

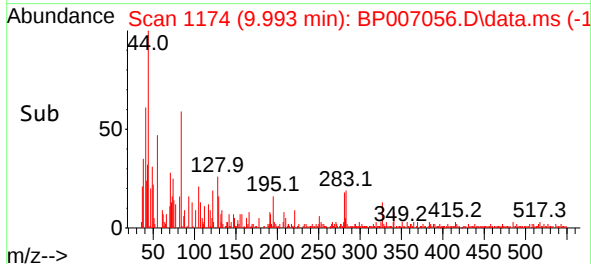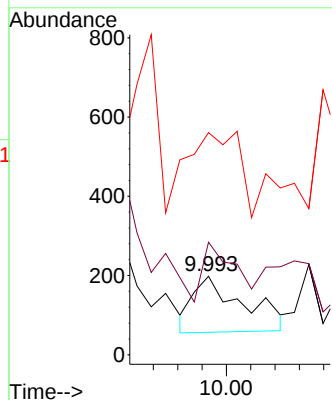

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.534 min Scan# 1946
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Tgt Ion:164 Resp: 715079
Ion Ratio Lower Upper
164 100
162 101.0 80.2 120.2
160 44.7 34.5 51.7


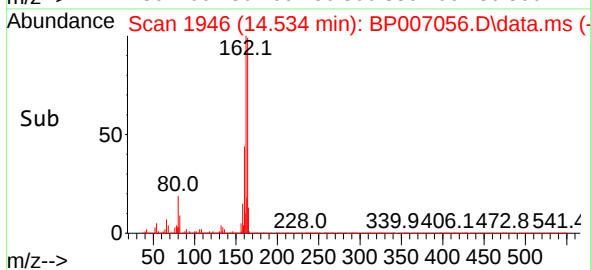
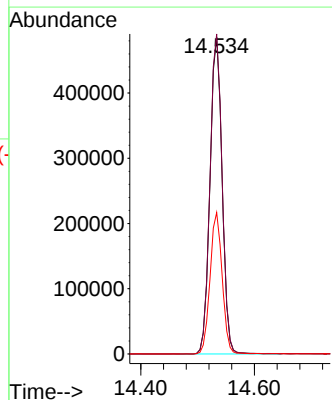
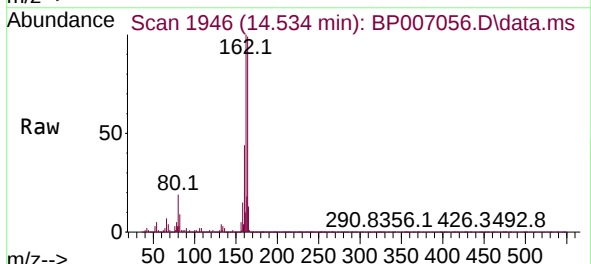




#42
2,4,6-Tribromophenol
Concen: 103.028 ng
RT: 16.022 min Scan# 2199
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35




Instrument :
BNA_P
ClientSampleId :
A002145


Tgt Ion:330 Resp: 886007
Ion Ratio Lower Upper
330 100
332 97.1 77.8 116.8
141 31.9 25.4 38.2

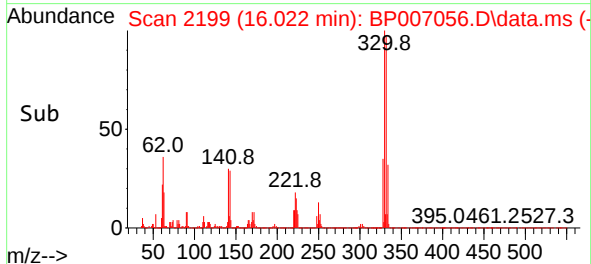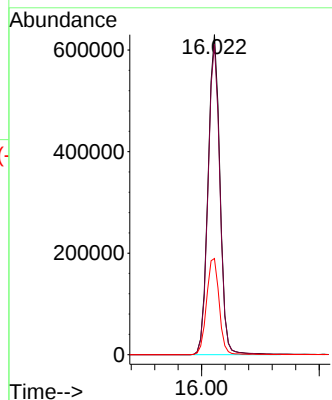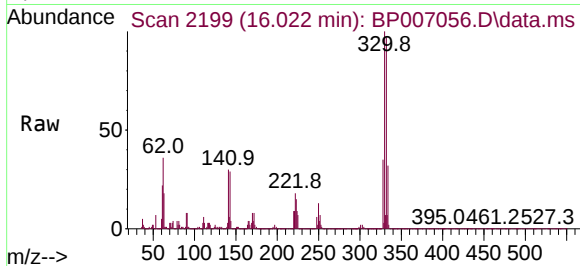

#45
2-Fluorobiphenyl
Concen: 59.846 ng
RT: 13.163 min Scan# 1713
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Tgt Ion:172 Resp: 3099934
Ion Ratio Lower Upper
172 100
171 35.3 27.9 41.9
170 23.5 18.6 27.8


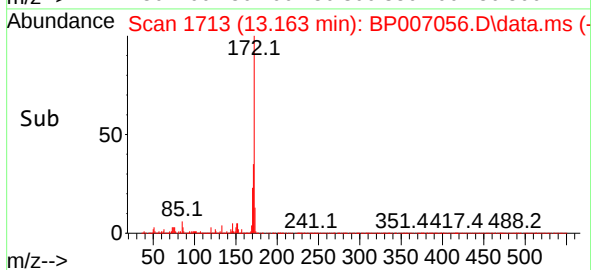
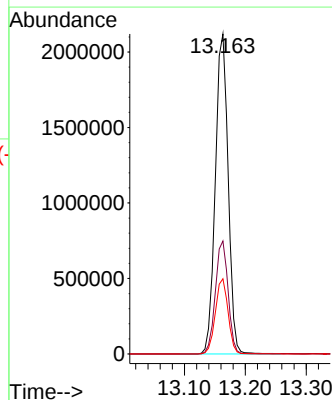
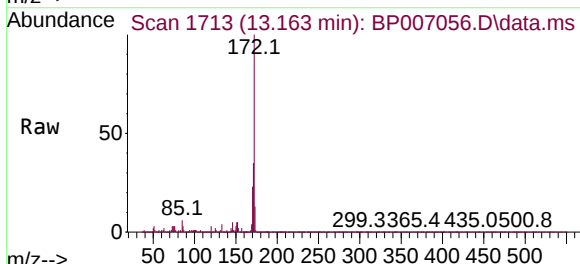


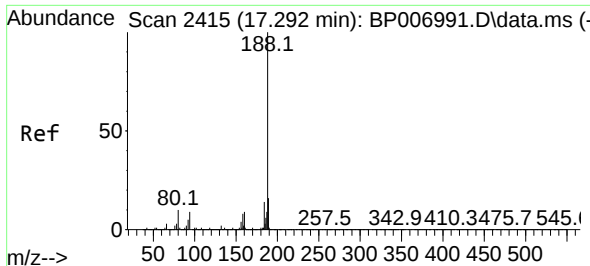

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.281 min Scan# 2413
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35




Instrument :
BNA_P
ClientSampleId :
A002145


Tgt Ion:188 Resp: 1536888
Ion Ratio Lower Upper
188 100
94 8.9 5.6 8.4#
80 9.2 6.3 9.5

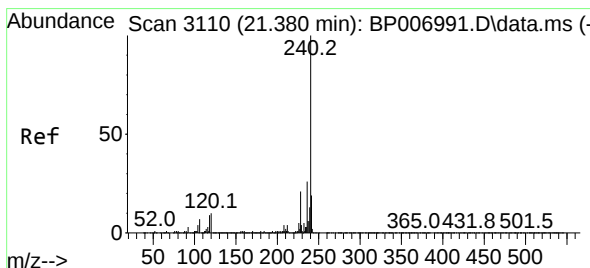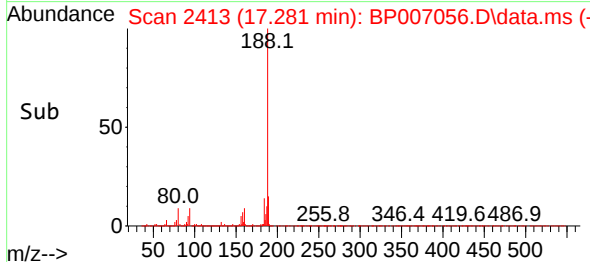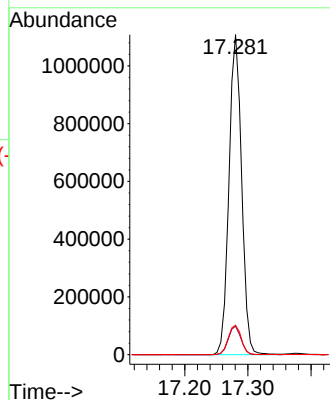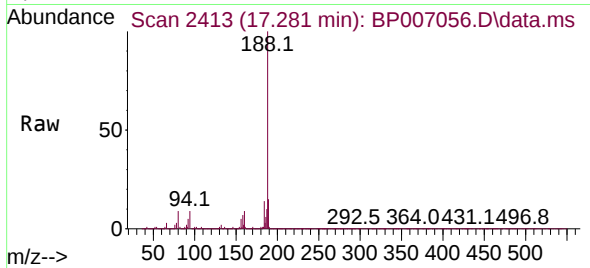

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.363 min Scan# 3107
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Tgt Ion:240 Resp: 1598138
Ion Ratio Lower Upper
240 100
120 10.5 6.5 9.7#
236 26.0 20.6 31.0


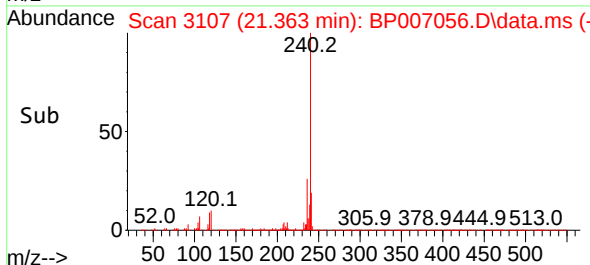
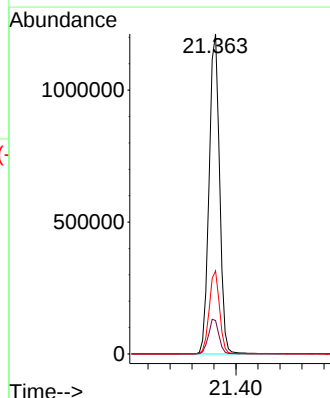
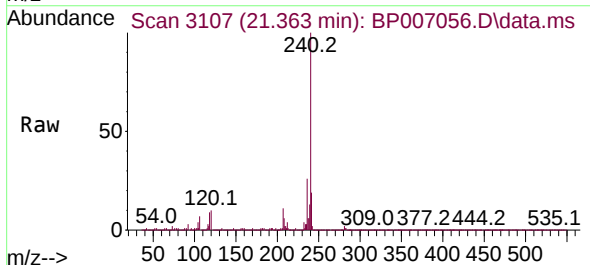




#79
Terphenyl-d14
Concen: 61.740 ng
RT: 19.833 min Scan# 2847
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Instrument :
BNA_P
ClientSampleId :
A002145

Tgt Ion:244 Resp: 5142741
Ion Ratio Lower Upper
244 100
212 7.1 6.0 9.0
122 10.9 7.1 10.7#

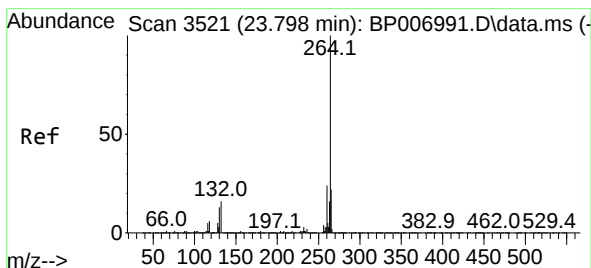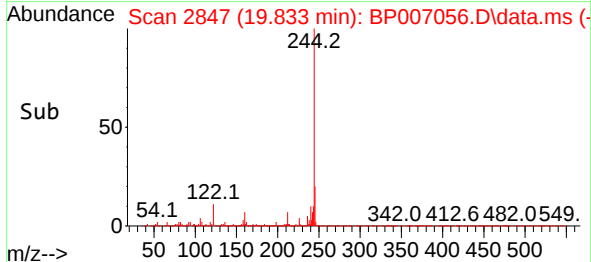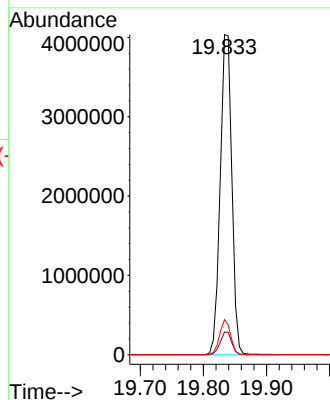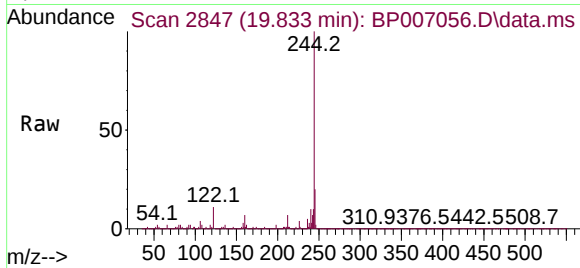

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.774 min Scan# 3517
Delta R.T. -0.006 min
Lab File: BP007056.D
Acq: 20 Sep 2021 18:35

Tgt Ion:264 Resp: 1654858
Ion Ratio Lower Upper
264 100
260 23.9 18.6 28.0
265 22.5 17.6 26.4

