
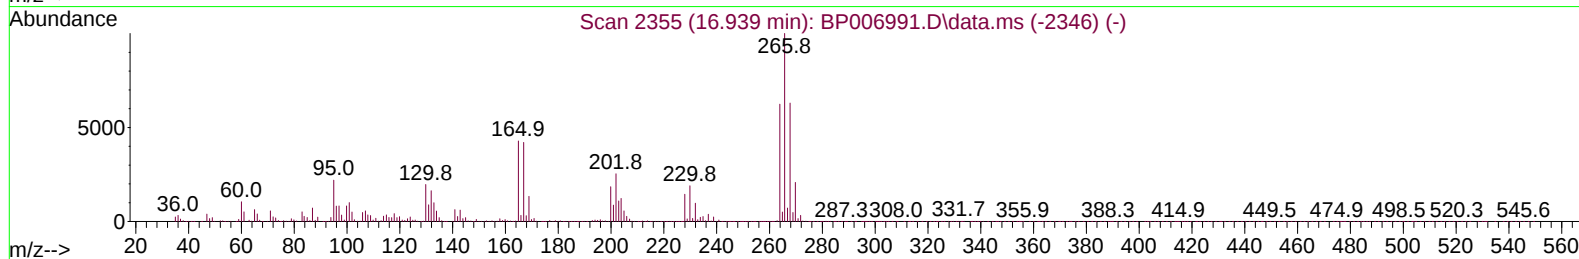
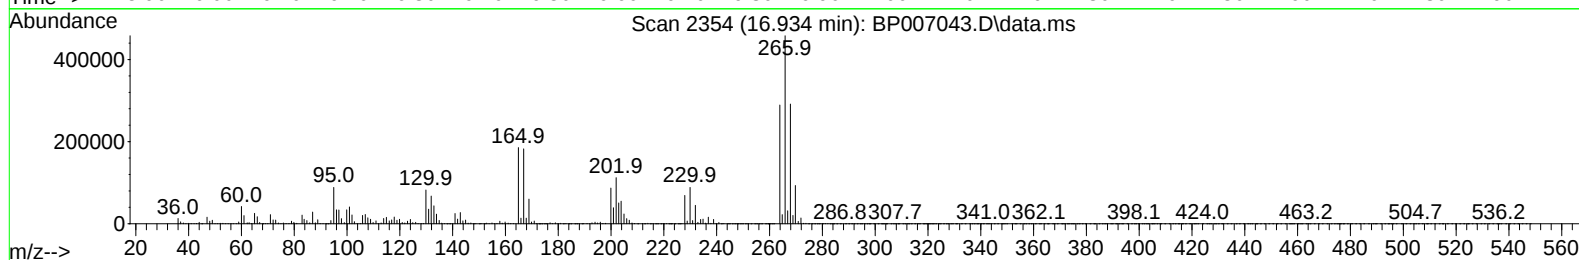


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
Data File : BP007043.D
Acq On : 20 Sep 2021 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 11:24:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 17 10:50:16 2021
Response via : Initial Calibration

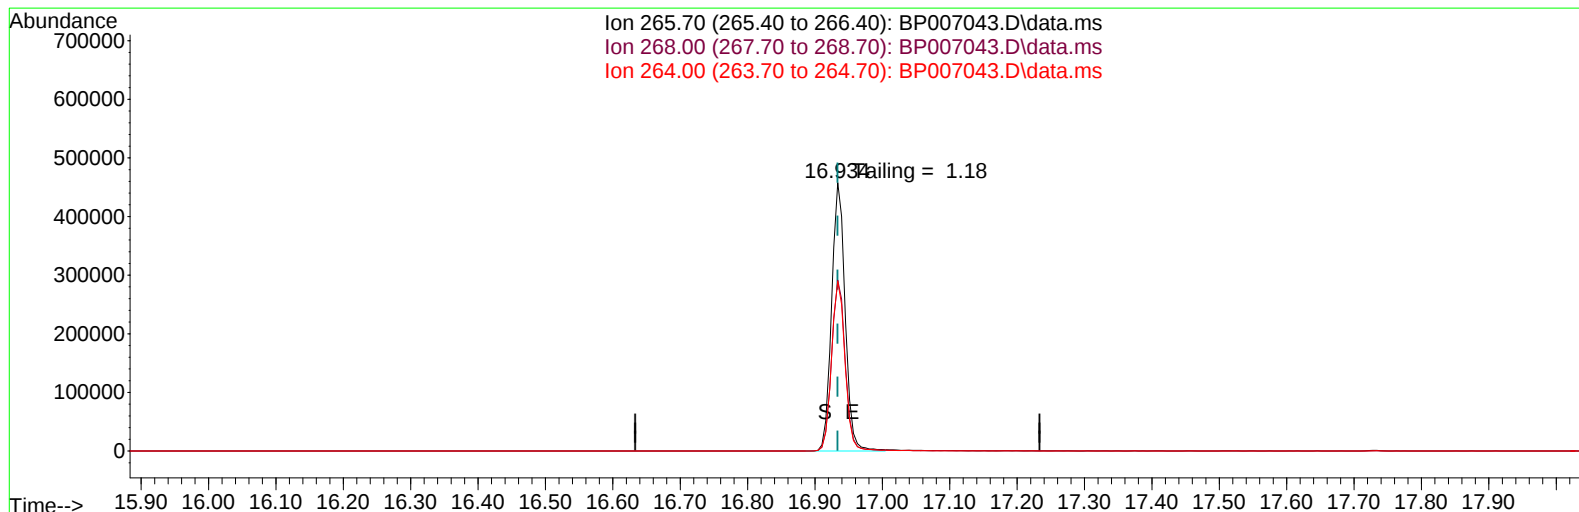

TIC: BP007043.D\data.ms

(70) Pentachlorophenol (C)




16.934min (+ 0.000) 126780.01 ng

response 642438

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.67
264.00	62.90	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
Data File : BP007043.D
Acq On : 20 Sep 2021 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 11:24:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 17 10:50:16 2021
Response via : Initial Calibration

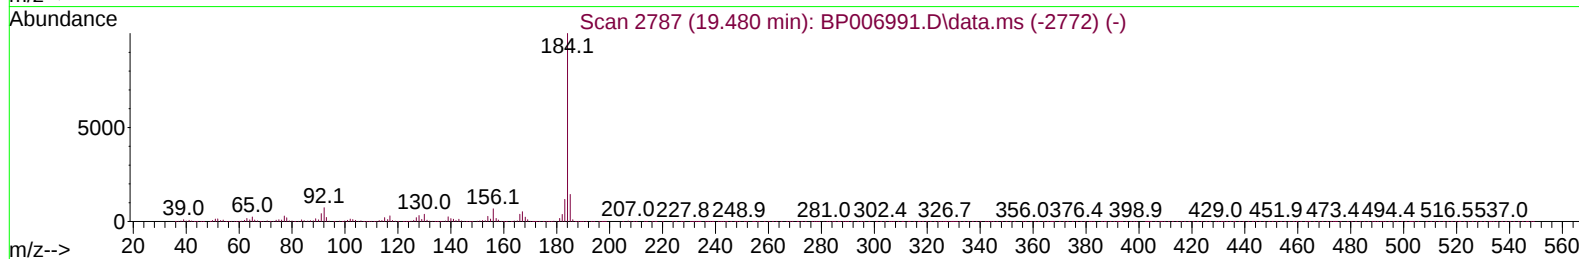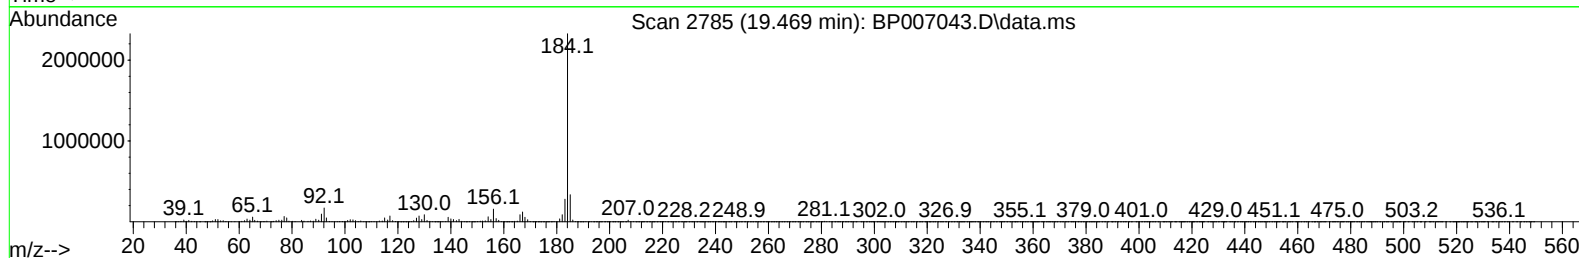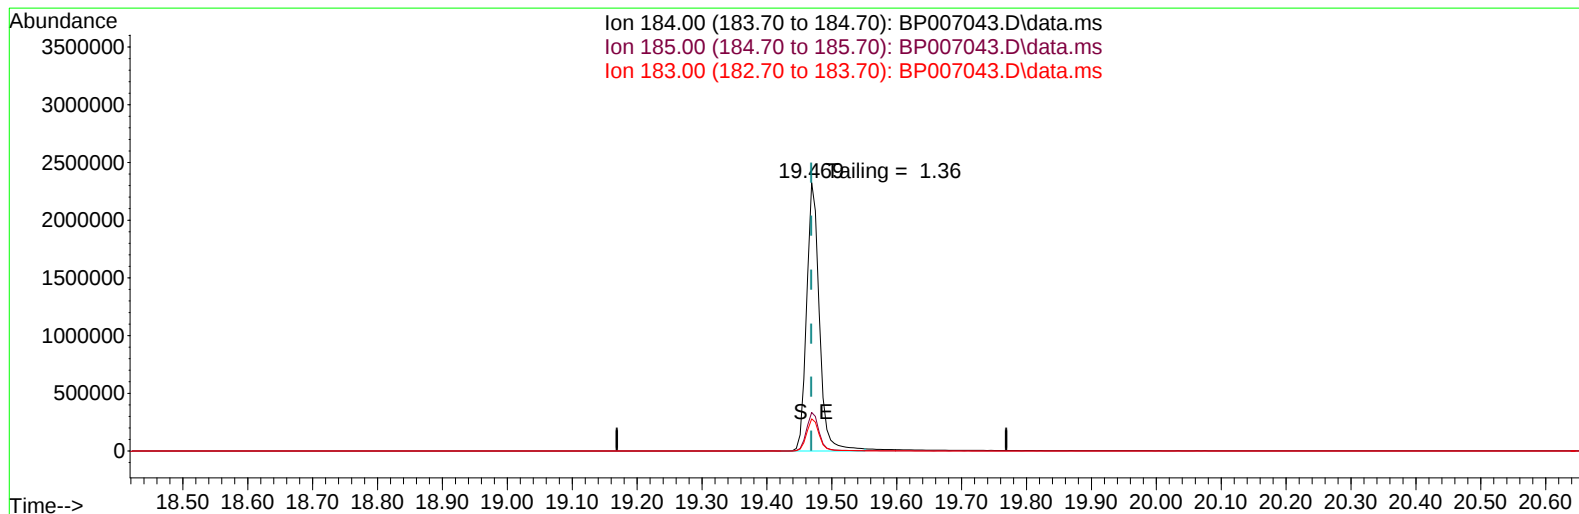

TIC: BP007043.D\data.ms

(77) Benzidine**19.469min (+ 0.000) -20.00 ng****response 3234888**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.39
183.00	11.90	12.00
0.00	0.00	0.00