
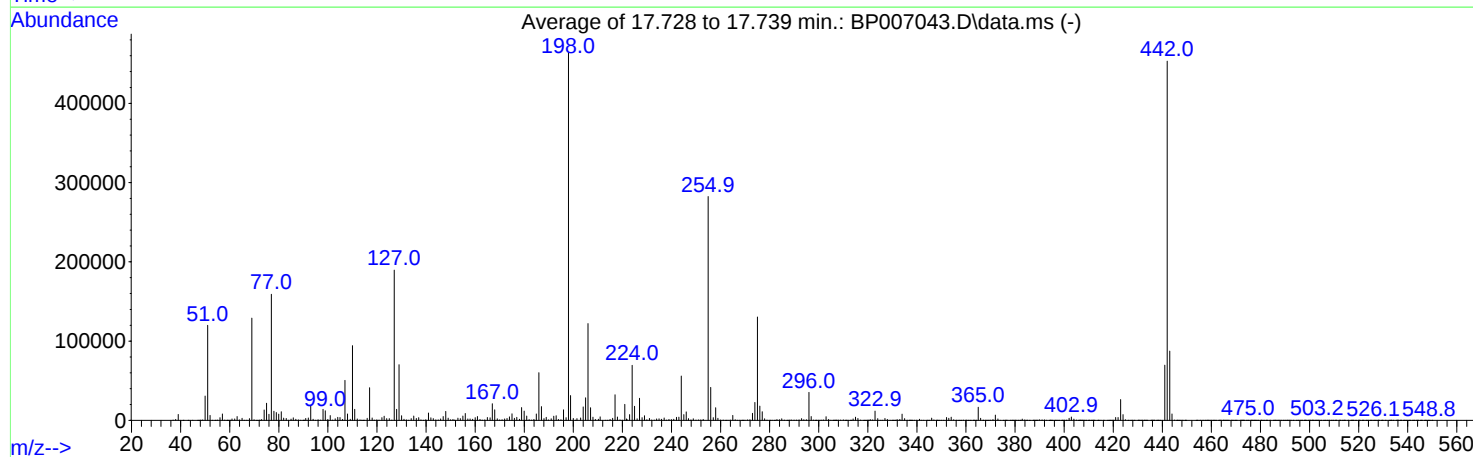


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
 Data File : BP007043.D
 Acq On : 20 Sep 2021 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 17 10:50:16 2021

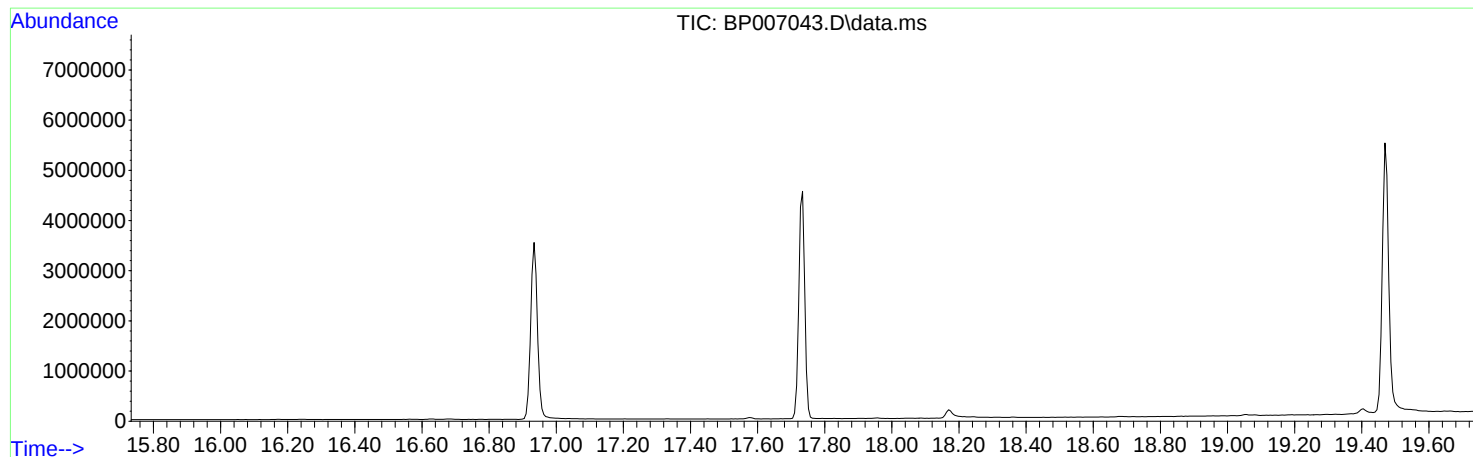




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	119905	PASS
68	69	0.00	2	1.8	2329	PASS
69	198	0.00	100	27.8	128936	PASS
70	69	0.00	2	0.6	734	PASS
127	198	10	80	40.9	189621	PASS
197	198	0.00	2	0.8	3525	PASS
198	198	100	100	100.0	464126	PASS
199	198	5	9	6.7	31261	PASS
275	198	10	60	28.1	130448	PASS
365	198	1	100	3.6	16491	PASS
441	198	0.01	100	15.0	69704	PASS
442	442	100	100	100.0	453141	PASS
443	442	15	24	19.3	87456	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
Data File : BP007043.D
Acq On : 20 Sep 2021 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 20 11:24:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 17 10:50:16 2021
Response via : Initial Calibration

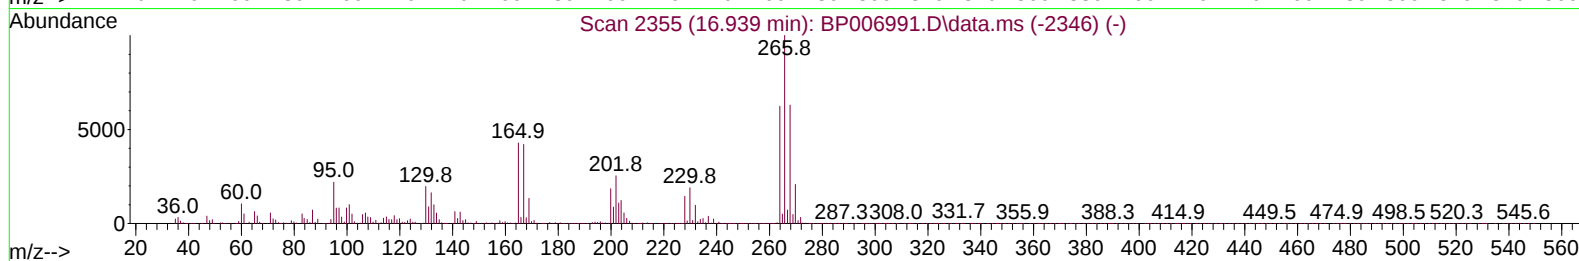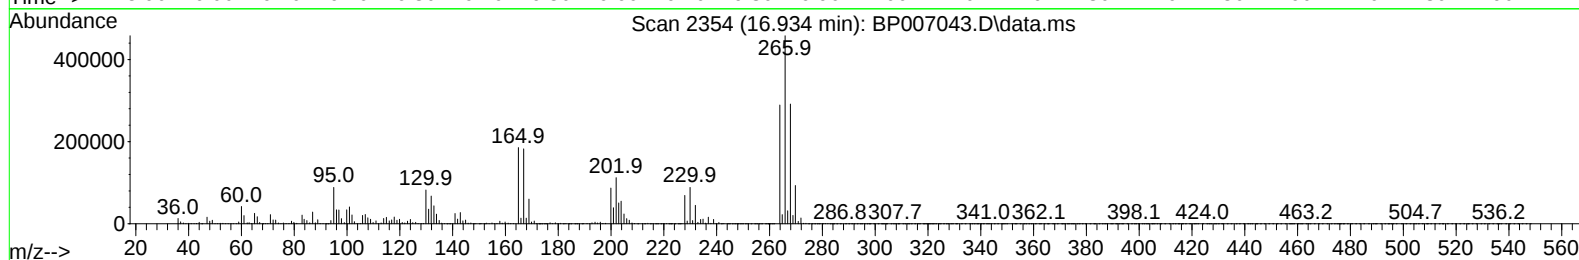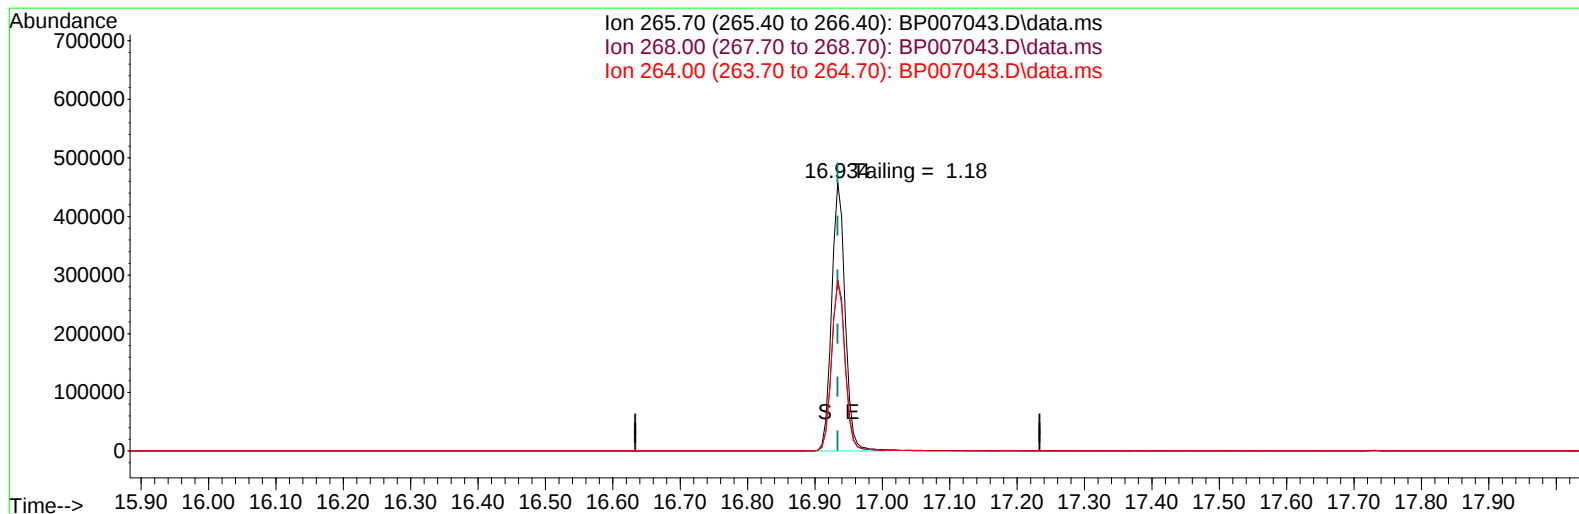

TIC: BP007043.D\data.ms

(70) Pentachlorophenol (C)

16.934min (+ 0.000) 126780.01 ng




response 642438

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.67
264.00	62.90	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
 Data File : BP007043.D
 Acq On : 20 Sep 2021 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 20 11:24:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 10:50:16 2021
 Response via : Initial Calibration

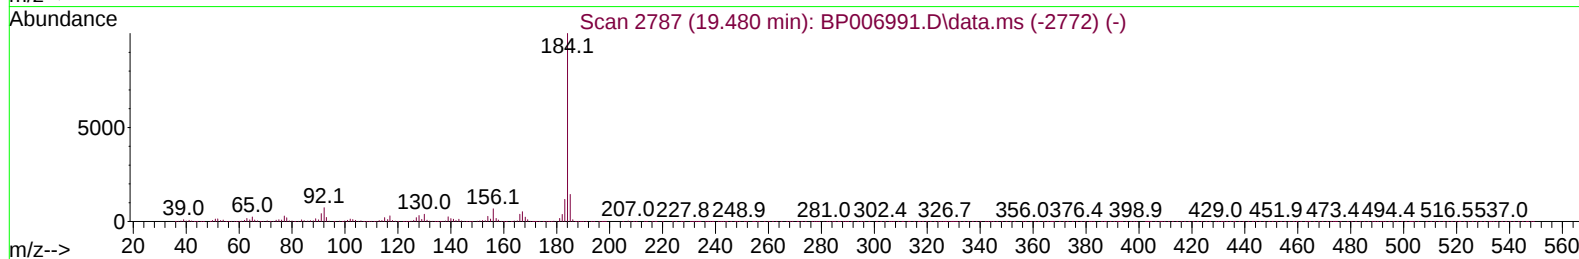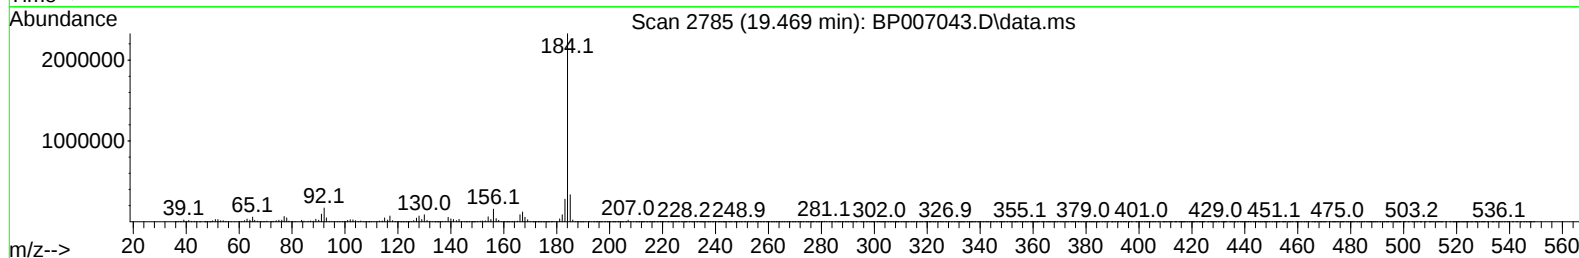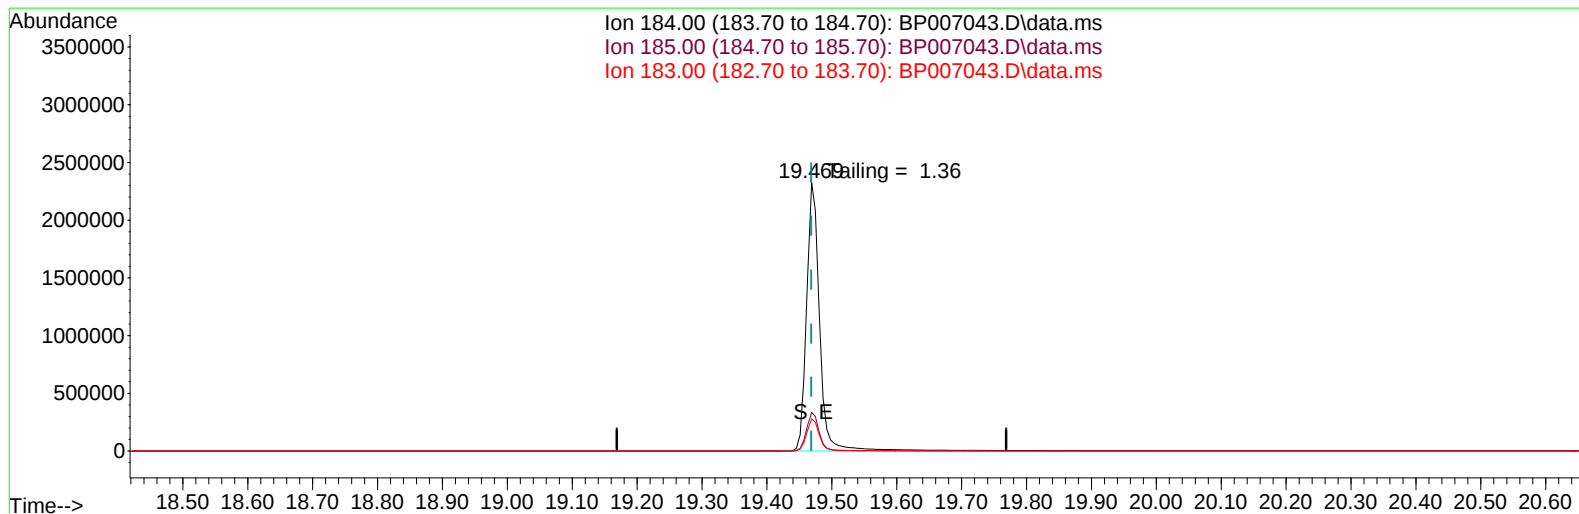

TIC: BP007043.D\data.ms

(77) Benzidine

19.469min (+ 0.000) -20.00 ng

response 3234888

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.39
183.00	11.90	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2021	BNA_P	<u>BP007043.D</u>
Compound Name	Response	Retention Time
DDT	1733933	20.67
DDD	15879	20.24
DDE	3857	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19736	1753669	1.13

Instrument :
BNA_P
ClientSampleId :
DFTPP