
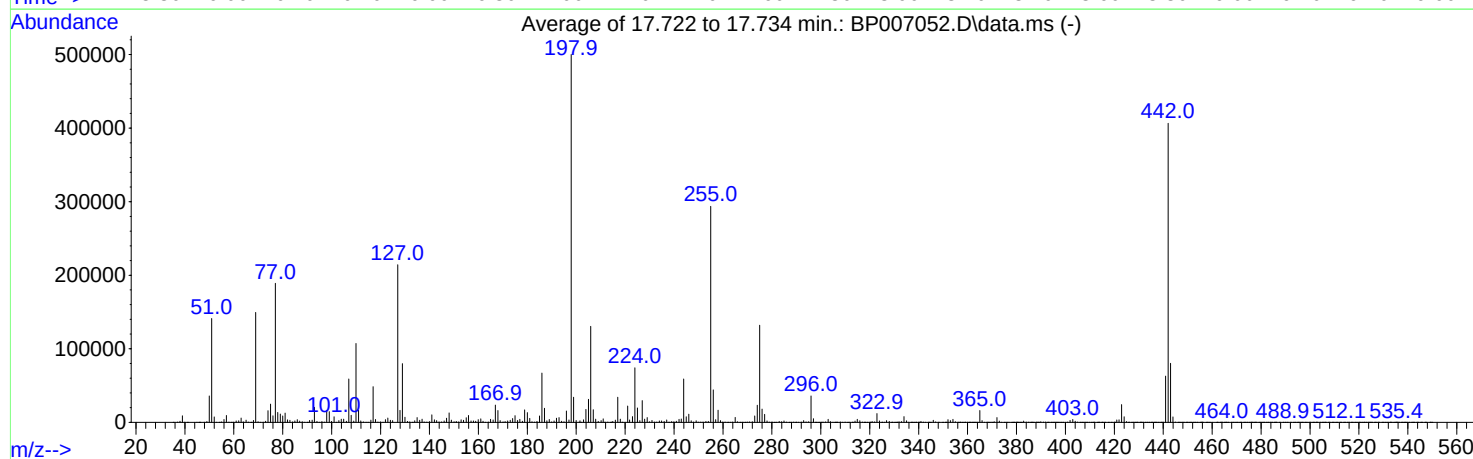


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
 Data File : BP007052.D
 Acq On : 20 Sep 2021 16:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 17 10:50:16 2021

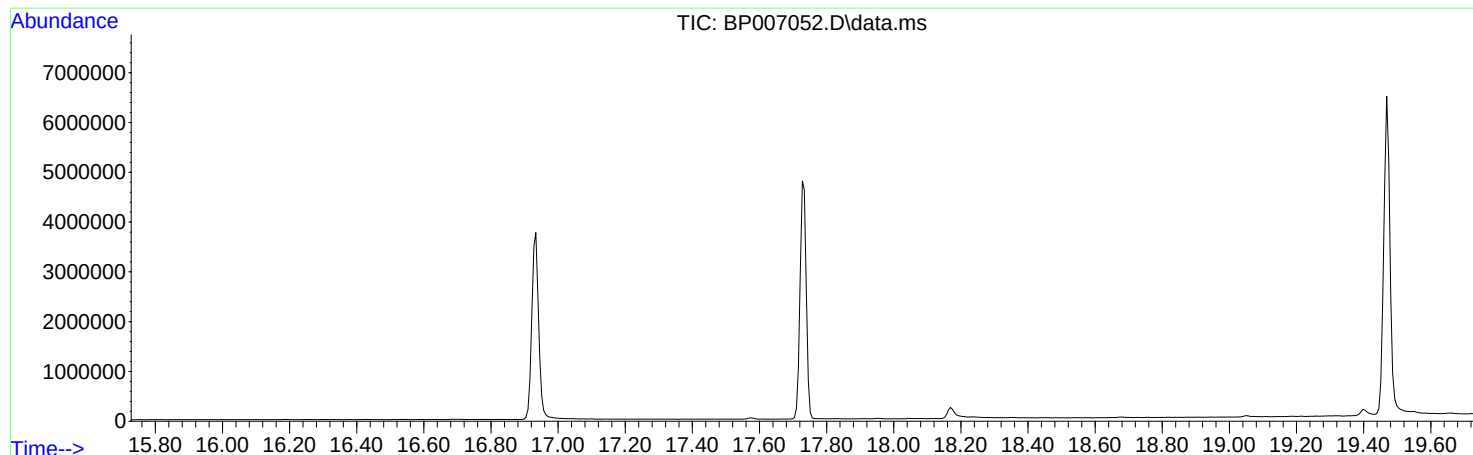




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	141172	PASS
68	69	0.00	2	1.8	2668	PASS
69	198	0.00	100	29.9	149391	PASS
70	69	0.00	2	0.5	814	PASS
127	198	10	80	42.9	214298	PASS
197	198	0.00	2	0.7	3336	PASS
198	198	100	100	100.0	500068	PASS
199	198	5	9	6.8	34111	PASS
275	198	10	60	26.4	132077	PASS
365	198	1	100	3.2	16193	PASS
441	198	0.01	100	12.6	62909	PASS
442	442	100	100	100.0	406613	PASS
443	442	15	24	19.7	80173	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
 Data File : BP007052.D
 Acq On : 20 Sep 2021 16:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 20 17:42:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 10:50:16 2021
 Response via : Initial Calibration

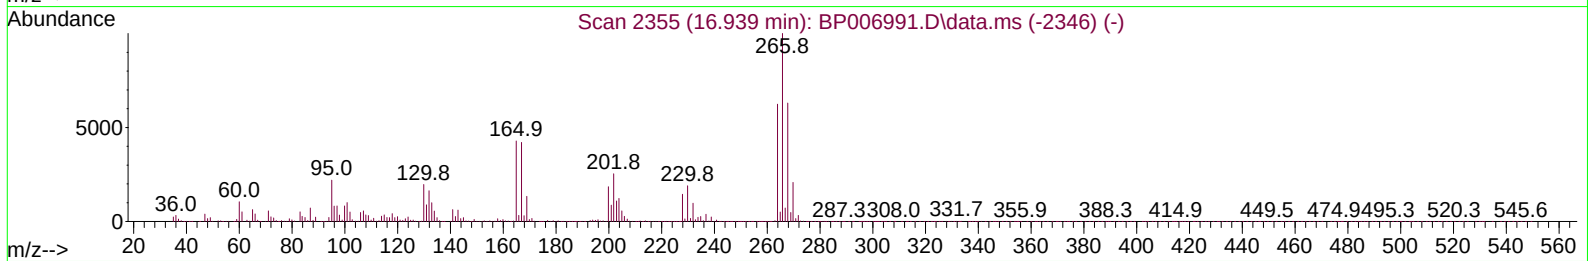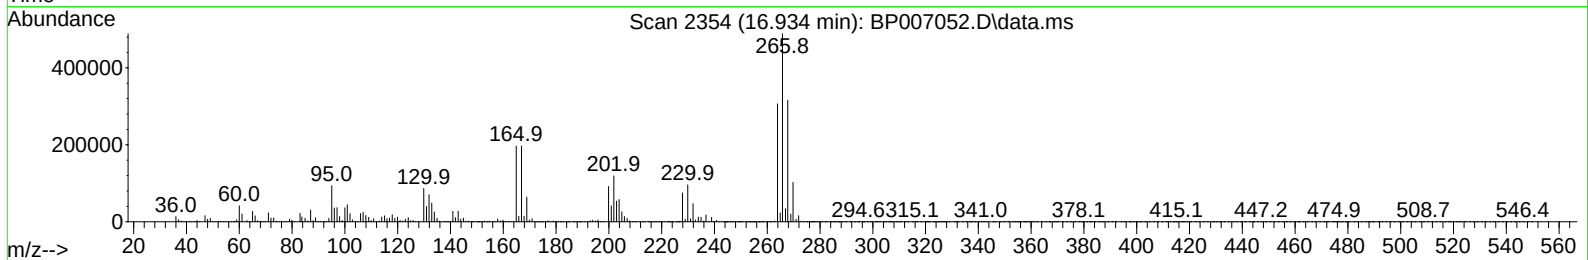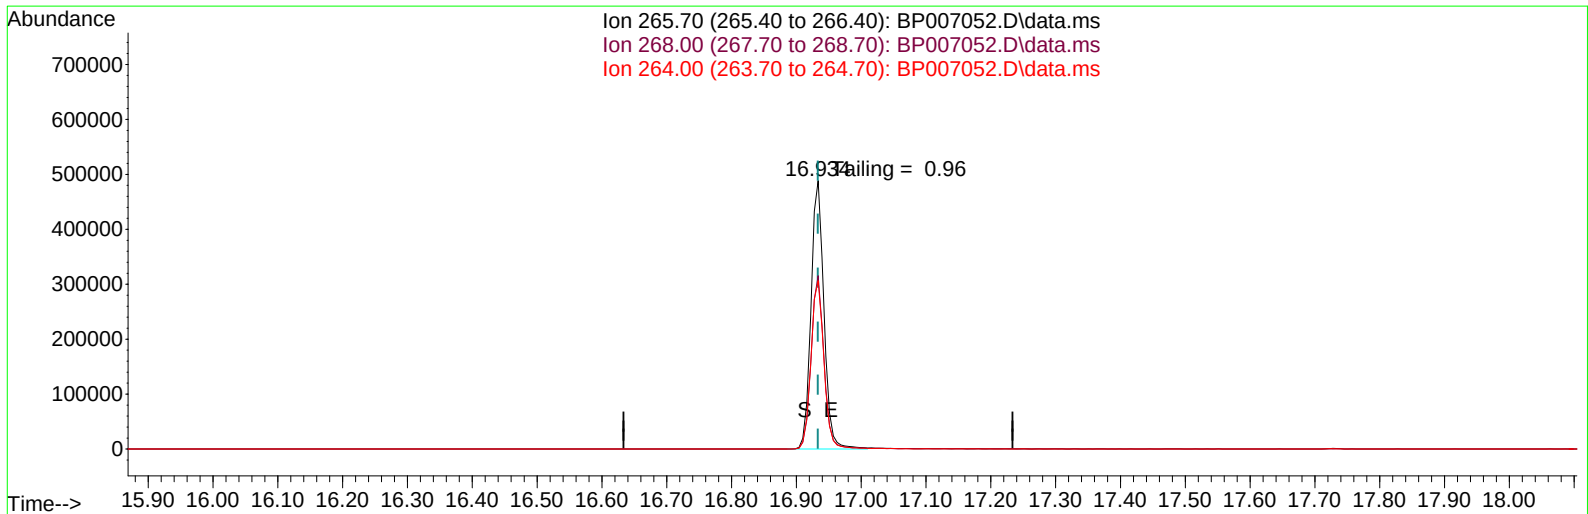

TIC: BP007052.D\data.ms

(70) Pentachlorophenol (C)

16.934min (+ 0.000) 160240.73 ng




response 684037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.59
264.00	62.90	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092021\
 Data File : BP007052.D
 Acq On : 20 Sep 2021 16:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 20 17:42:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 10:50:16 2021
 Response via : Initial Calibration

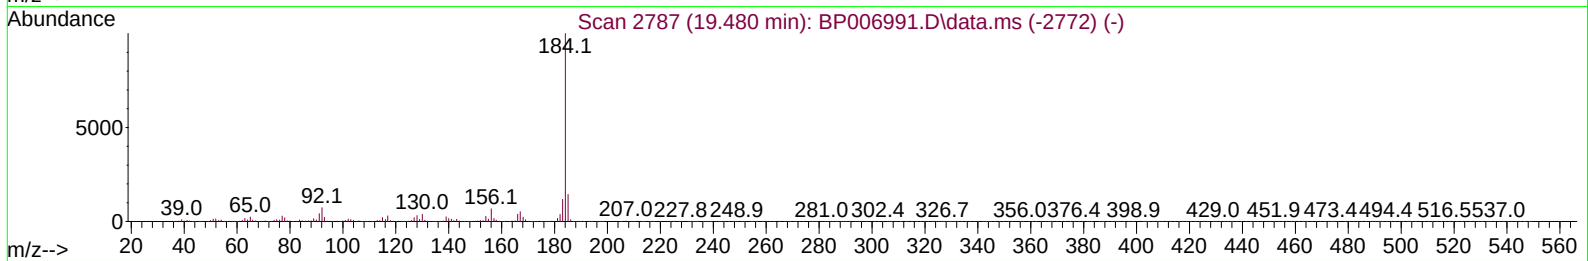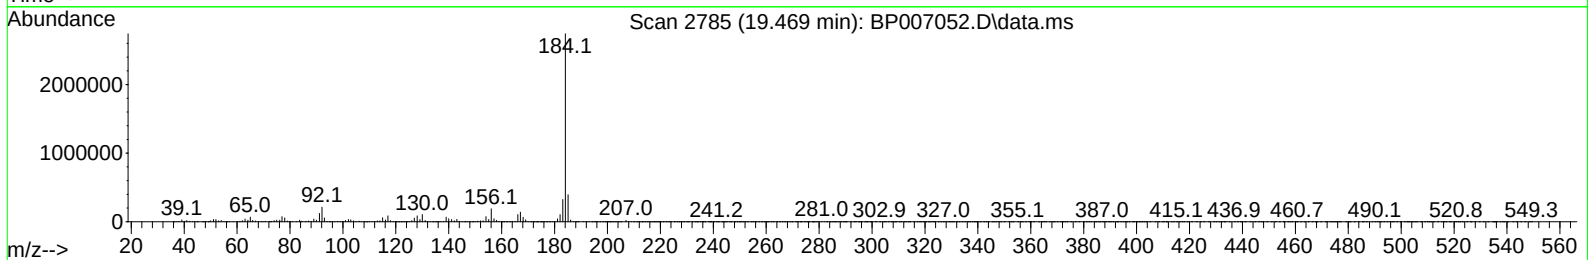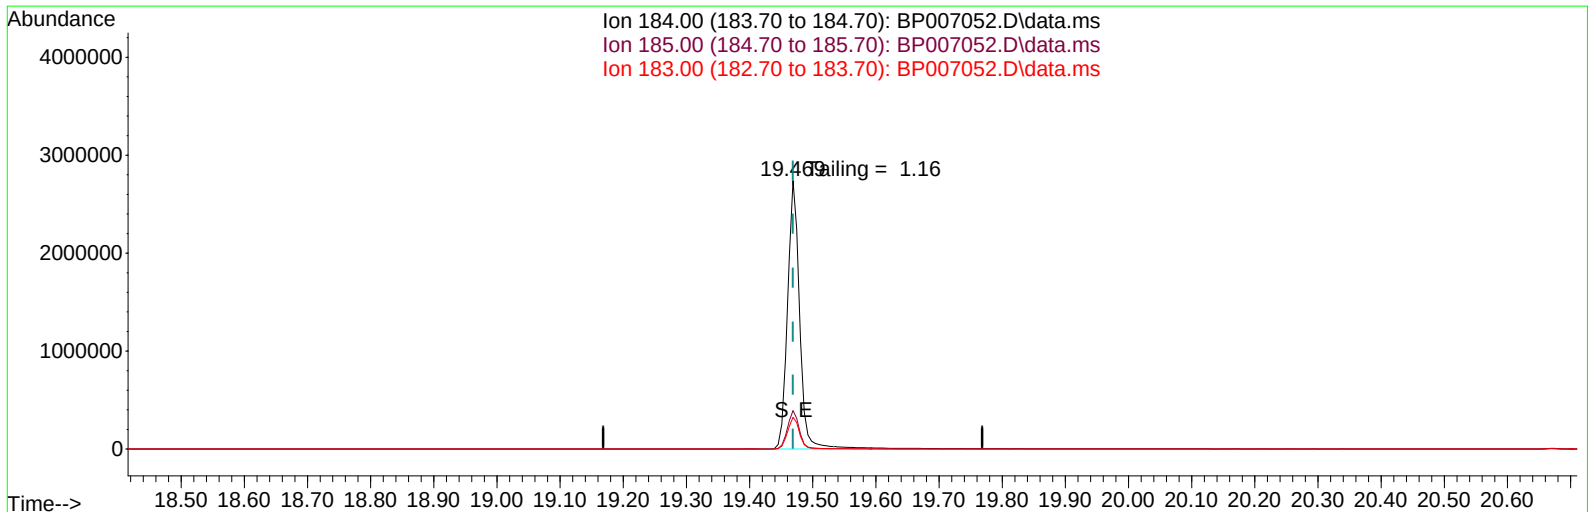

TIC: BP007052.D\data.ms

(77) Benzidine

19.469min (+ 0.000) -20.00 ng

response 3676010

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.35
183.00	11.90	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2021	BNA_P	<u>BP007052.D</u>
Compound Name	Response	Retention Time
DDT	1873715	20.67
DDD	10549	20.233
DDE	3456	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14005	1887720	0.74

Instrument :
BNA_P
ClientSampleId :
DFTPP