
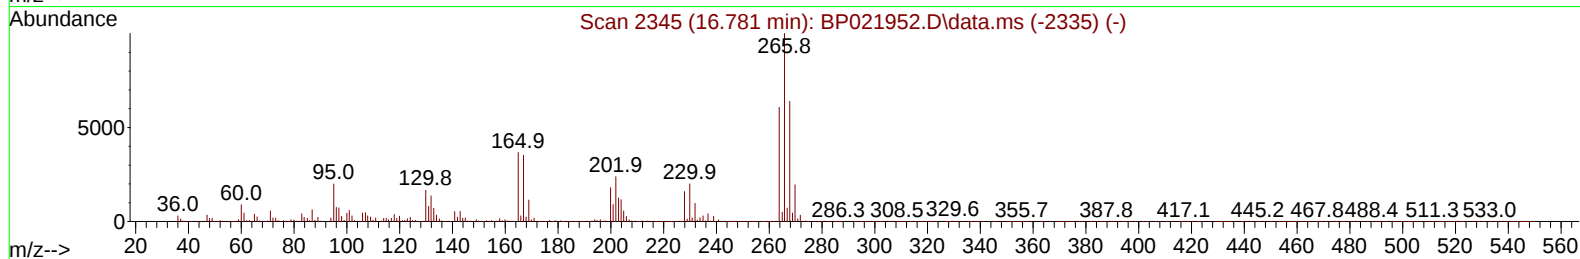
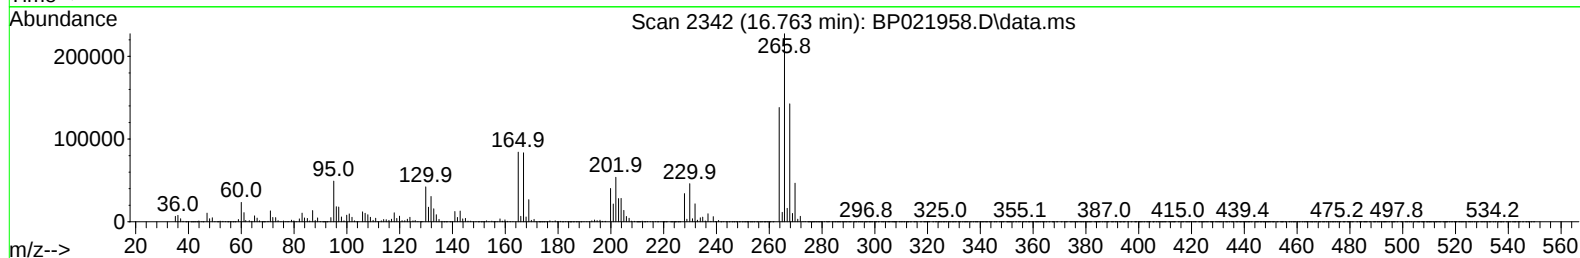


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092024\
Data File : BP021958.D
Acq On : 20 Sep 2024 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 11:07:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

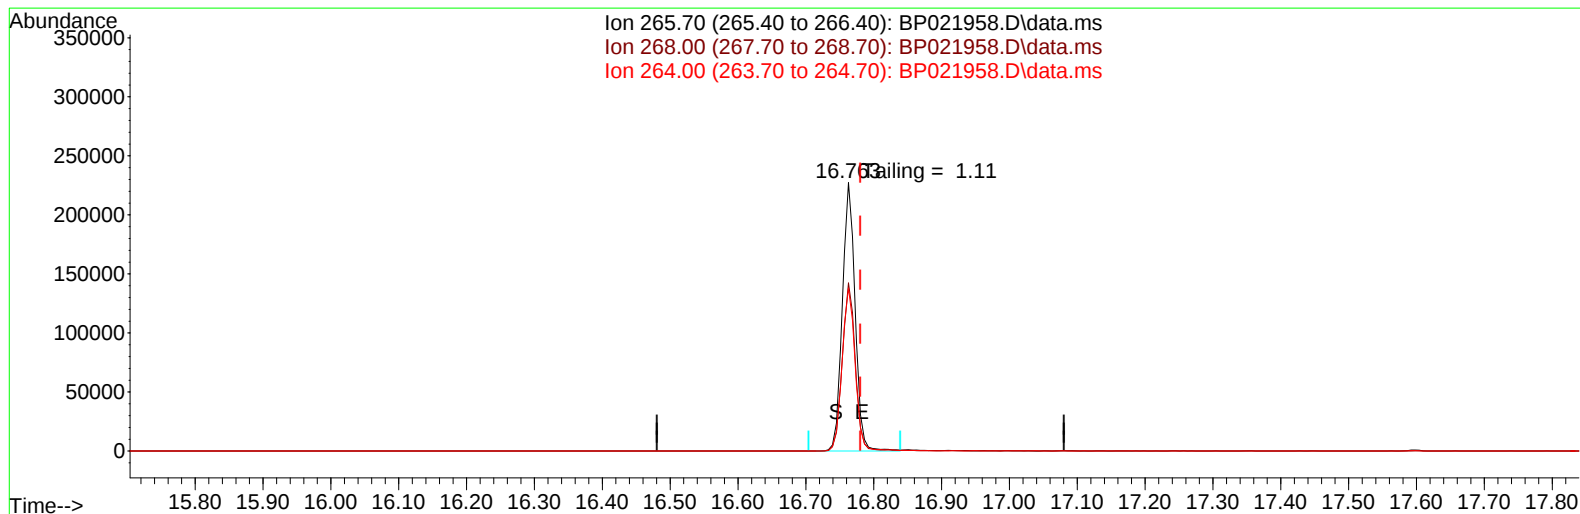

TIC: BP021958.D\data.ms

(70) Pentachlorophenol (C)




16.763min (-0.018) 10127038.21 ng

response 297068

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.70
264.00	60.70	60.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092024\
Data File : BP021958.D
Acq On : 20 Sep 2024 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 11:07:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

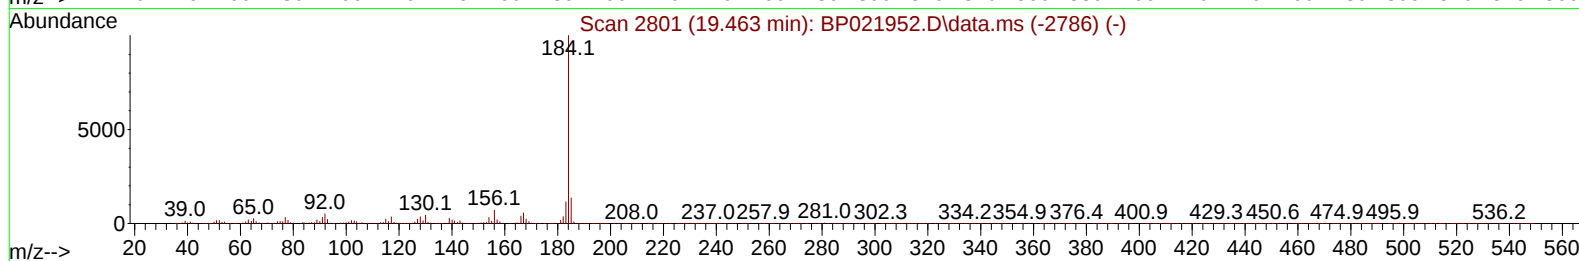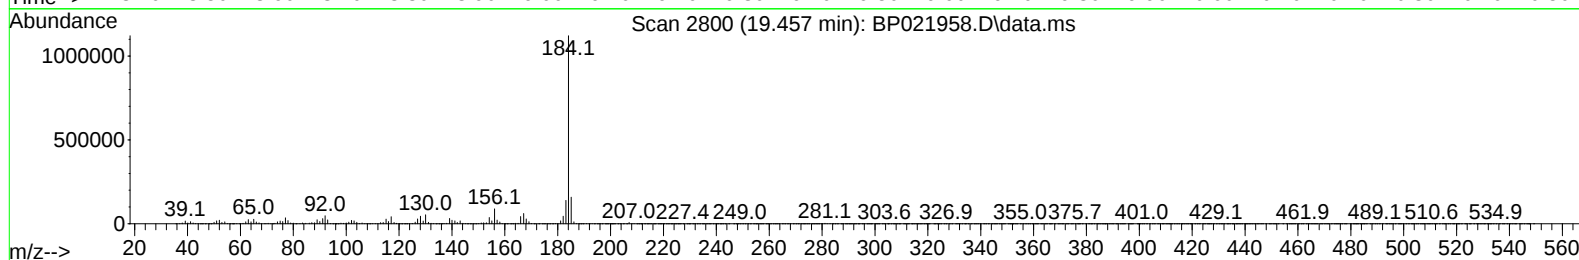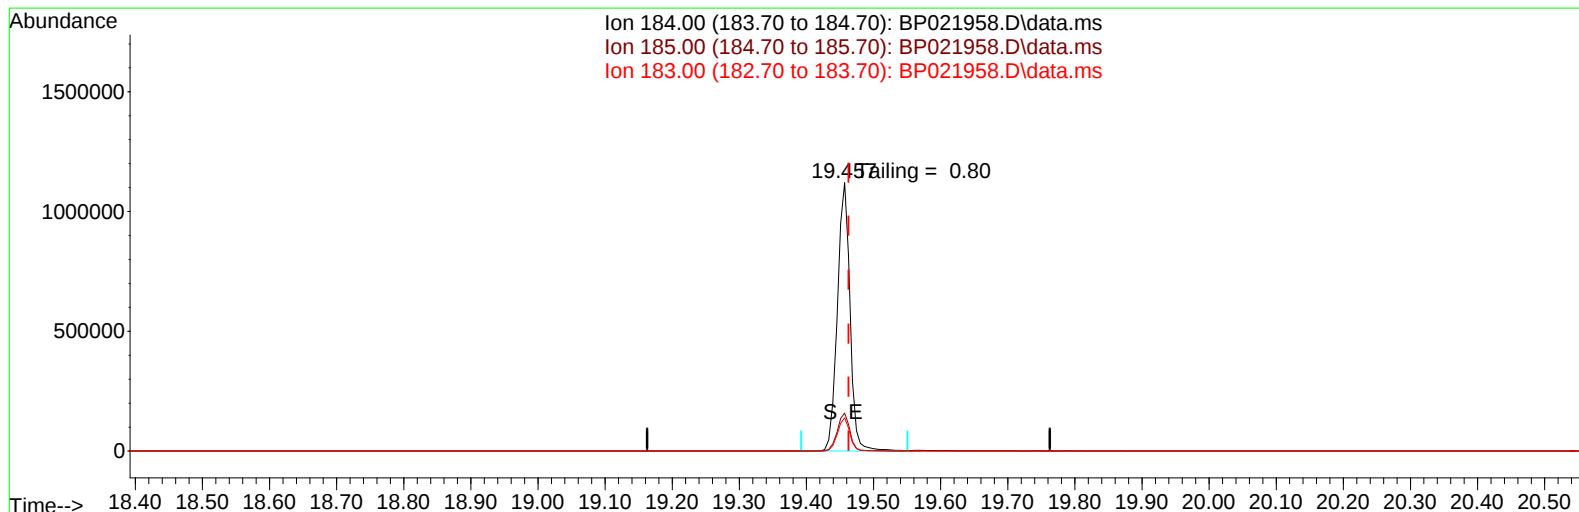

TIC: BP021958.D\data.ms

(77) Benzidine**19.457min (-0.006) 3881466.98 ng****response 1470436**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.16
183.00	11.50	12.39
0.00	0.00	0.00