
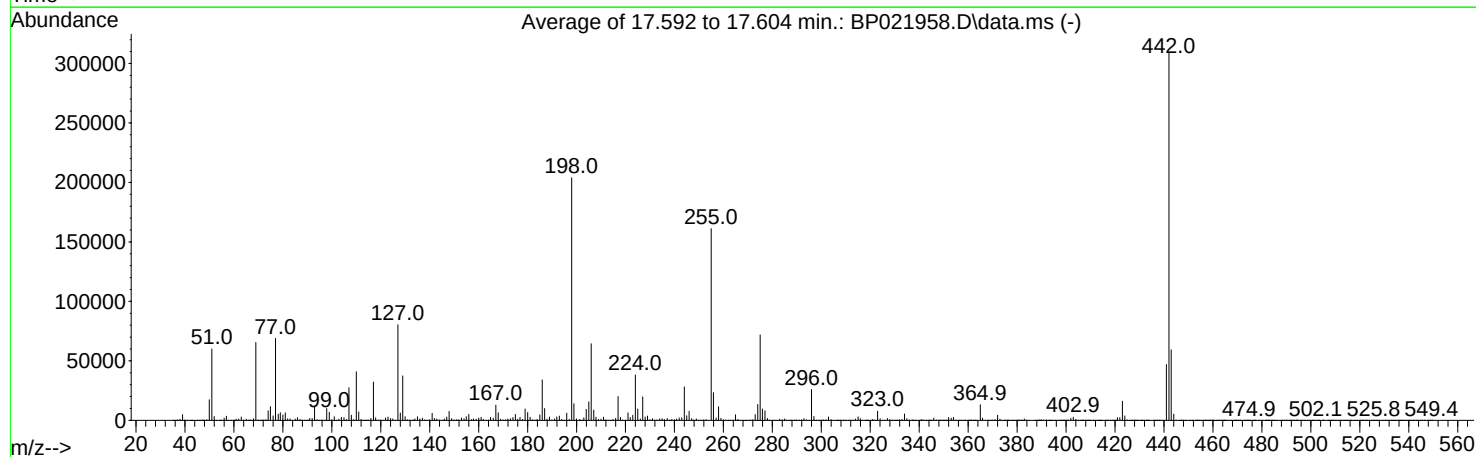


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092024\
Data File : BP021958.D
Acq On : 20 Sep 2024 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 20 01:22:00 2024

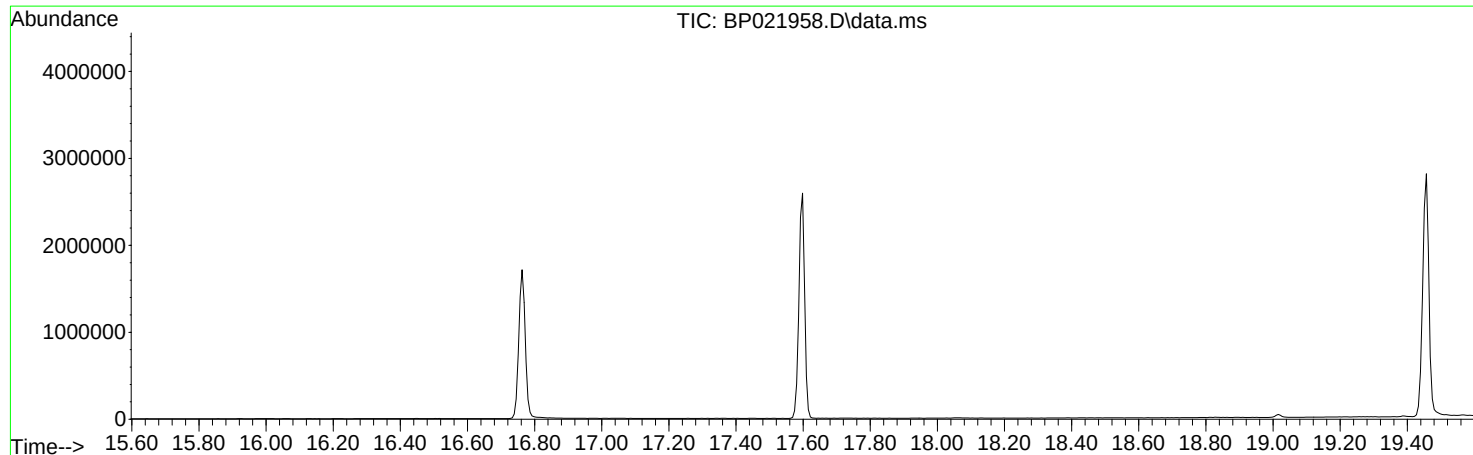

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	60008	PASS
68	69	0.00	2	2.0	1307	PASS
69	198	0.00	100	32.1	65461	PASS
70	69	0.00	2	0.6	417	PASS
127	198	10	80	39.5	80486	PASS
197	198	0.00	2	0.4	870	PASS
198	198	100	100	100.0	203944	PASS
199	198	5	9	6.9	14037	PASS
275	198	10	60	35.2	71772	PASS
365	198	1	100	6.5	13246	PASS
441	198	0.01	100	23.0	46985	PASS
442	442	100	100	100.0	309181	PASS
443	442	15	24	19.2	59344	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/20/2024	BNA_P	<u>BP021958.D</u>
Compound Name	Response	Retention Time
DDT	921261	20.751
DDD	12532	20.345
DDE	733	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13265	934526	1.42

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092024\
Data File : BP021958.D
Acq On : 20 Sep 2024 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 20 11:07:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

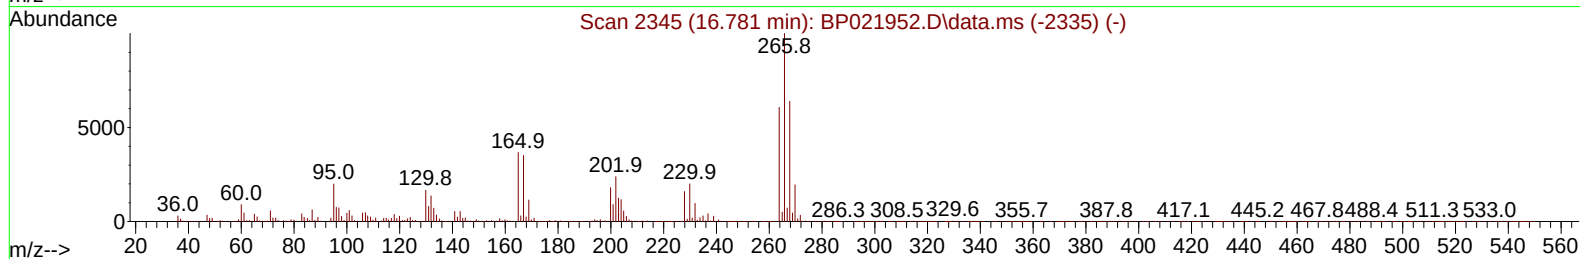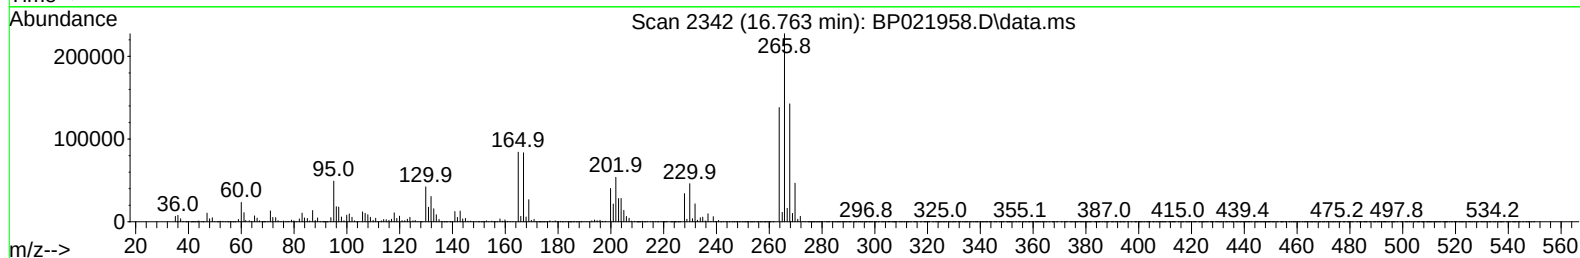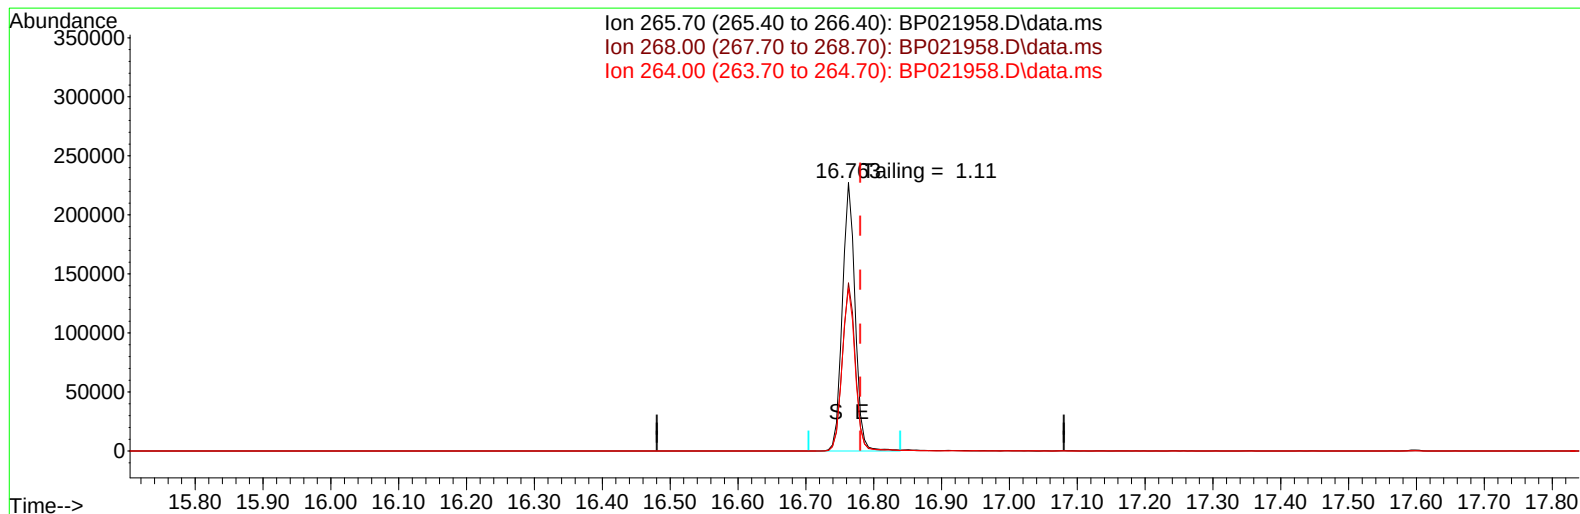

TIC: BP021958.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.018) 10127038.21 ng




response 297068

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.70
264.00	60.70	60.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092024\
 Data File : BP021958.D
 Acq On : 20 Sep 2024 08:24
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 20 11:07:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 20 01:22:00 2024
 Response via : Initial Calibration

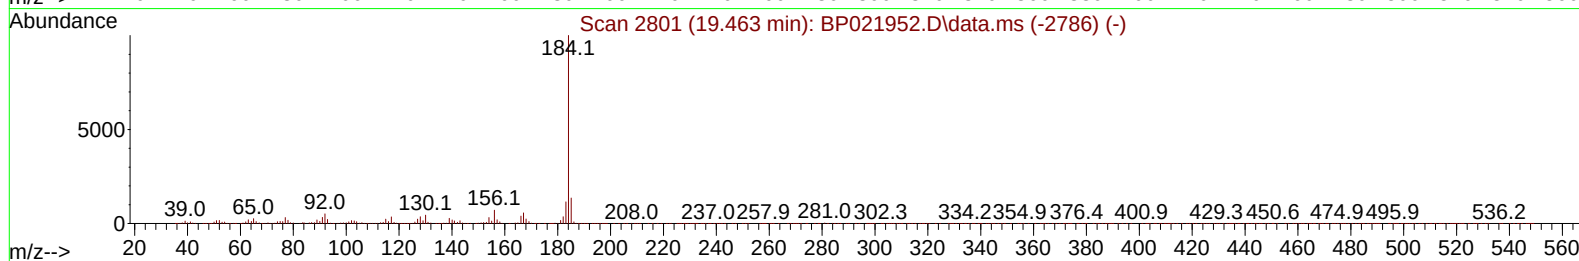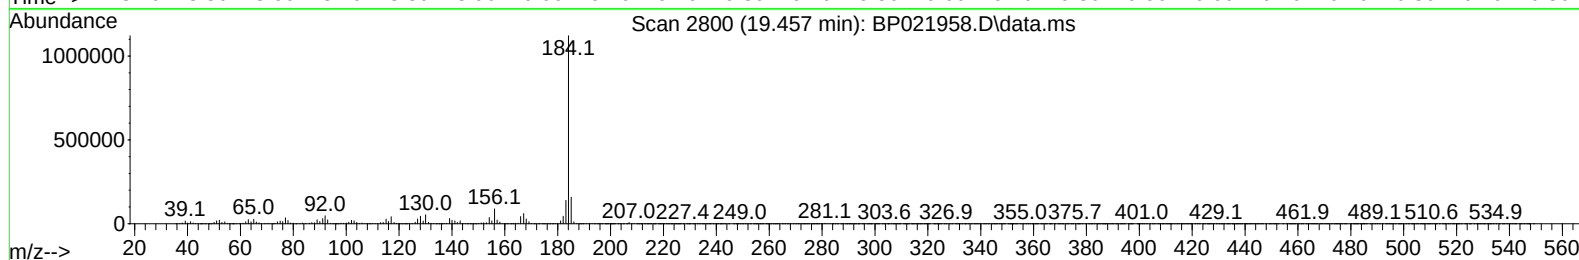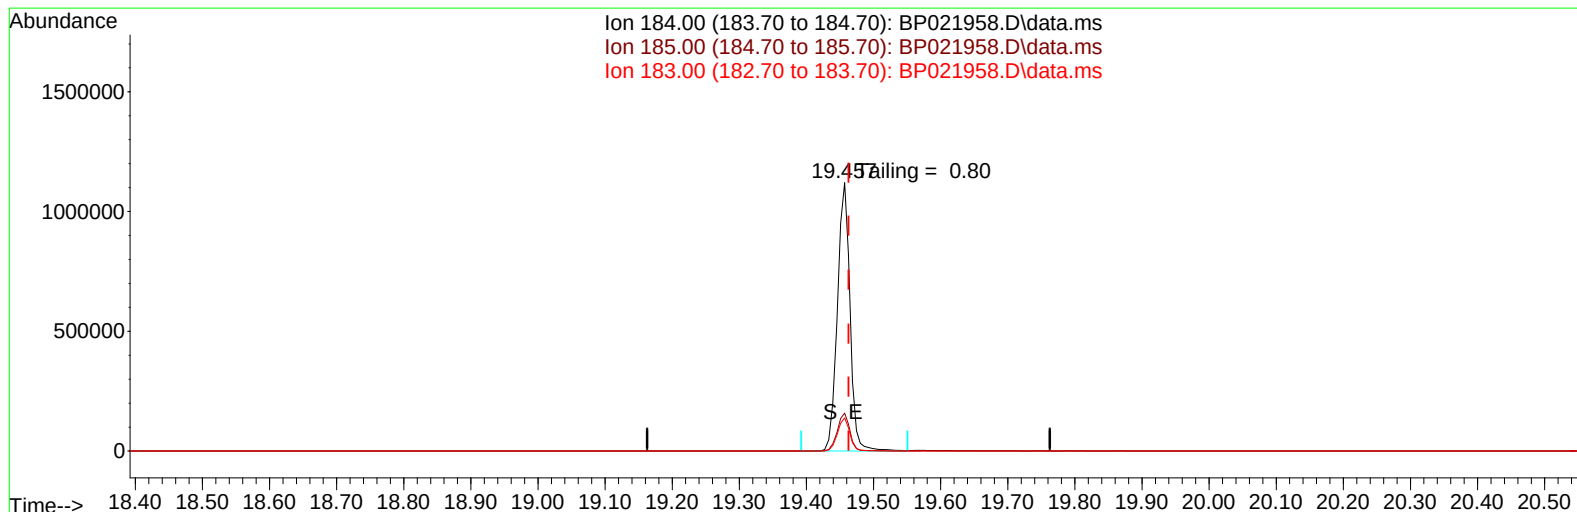

TIC: BP021958.D\data.ms

(77) Benzidine

19.457min (-0.006) 3881466.98 ng

response 1470436

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.16
183.00	11.50	12.39
0.00	0.00	0.00