
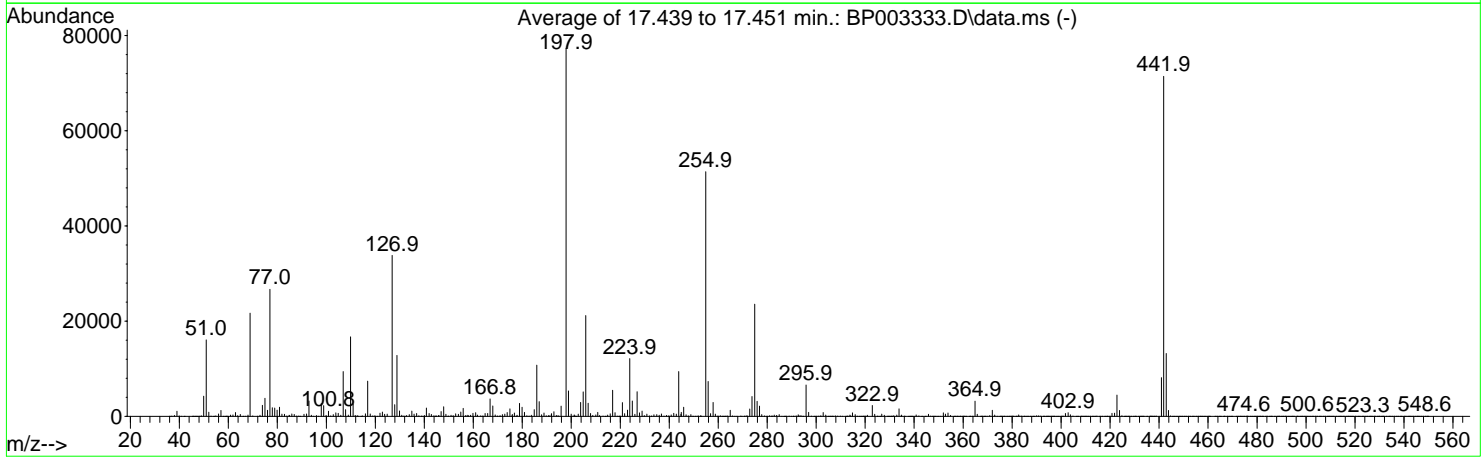


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092220\
 Data File : BP003333.D
 Acq On : 22 Sep 2020 11:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampled :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 12:48:08 2020

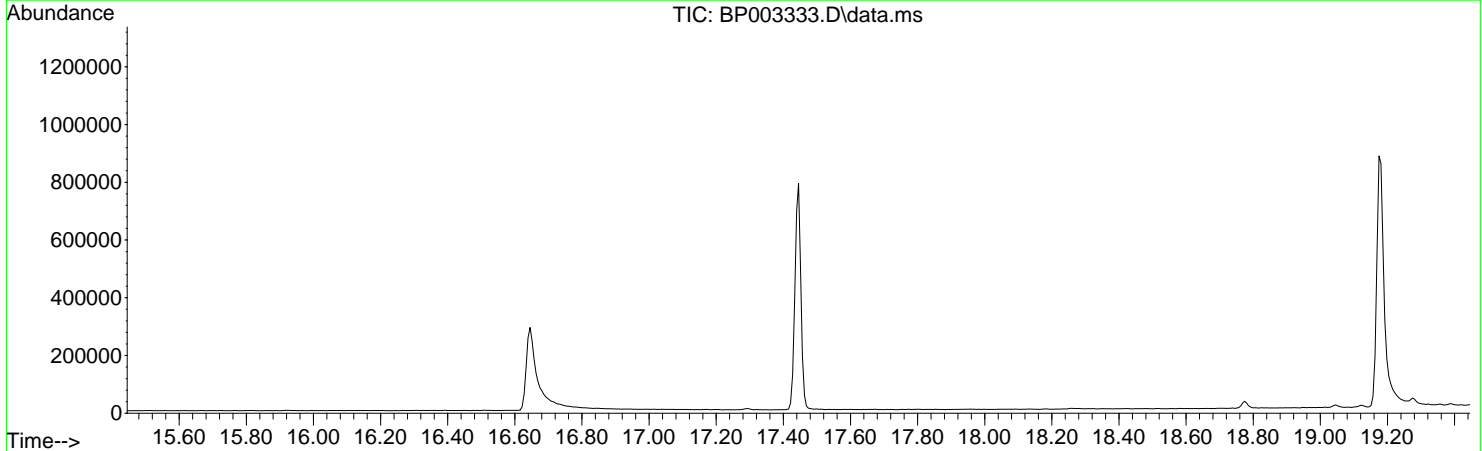

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.8	16071	PASS
68	69	0.00	2	1.2	263	PASS
69	198	0.00	100	28.1	21690	PASS
70	69	0.00	2	0.4	91	PASS
127	198	10	80	43.7	33804	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77278	PASS
199	198	5	9	6.9	5345	PASS
275	198	10	60	30.5	23560	PASS
365	198	1	100	4.2	3211	PASS
441	198	0.01	100	10.5	8152	PASS
442	198	50	100	92.4	71435	PASS
443	442	15	24	18.5	13227	PASS