
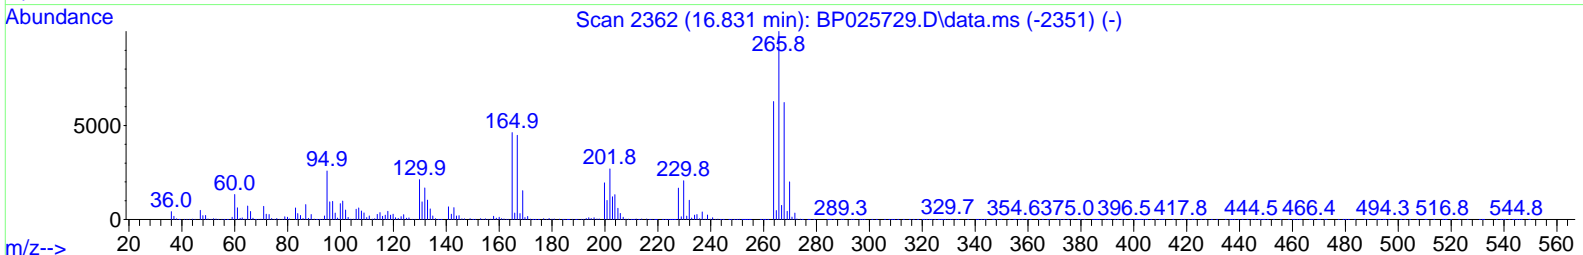
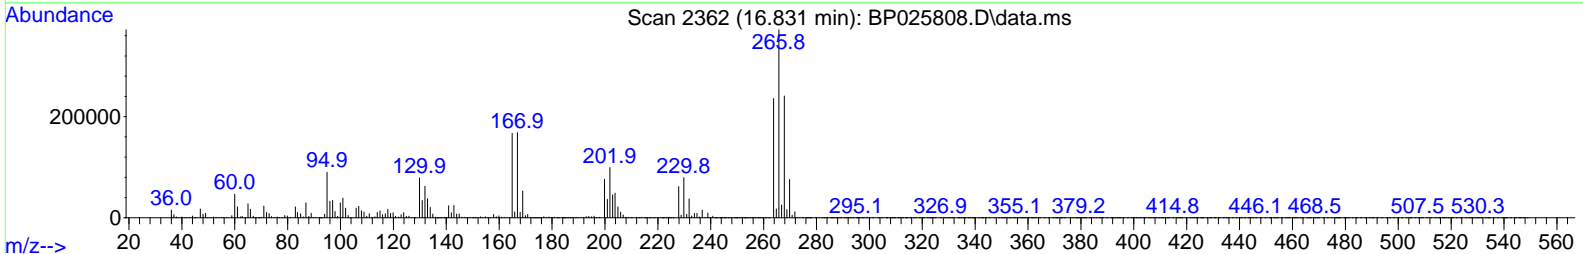


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092225\
 Data File : BP025808.D
 Acq On : 22 Sep 2025 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 11:14:36 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 16:45:04 2025
 Response via : Initial Calibration

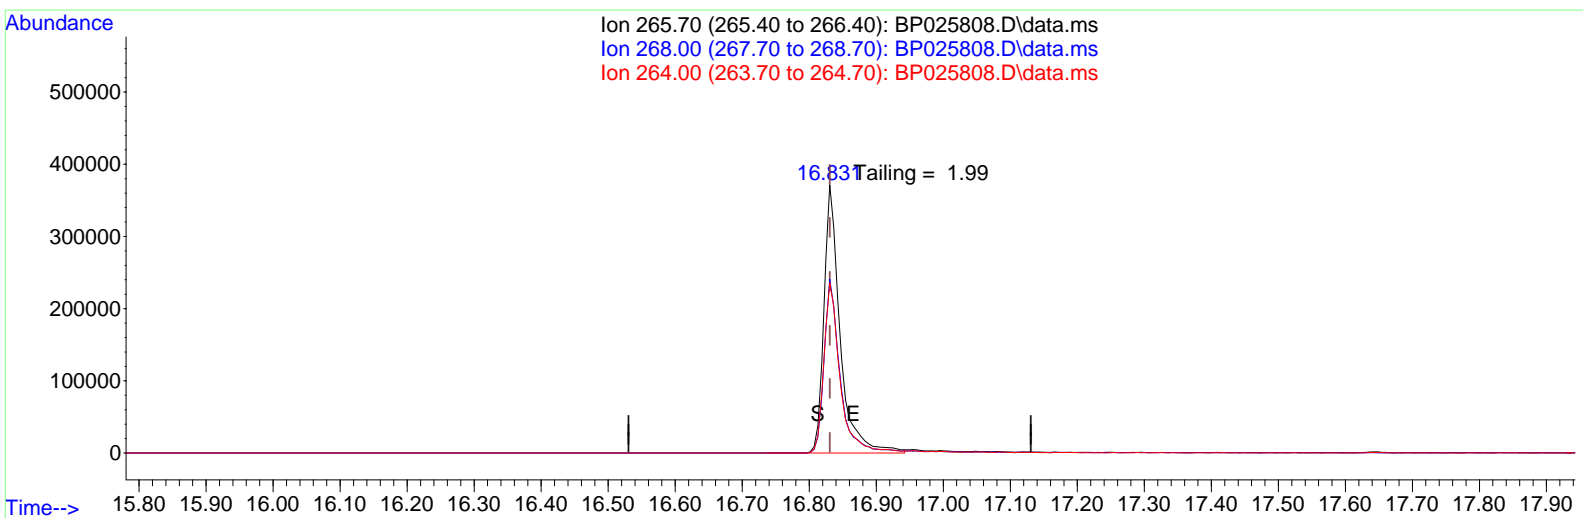

TIC: BP025808.D\data.ms

(70) Pentachlorophenol (C)




16.831min (+ 0.000) 2091525.94 ng

response 625723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.74
264.00	62.70	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092225\
 Data File : BP025808.D
 Acq On : 22 Sep 2025 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 11:14:36 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 16:45:04 2025
 Response via : Initial Calibration

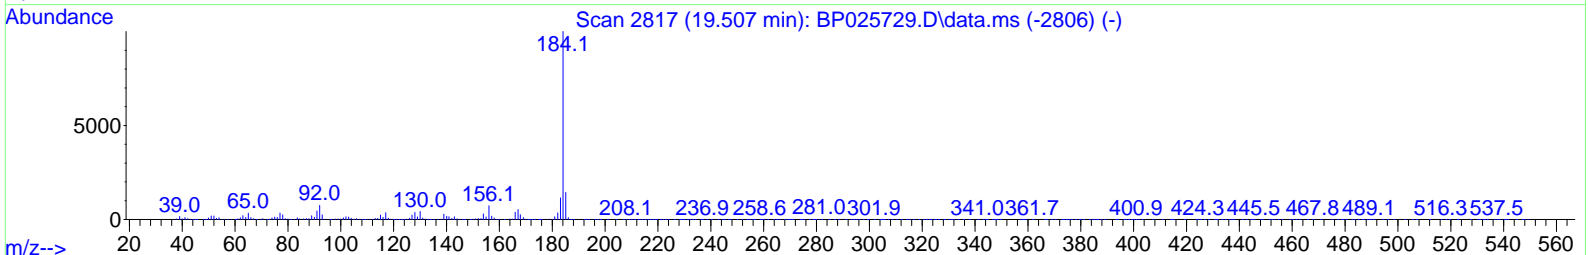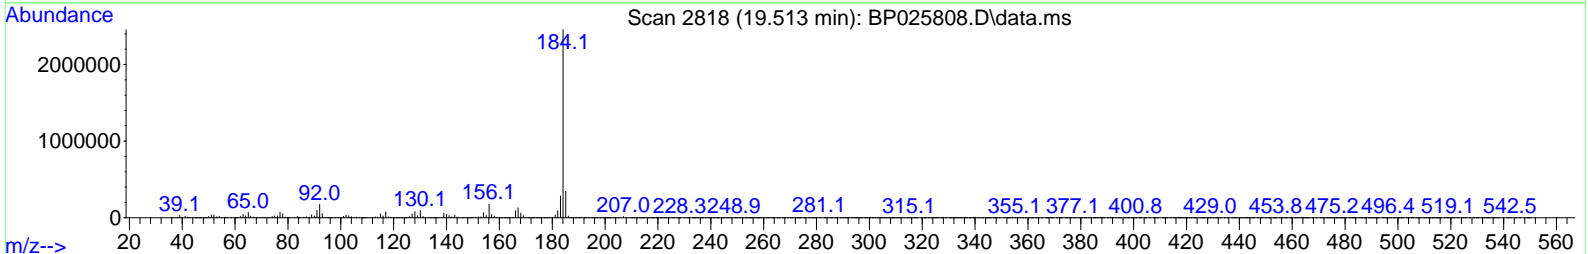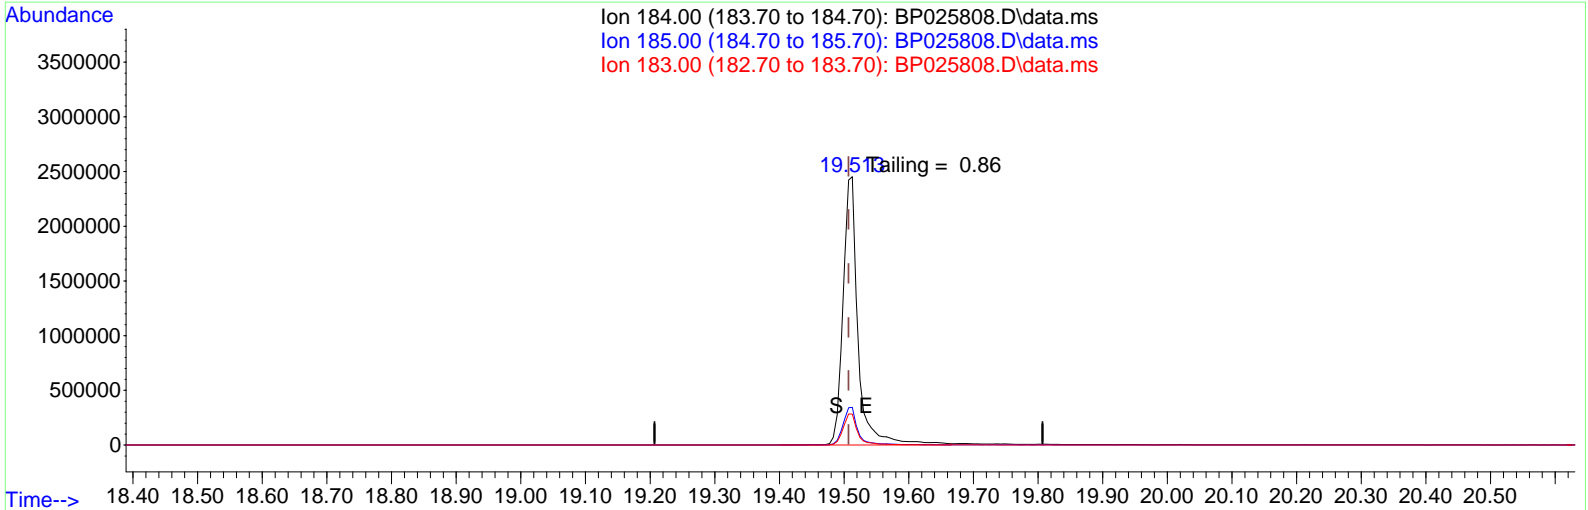

TIC: BP025808.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 1520849.41 ng

response 3942774

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.02
183.00	11.50	11.54
0.00	0.00	0.00