
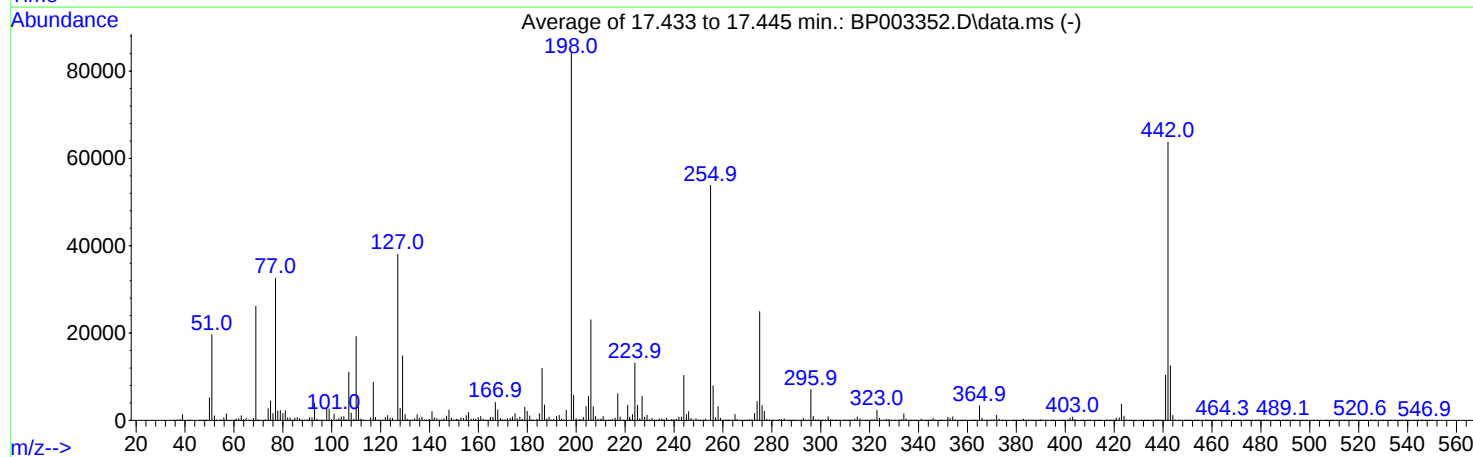


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092320\
 Data File : BP003352.D
 Acq On : 23 Sep 2020 11:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 12:48:08 2020

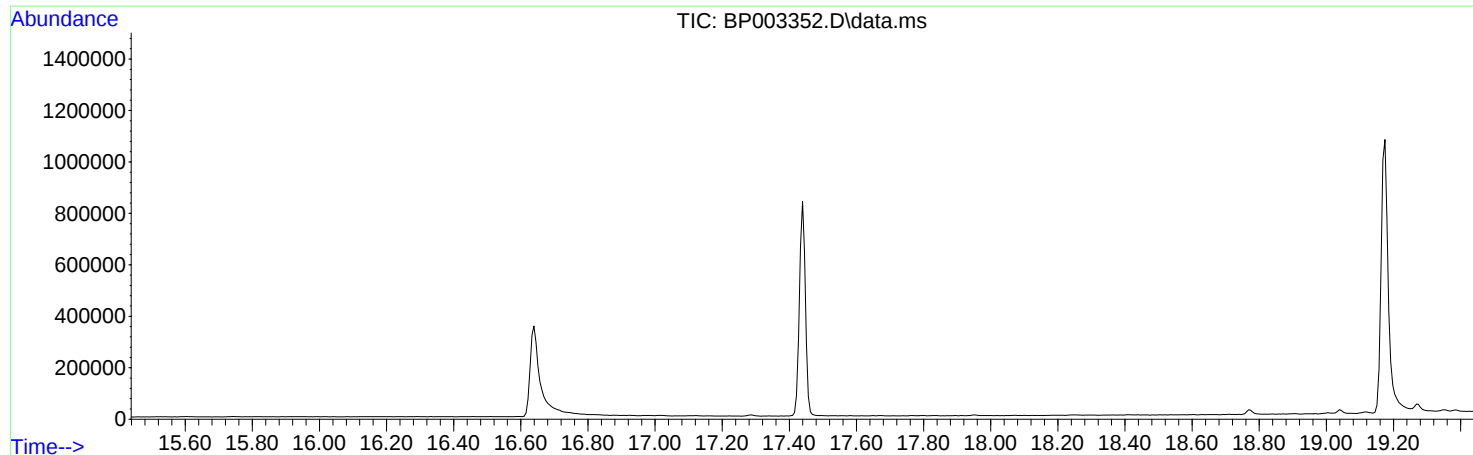

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.3	19603	PASS
68	69	0.00	2	1.9	492	PASS
69	198	0.00	100	31.0	26128	PASS
70	69	0.00	2	0.6	144	PASS
127	198	10	80	45.1	38017	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84259	PASS
199	198	5	9	6.8	5729	PASS
275	198	10	60	29.6	24936	PASS
365	198	1	100	4.0	3376	PASS
441	198	0.01	100	12.3	10347	PASS
442	198	50	100	75.6	63725	PASS
443	442	15	24	19.6	12518	PASS