

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
 Data File : BP007144.D
 Acq On : 24 Sep 2021 02:08
 Operator : CG/JU
 Sample : M3870-01 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	398	405	417	rBV	1713414	2645893	46.60%	6.288%
2	7.057	668	675	692	rBV	1646678	2711840	47.76%	6.444%
3	7.893	809	817	824	rBV	1191987	1886616	33.23%	4.483%
4	9.051	1006	1014	1023	rBV	1013755	1692346	29.81%	4.022%
5	10.481	1250	1257	1266	rBV	74983	153144	2.70%	0.364%
6	10.692	1284	1293	1303	rBV	1574630	2662908	46.90%	6.328%
7	13.145	1703	1710	1722	rBV	2918886	4303289	75.80%	10.226%
8	14.363	1911	1917	1924	rBV6	20780	60839	1.07%	0.145%
9	14.522	1937	1944	1957	rVB	2439260	3564567	62.78%	8.471%
10	16.010	2190	2197	2206	rBV	2241998	3233940	56.96%	7.685%
11	17.268	2405	2411	2417	rBV	2923155	4086947	71.98%	9.712%
12	18.157	2558	2562	2569	rBV2	191356	301156	5.30%	0.716%
13	19.274	2749	2752	2756	rBV	175966	215293	3.79%	0.512%
14	19.827	2841	2846	2850	rBV	4734360	5677536	100.00%	13.492%
15	21.351	3101	3105	3110	rVB	3323778	4218192	74.30%	10.024%
16	23.762	3510	3515	3523	rVB2	2233604	4665540	82.18%	11.087%




Sum of corrected areas: 42080046

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
Data File : BP007144.D
Acq On : 24 Sep 2021 02:08
Operator : CG/JU
Sample : M3870-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-C

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

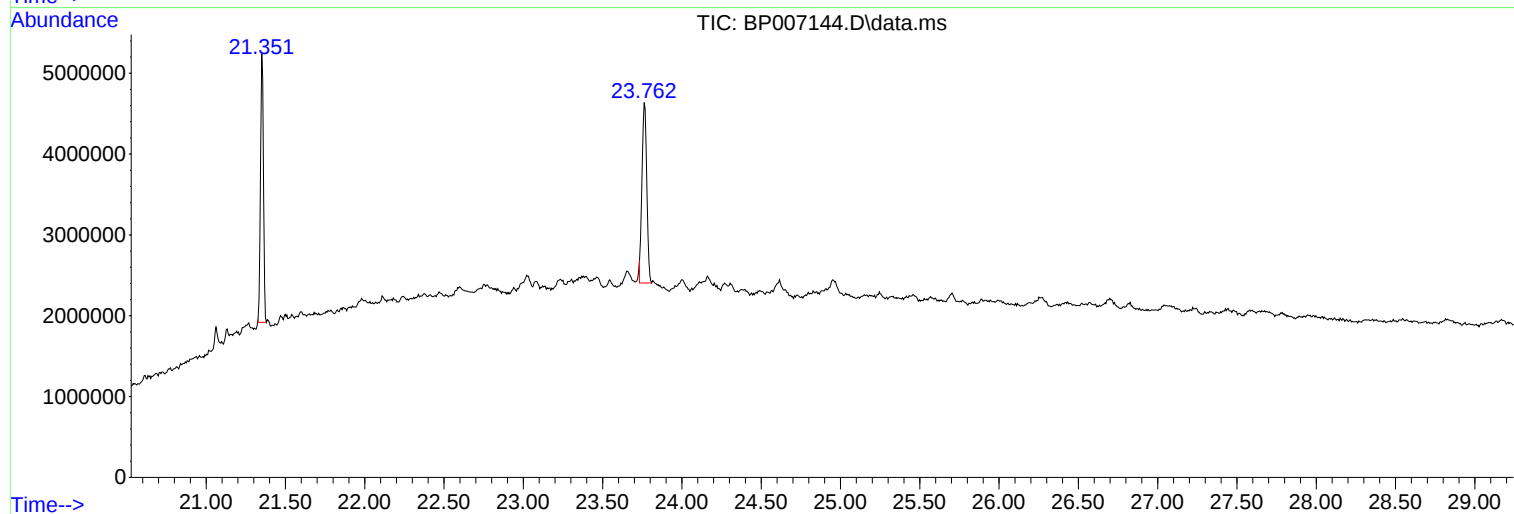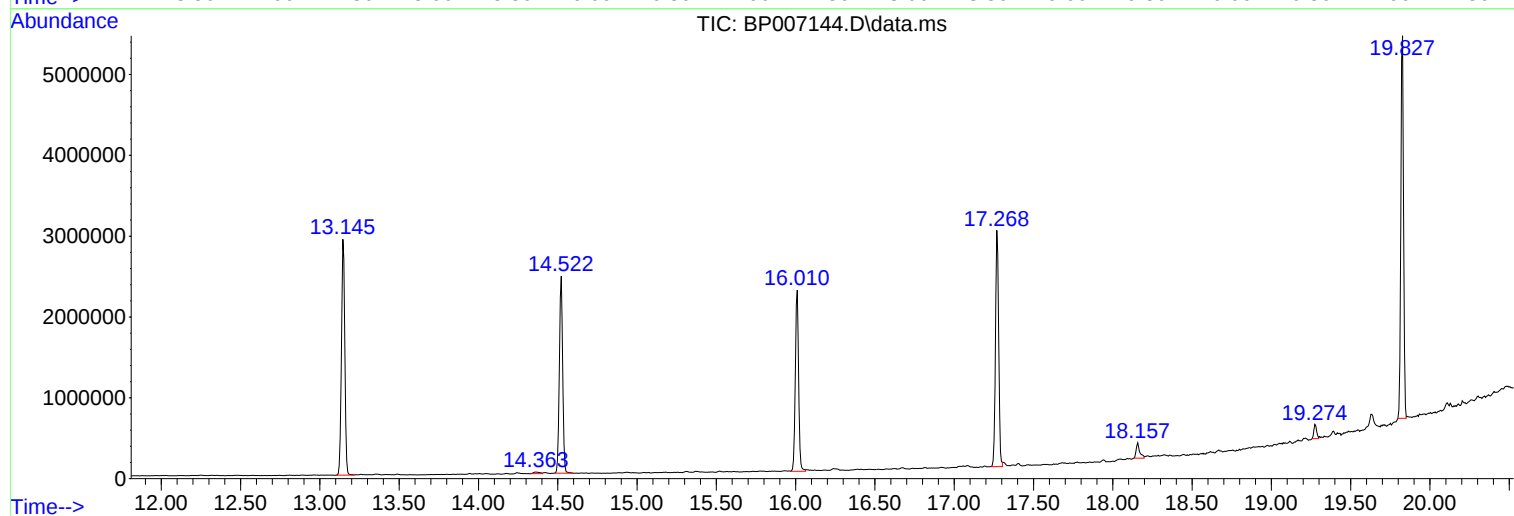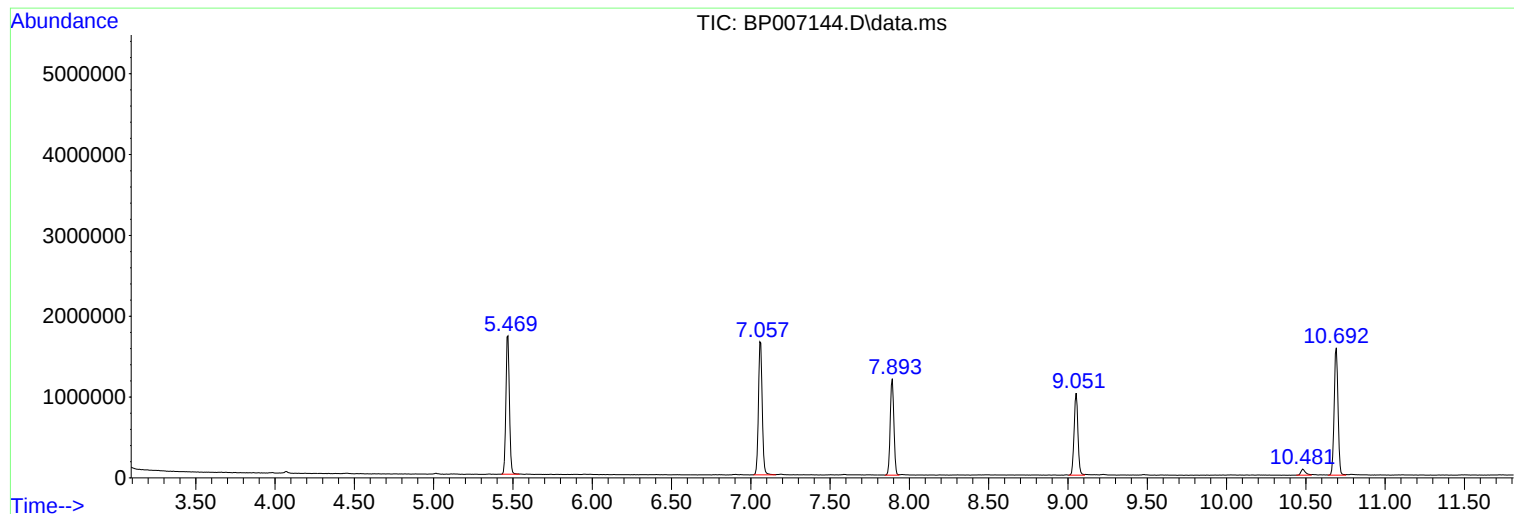

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
Data File : BP007144.D
Acq On : 24 Sep 2021 02:08
Operator : CG/JU
Sample : M3870-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-C

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
Data File : BP007144.D
Acq On : 24 Sep 2021 02:08
Operator : CG/JU
Sample : M3870-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-C

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
