

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
 Data File : BP007148.D
 Acq On : 24 Sep 2021 04:24
 Operator : CG/JU
 Sample : M3881-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OK-01-092221

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	398	405	415	rVB	348328	534209	12.96%	2.123%
2	7.063	669	676	689	rVB	323164	536668	13.02%	2.133%
3	7.893	807	817	825	rBV	1188240	1880410	45.61%	7.473%
4	9.052	1007	1014	1024	rBV	185608	333793	8.10%	1.327%
5	10.481	1252	1257	1268	rBV	63479	141199	3.42%	0.561%
6	10.693	1284	1293	1304	rBV	1592862	2634273	63.90%	10.469%
7	13.145	1702	1710	1719	rBV	605990	915374	22.20%	3.638%
8	14.522	1935	1944	1952	rBV	2262225	3522146	85.43%	13.997%
9	16.010	2192	2197	2205	rBV	428859	609181	14.78%	2.421%
10	17.275	2405	2412	2417	rBV	2751948	4000855	97.05%	15.900%
11	17.316	2417	2419	2424	rVB	129437	146948	3.56%	0.584%
12	17.410	2431	2435	2438	rVB	39793	51896	1.26%	0.206%
13	18.157	2559	2562	2565	rBV2	60497	72770	1.77%	0.289%
14	19.280	2749	2753	2758	rBV	262095	346628	8.41%	1.378%
15	19.633	2810	2813	2818	rVB	205692	268087	6.50%	1.065%
16	19.827	2842	2846	2851	rBV	950816	1129146	27.39%	4.487%
17	21.357	3102	3106	3110	rVB	3223157	3916512	95.00%	15.565%
18	23.774	3511	3517	3526	rVB2	2099794	4122666	100.00%	16.384%


Sum of corrected areas: 25162761

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
Data File : BP007148.D
Acq On : 24 Sep 2021 04:24
Operator : CG/JU
Sample : M3881-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-01-092221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

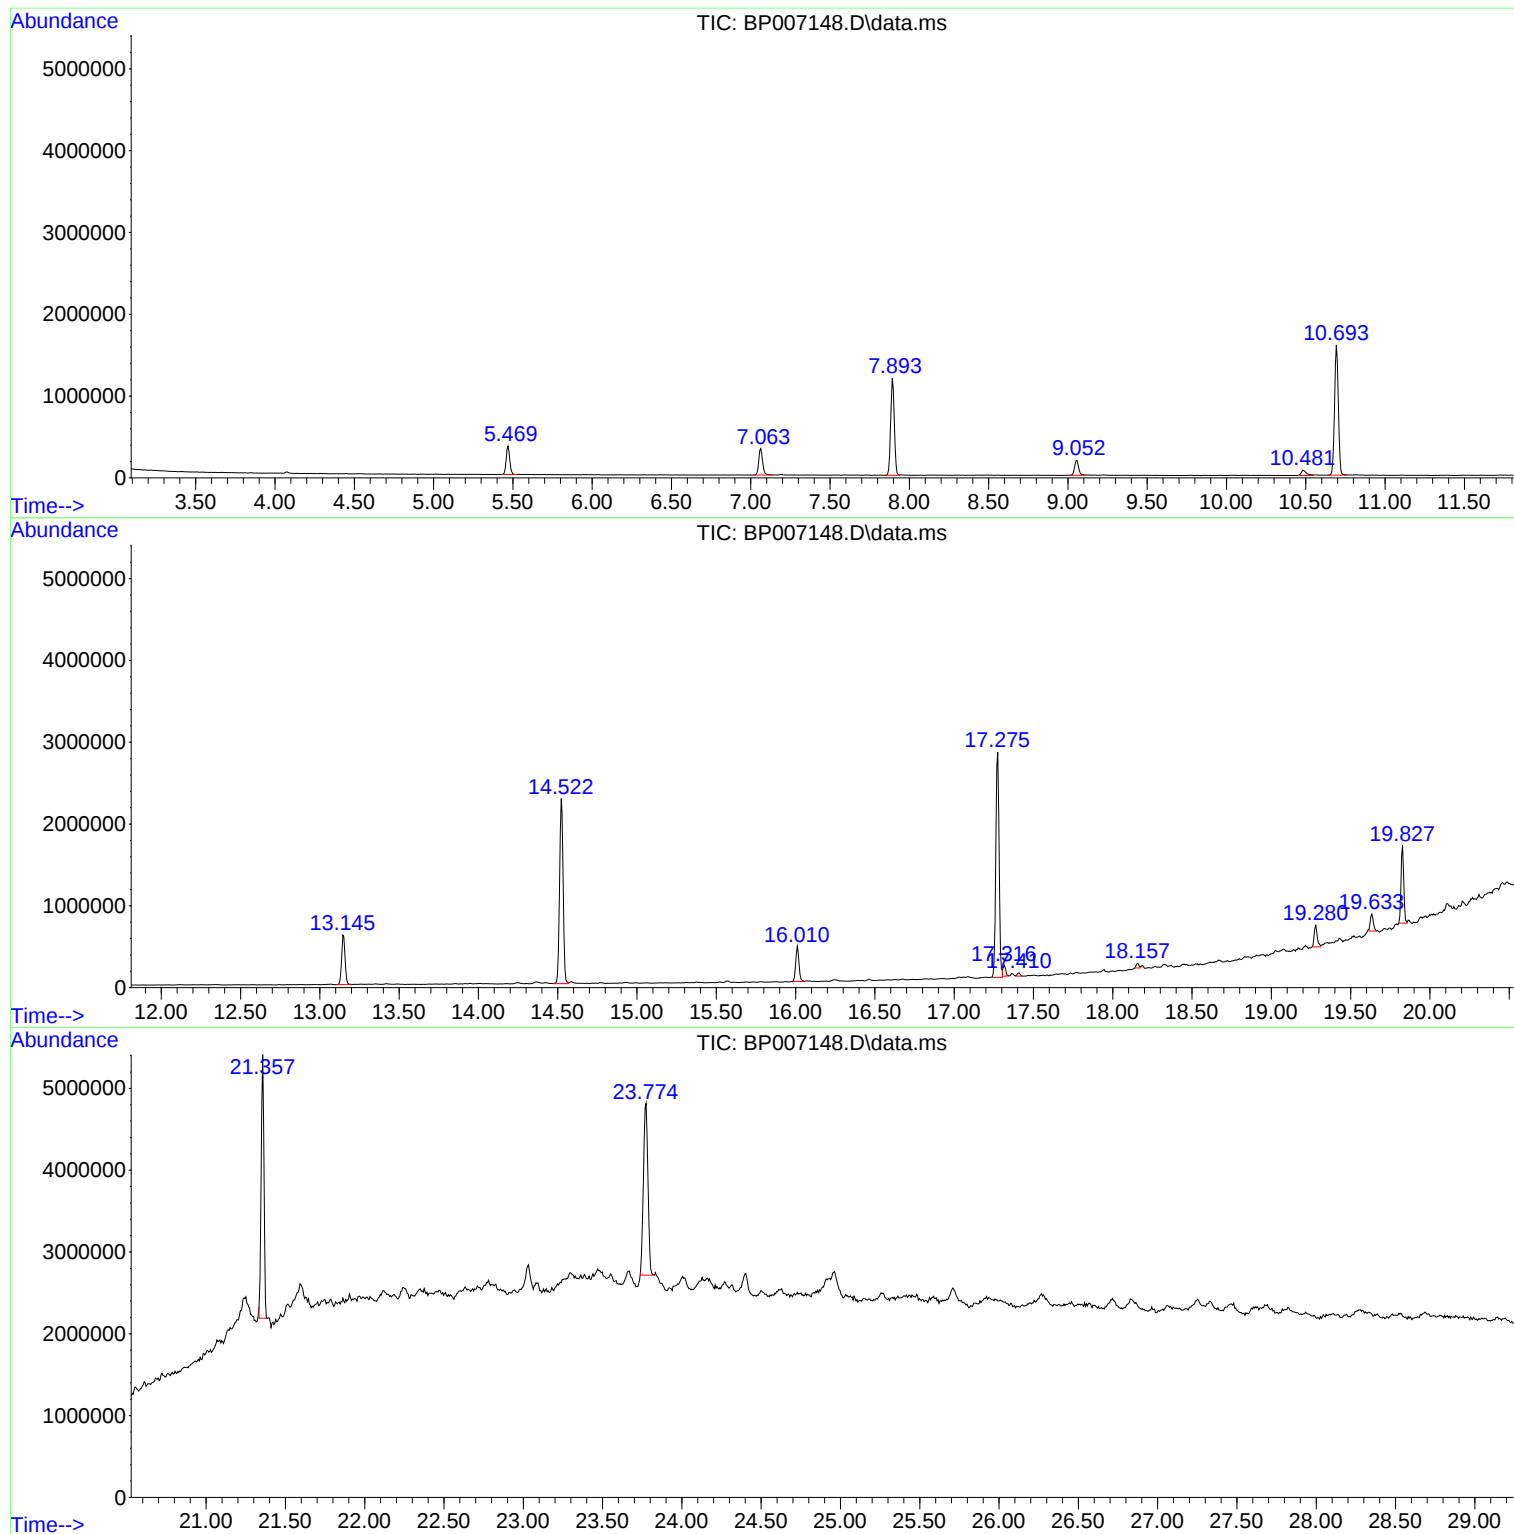

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
Data File : BP007148.D
Acq On : 24 Sep 2021 04:24
Operator : CG/JU
Sample : M3881-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-01-092221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
Data File : BP007148.D
Acq On : 24 Sep 2021 04:24
Operator : CG/JU
Sample : M3881-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-01-092221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
