
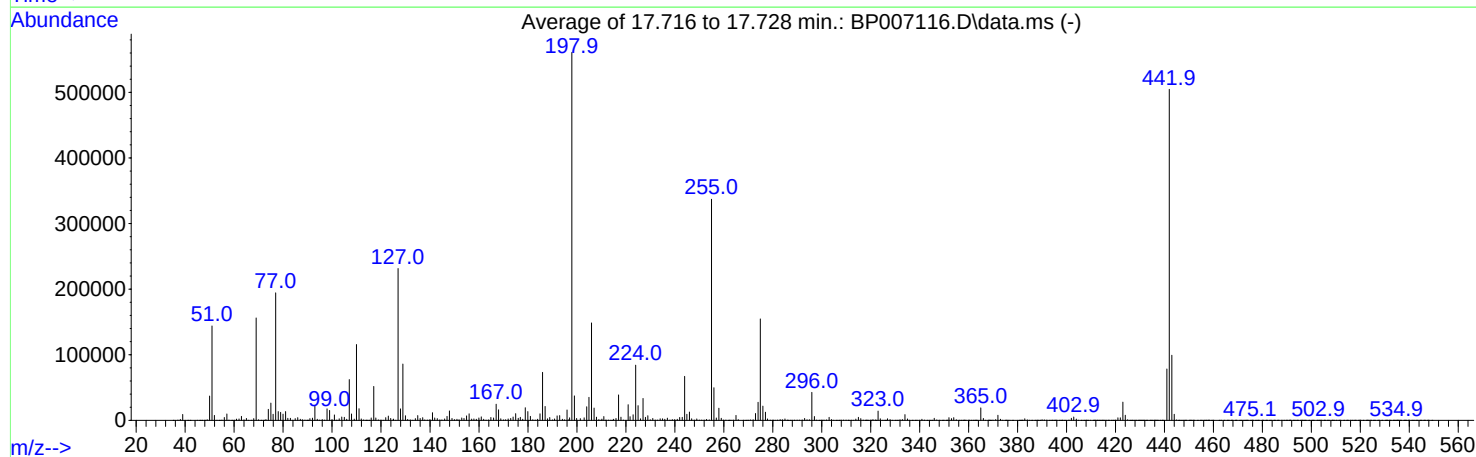


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
 Data File : BP007116.D
 Acq On : 23 Sep 2021 09:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 23 11:17:25 2021

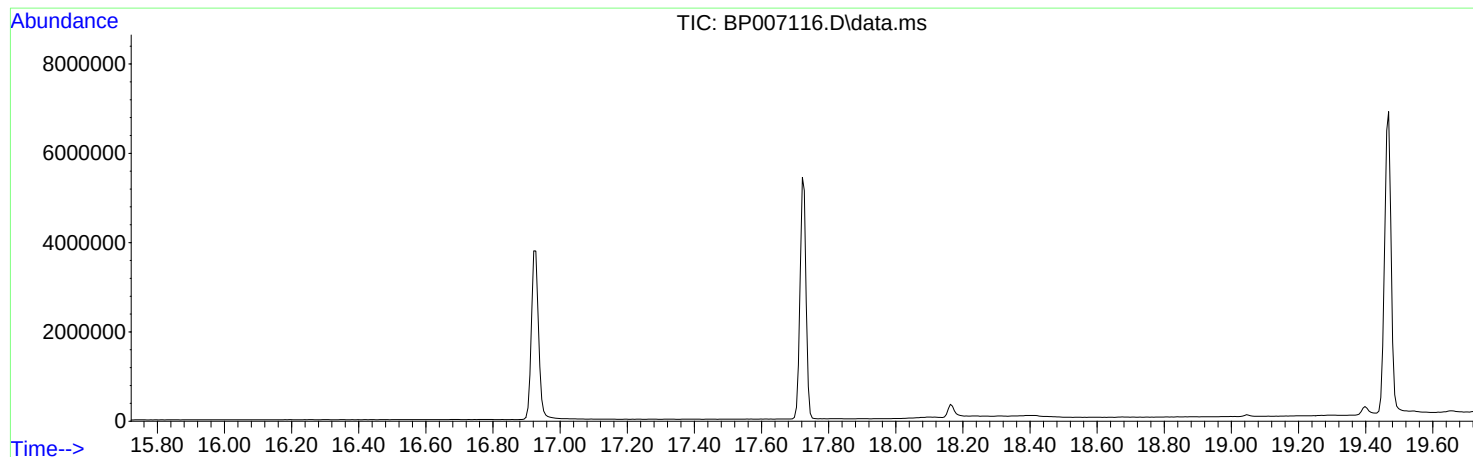




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	144000	PASS
68	69	0.00	2	1.7	2719	PASS
69	198	0.00	100	27.9	156279	PASS
70	69	0.00	2	0.6	882	PASS
127	198	10	80	41.3	231564	PASS
197	198	0.00	2	0.7	3889	PASS
198	198	100	100	100.0	560870	PASS
199	198	5	9	6.7	37439	PASS
275	198	10	60	27.6	154809	PASS
365	198	1	100	3.4	19094	PASS
441	198	0.01	100	14.0	78379	PASS
442	442	100	100	100.0	504671	PASS
443	442	15	24	19.7	99278	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
Data File : BP007116.D
Acq On : 23 Sep 2021 09:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 23 11:11:41 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 16:50:24 2021
Response via : Initial Calibration

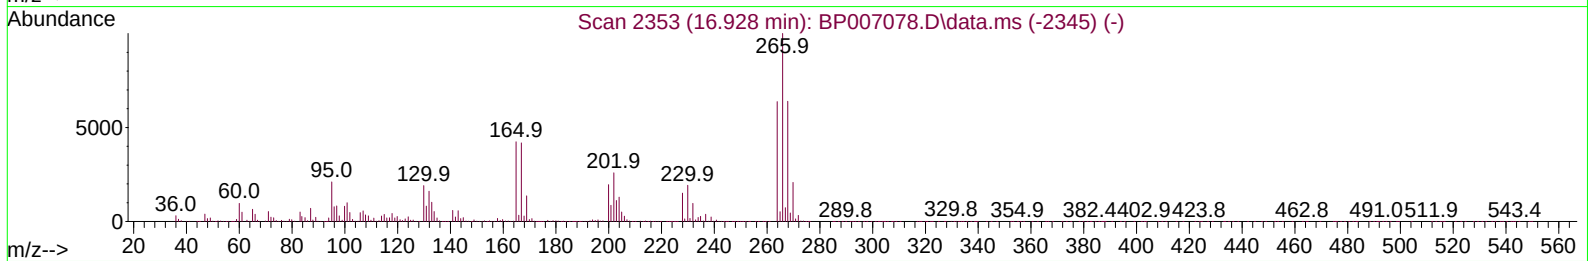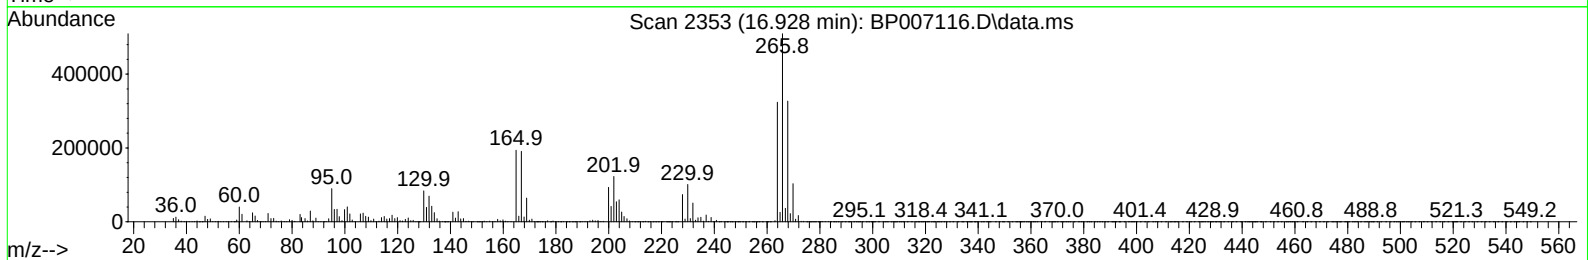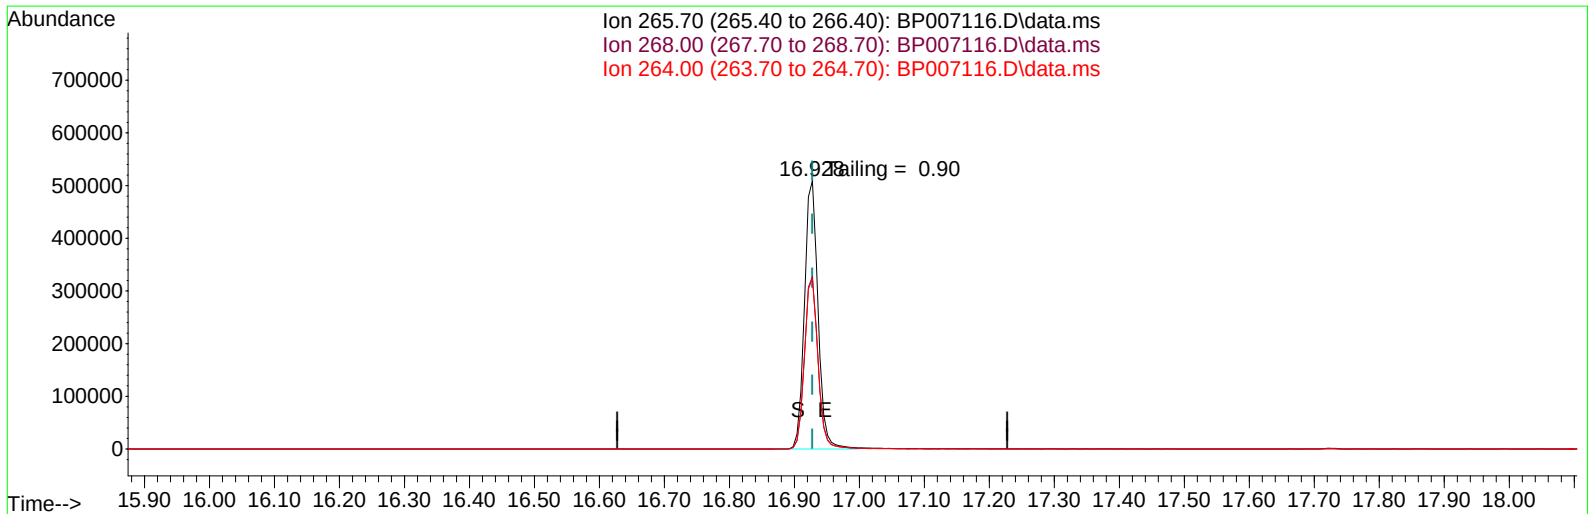

TIC: BP007116.D\data.ms

(70) Pentachlorophenol (C)

16.928min (-0.000) 1546174.70 ng




response 744374

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.15
264.00	62.90	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
 Data File : BP007116.D
 Acq On : 23 Sep 2021 09:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 23 11:11:41 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 16:50:24 2021
 Response via : Initial Calibration

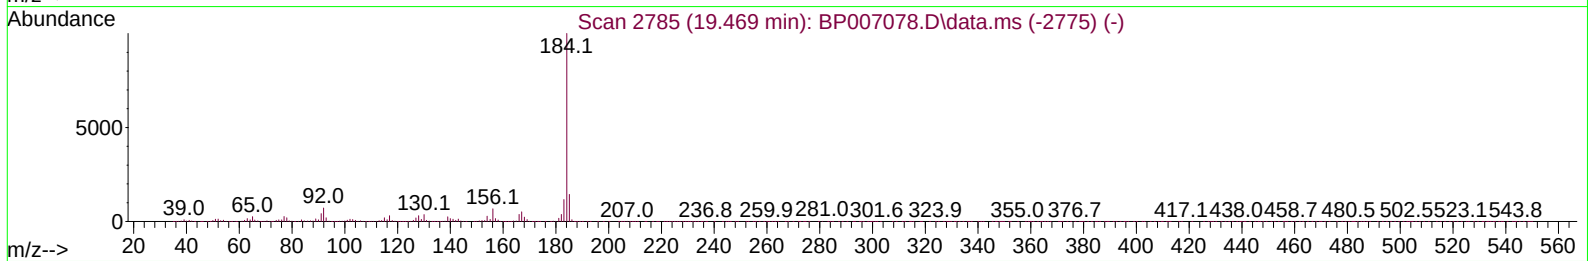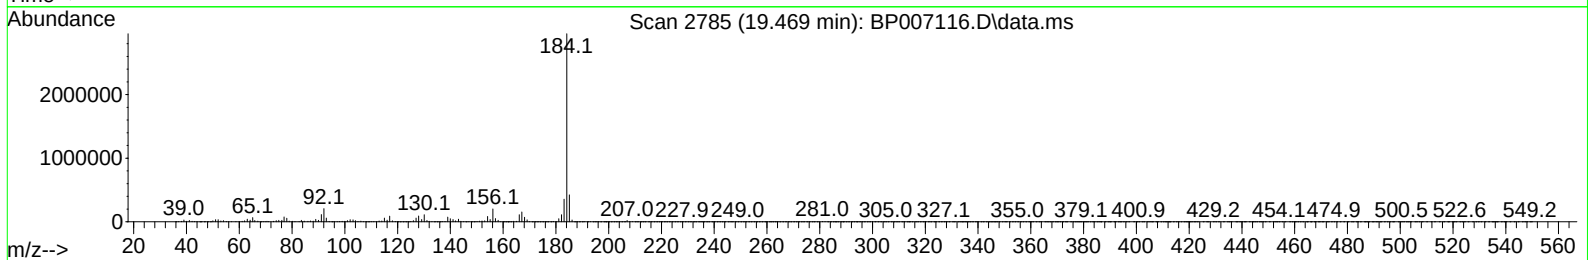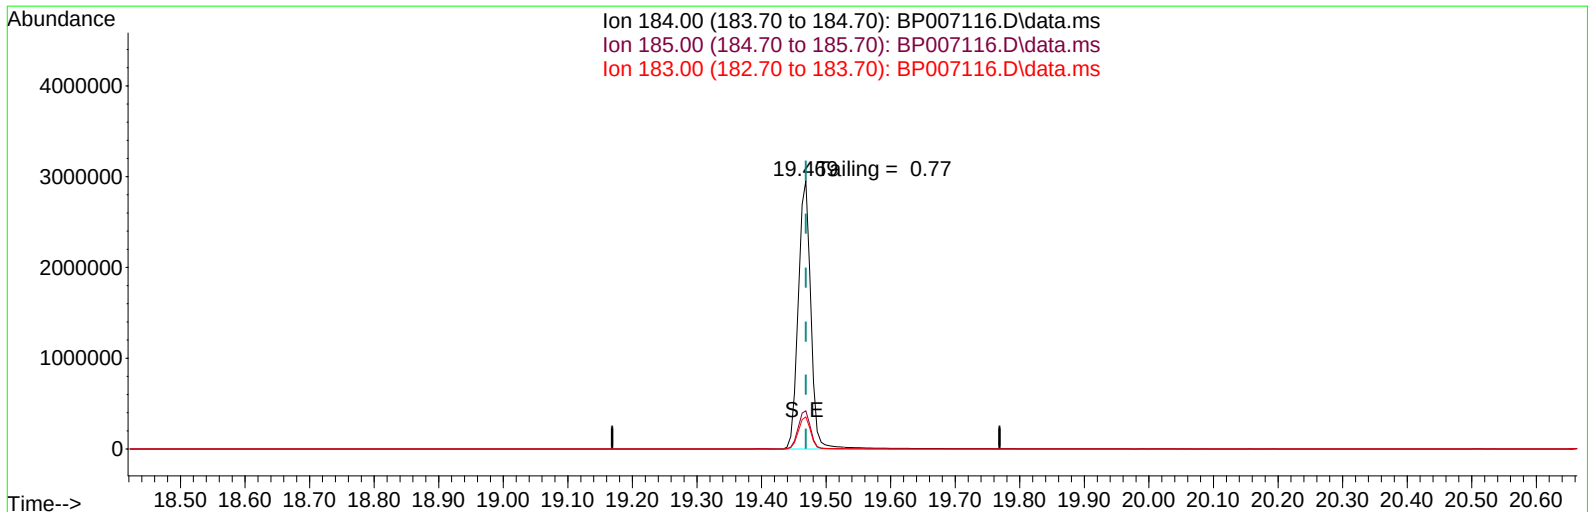

TIC: BP007116.D\data.ms

(77) Benzidine

19.469min (-0.000) 412798.49 ng

response 4034130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.29
183.00	11.90	12.00
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
9/23/2021	BNA_P	<u>BP007116.D</u>
Compound Name	Response	Retention Time
DDT	2041010	20.66
DDD	12641	20.23
DDE	2939	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15580	2056590	0.76