
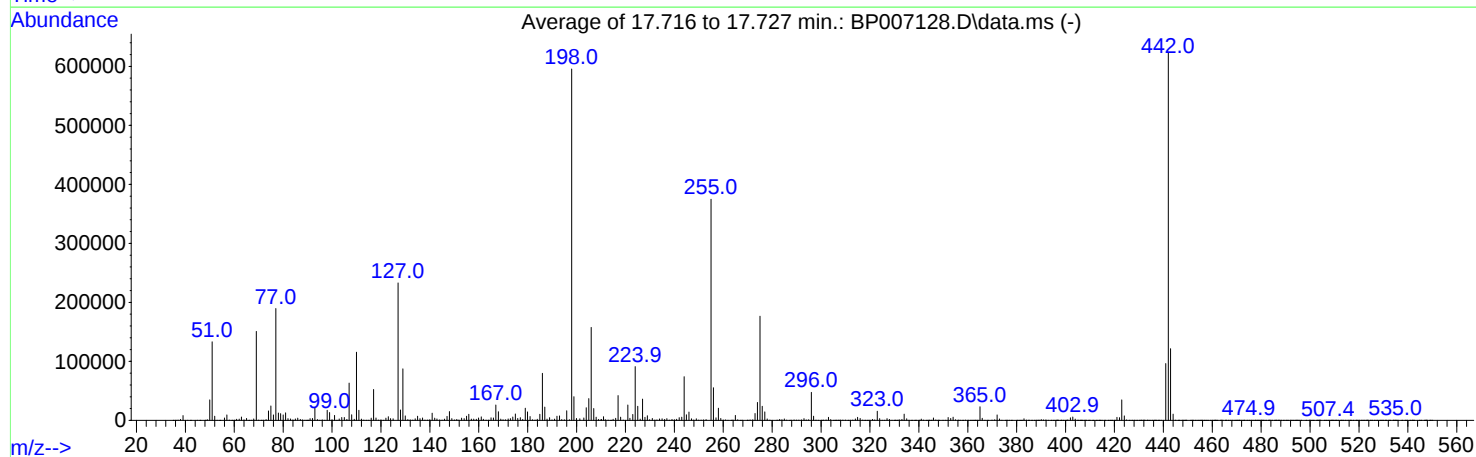


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
 Data File : BP007128.D
 Acq On : 23 Sep 2021 16:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 23 11:17:25 2021

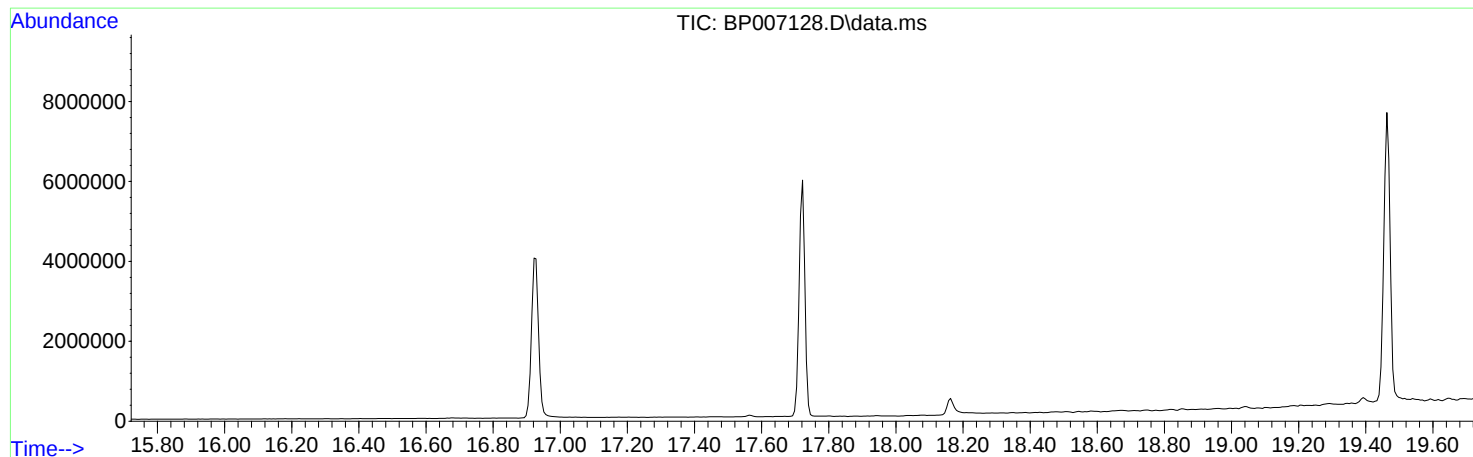




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	133115	PASS
68	69	0.00	2	1.7	2564	PASS
69	198	0.00	100	25.3	150884	PASS
70	69	0.00	2	0.4	590	PASS
127	198	10	80	39.1	233102	PASS
197	198	0.00	2	0.2	984	PASS
198	198	100	100	100.0	595474	PASS
199	198	5	9	6.8	40246	PASS
275	198	10	60	29.6	176467	PASS
365	198	1	100	3.9	23004	PASS
441	198	0.01	100	16.2	96293	PASS
442	442	100	100	100.0	623531	PASS
443	442	15	24	19.5	121508	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
 Data File : BP007128.D
 Acq On : 23 Sep 2021 16:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 23 17:44:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

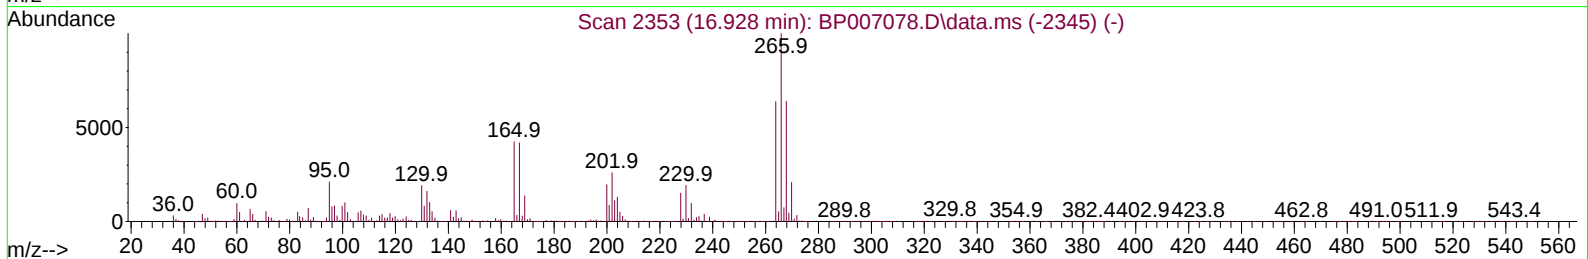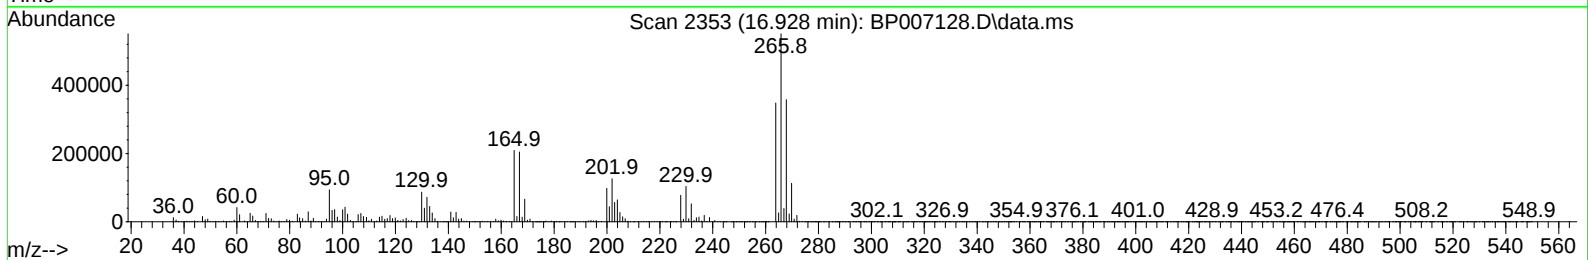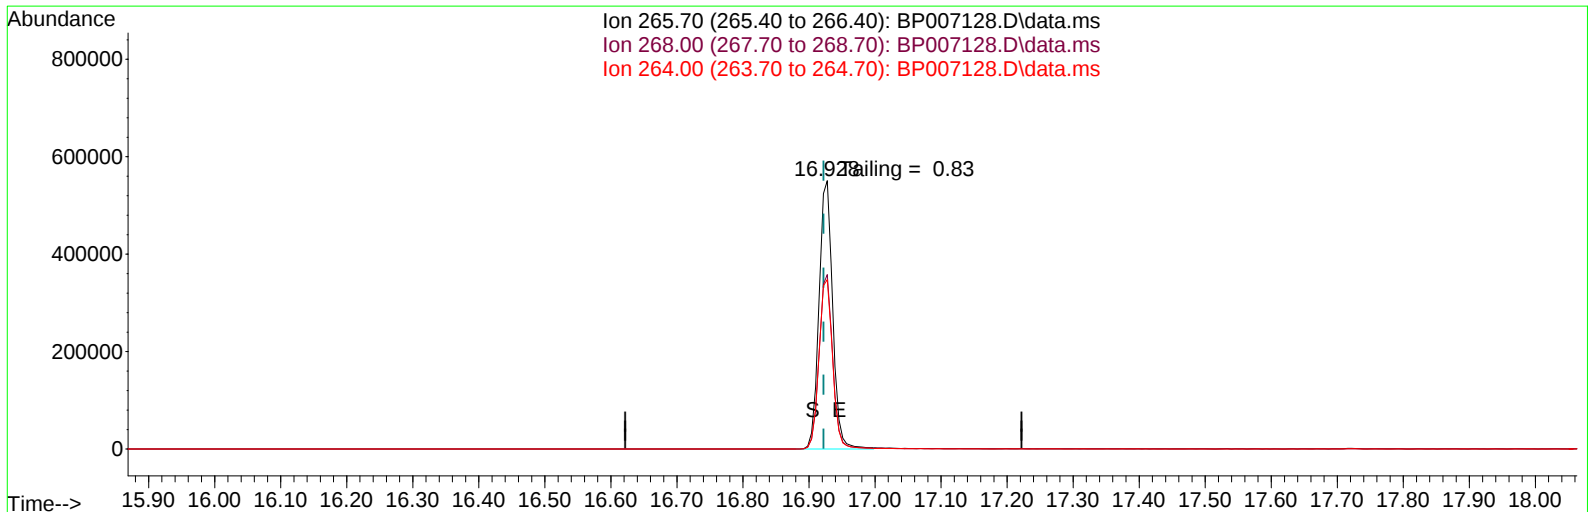

TIC: BP007128.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.006) 634169.74 ng




response 796663

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.98
264.00	62.90	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092321\
 Data File : BP007128.D
 Acq On : 23 Sep 2021 16:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 23 17:44:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

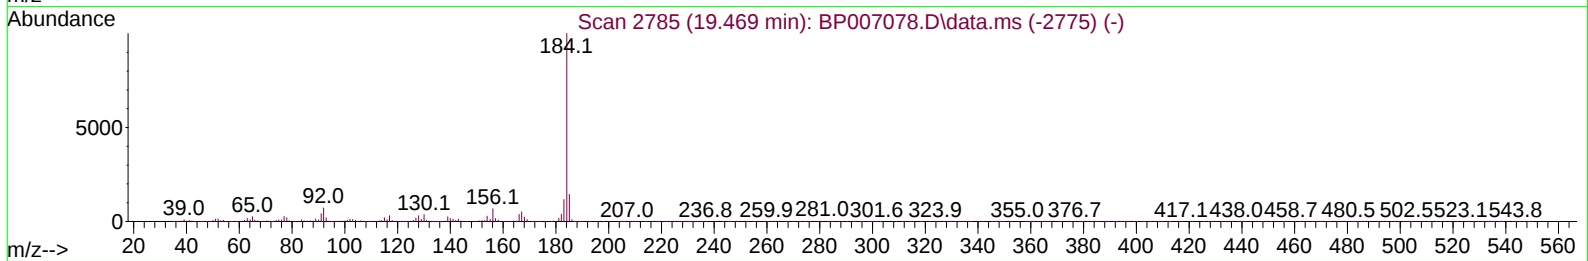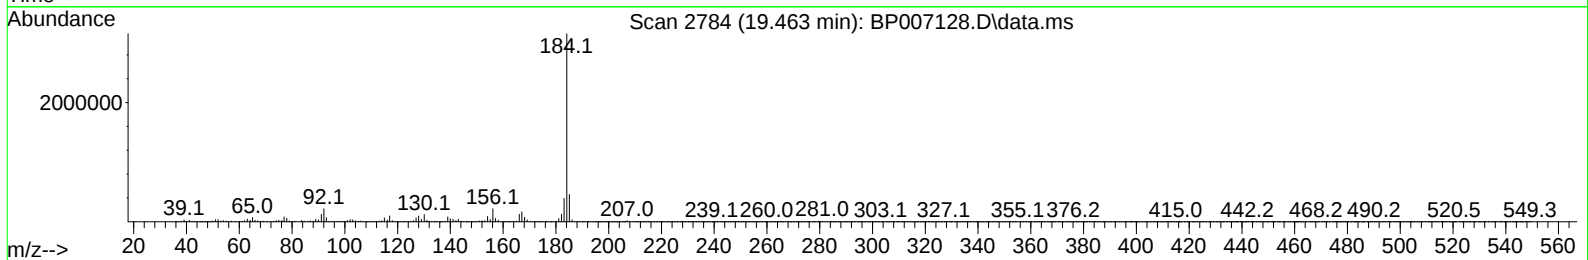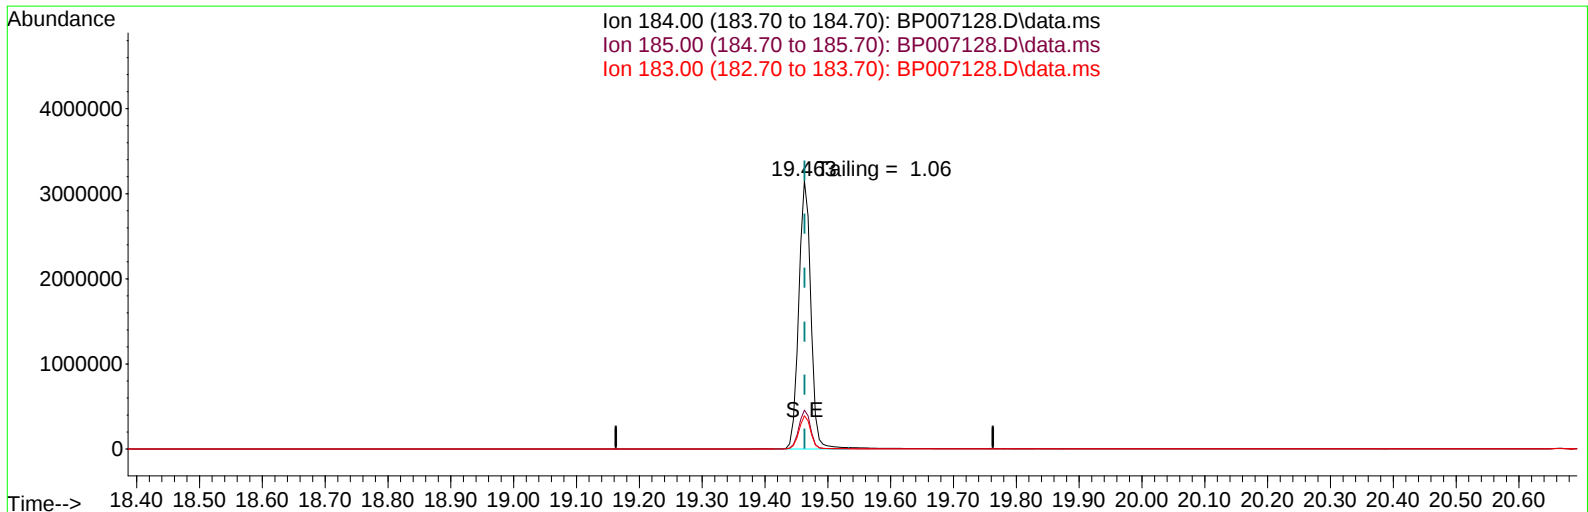

TIC: BP007128.D\data.ms

(77) Benzidine

19.463min (-0.000) 238082.75 ng

response 4287560

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.48
183.00	11.90	12.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2021	BNA_P	BP007128.D
Compound Name	Response	Retention Time
DDT	2129757	20.66
DDD	23502	20.23
DDE	6753	19.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30255	2160012	1.40