
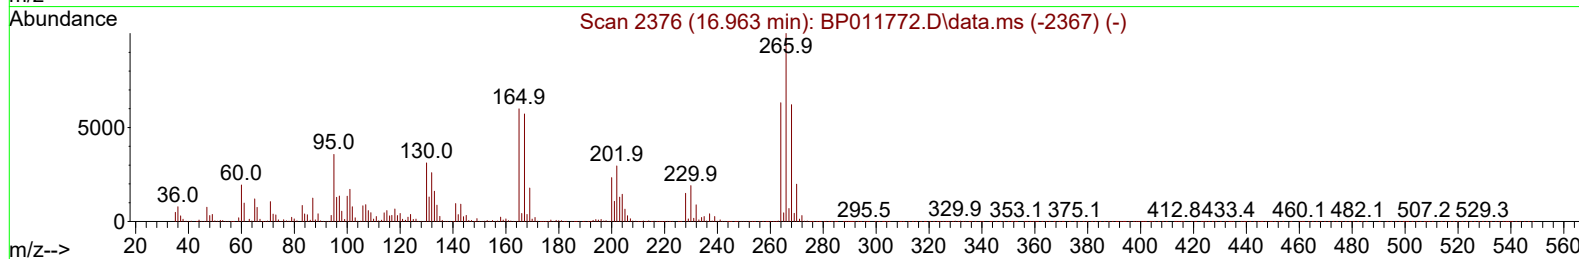
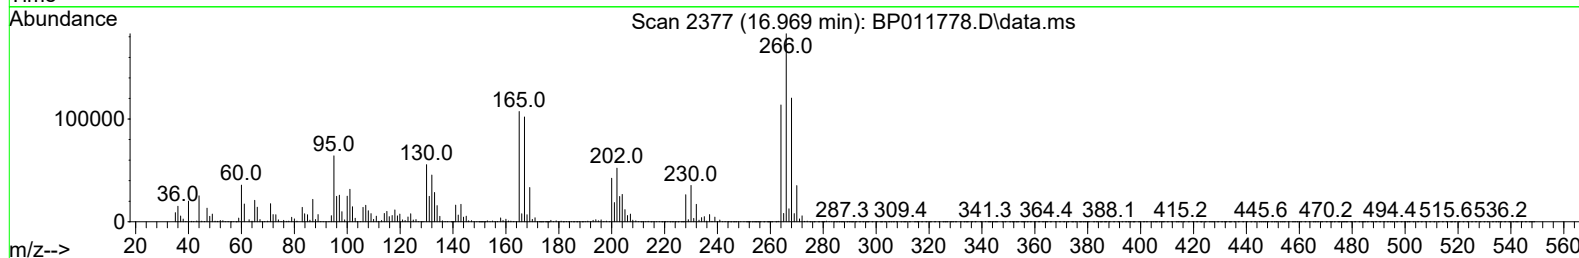


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
 Data File : BP011778.D
 Acq On : 23 Sep 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 04:45:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 02:45:14 2022
 Response via : Initial Calibration

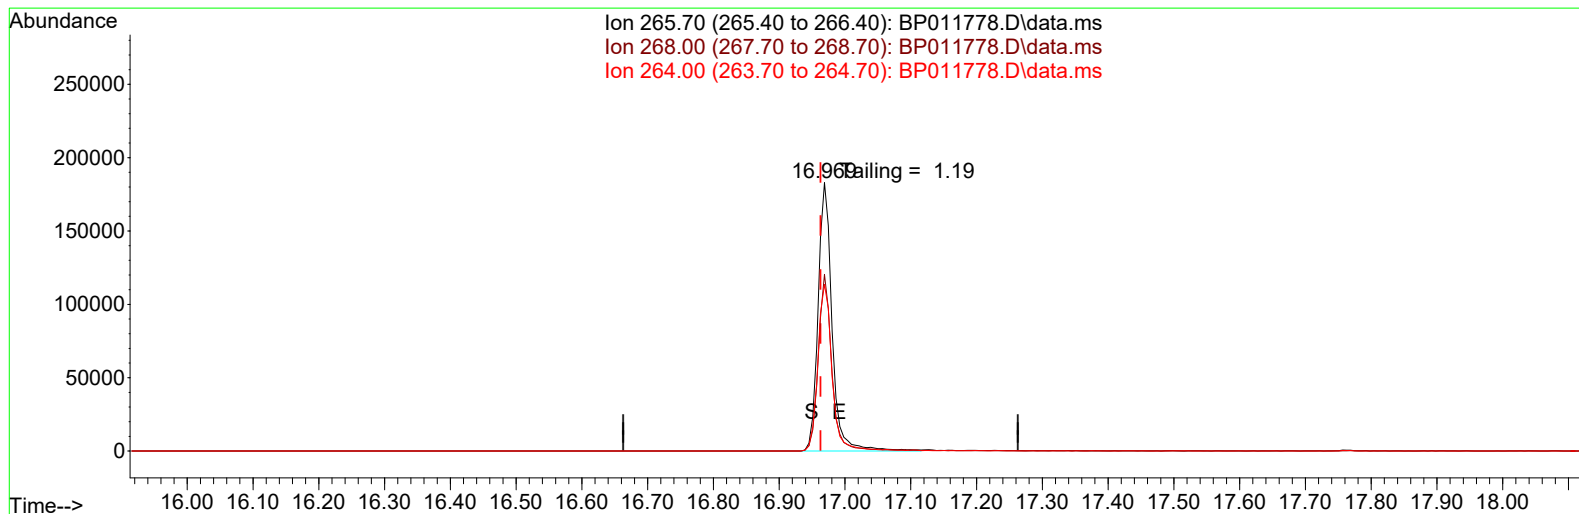

TIC: BP011778.D\data.ms

(70) Pentachlorophenol (C)




16.969min (+ 0.006) 2038145.44 ng

response 270351

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	65.81
264.00	63.20	62.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
Data File : BP011778.D
Acq On : 23 Sep 2022 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 04:45:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 02:45:14 2022
Response via : Initial Calibration

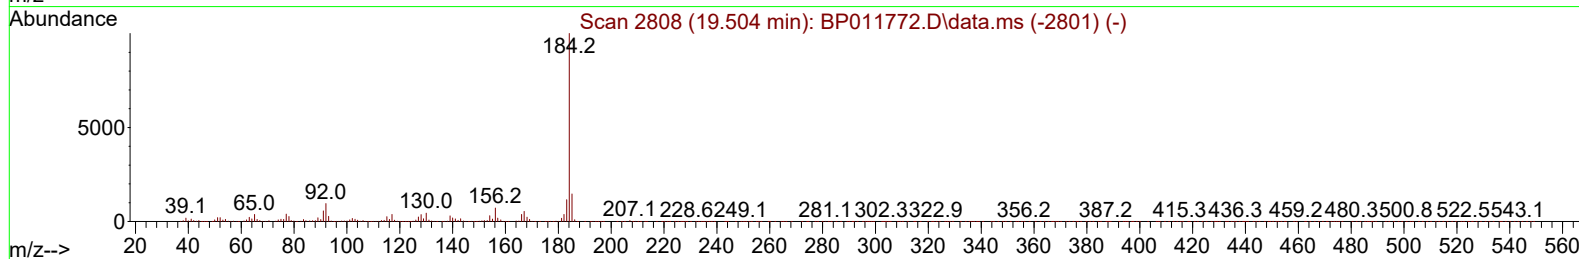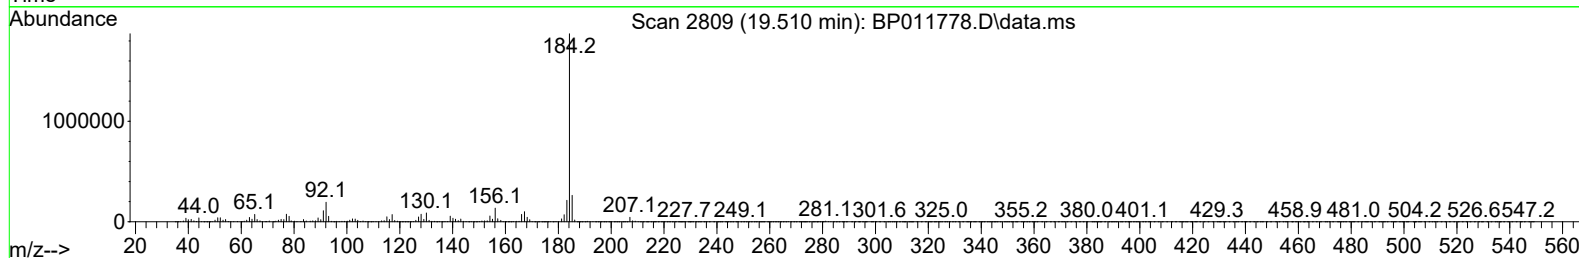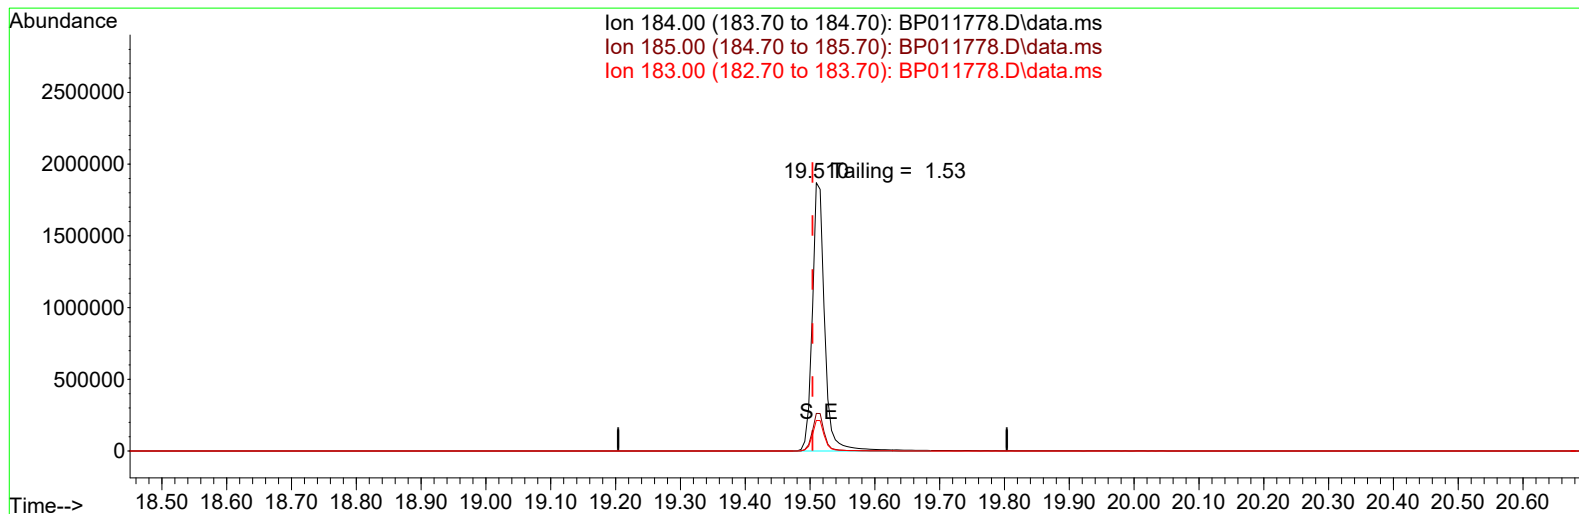

TIC: BP011778.D\data.ms

(77) Benzidine**19.510min (+ 0.006) 4904093.93 ng****response 2474650**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.01
183.00	11.60	11.43
0.00	0.00	0.00