

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
 Data File : BP011780.D
 Acq On : 23 Sep 2022 11:23
 Operator : CG/JU
 Sample : PB147850BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB147850BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP011780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	417	423	434	rBV	3787033	5758967	28.49%	8.046%
2	7.075	688	695	709	rBV	4145779	6576129	32.53%	9.187%
3	7.916	832	838	847	rVB	765718	1225520	6.06%	1.712%
4	9.081	1029	1036	1048	rBV	2351948	3917785	19.38%	5.473%
5	10.728	1309	1316	1329	rVB	1074853	1848801	9.15%	2.583%
6	13.187	1727	1734	1751	rBV	6158868	9084339	44.94%	12.692%
7	14.563	1960	1968	1976	rBV	1818853	2730920	13.51%	3.815%
8	16.051	2214	2221	2246	rBV	4449644	6359409	31.46%	8.885%
9	17.316	2429	2436	2449	rBV	2476178	3458680	17.11%	4.832%
10	19.875	2865	2871	2883	rBV	16027438	20216273	100.00%	28.244%
11	21.398	3125	3130	3143	rBV	3983929	5032788	24.89%	7.031%
12	23.851	3540	3547	3558	rVB2	2640849	5368176	26.55%	7.500%




Sum of corrected areas: 71577787

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
Data File : BP011780.D
Acq On : 23 Sep 2022 11:23
Operator : CG/JU
Sample : PB147850BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147850BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

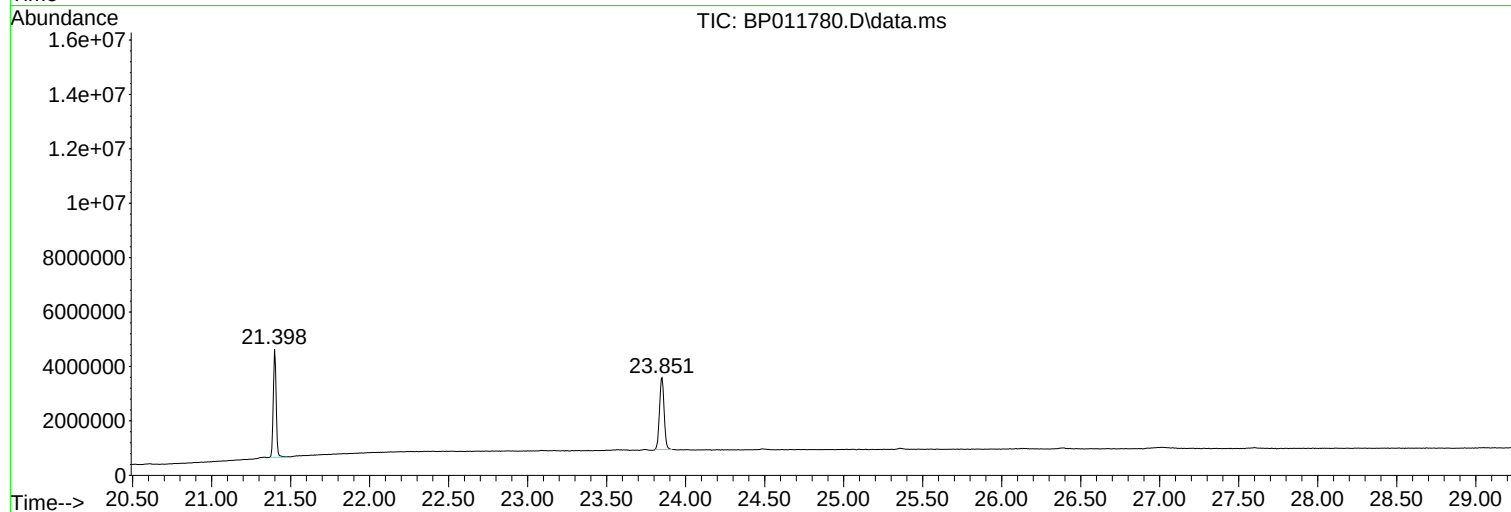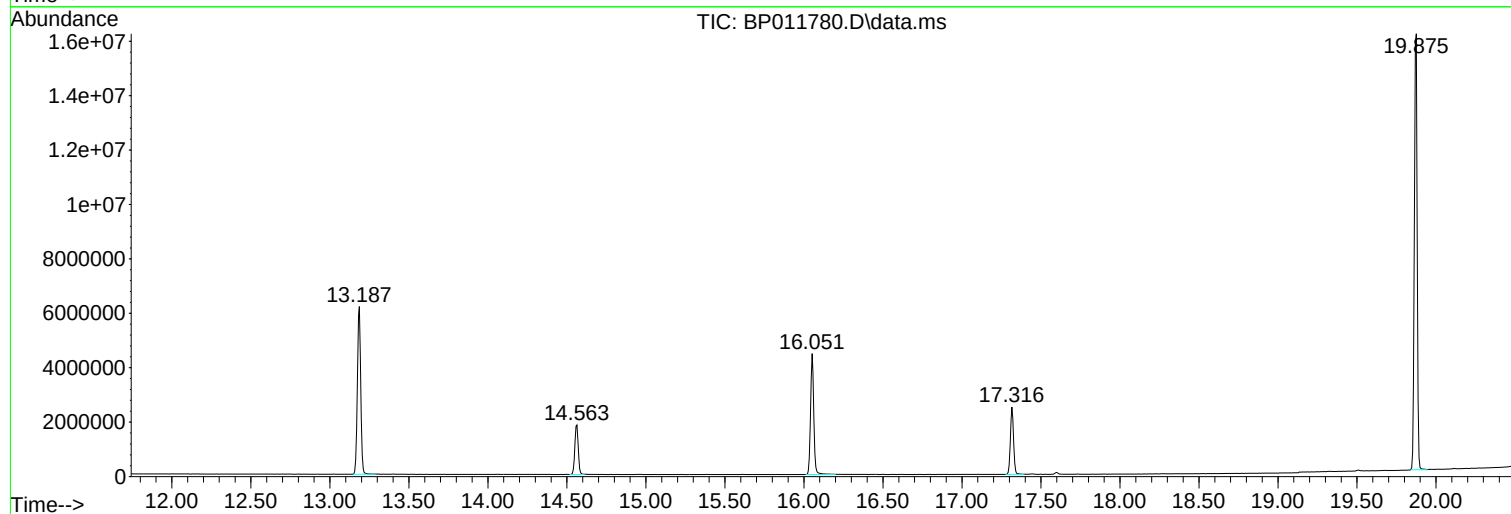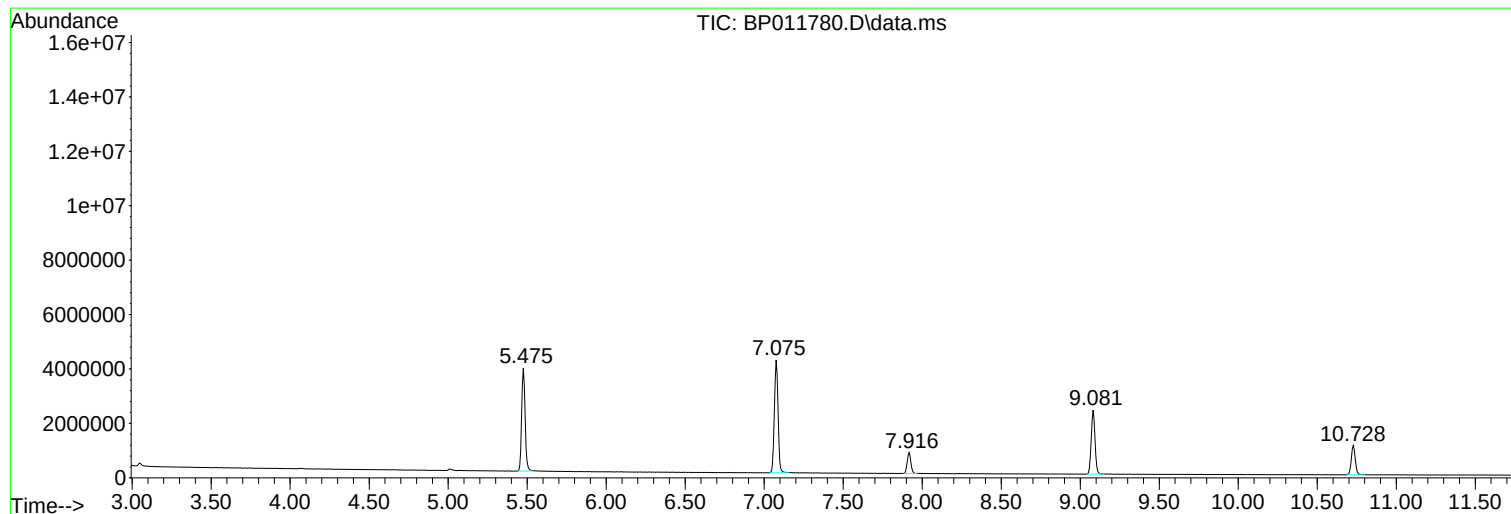

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
Data File : BP011780.D
Acq On : 23 Sep 2022 11:23
Operator : CG/JU
Sample : PB147850BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147850BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
Data File : BP011780.D
Acq On : 23 Sep 2022 11:23
Operator : CG/JU
Sample : PB147850BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147850BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------