


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
 Data File : BP011778.D
 Acq On : 23 Sep 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 22 02:45:14 2022

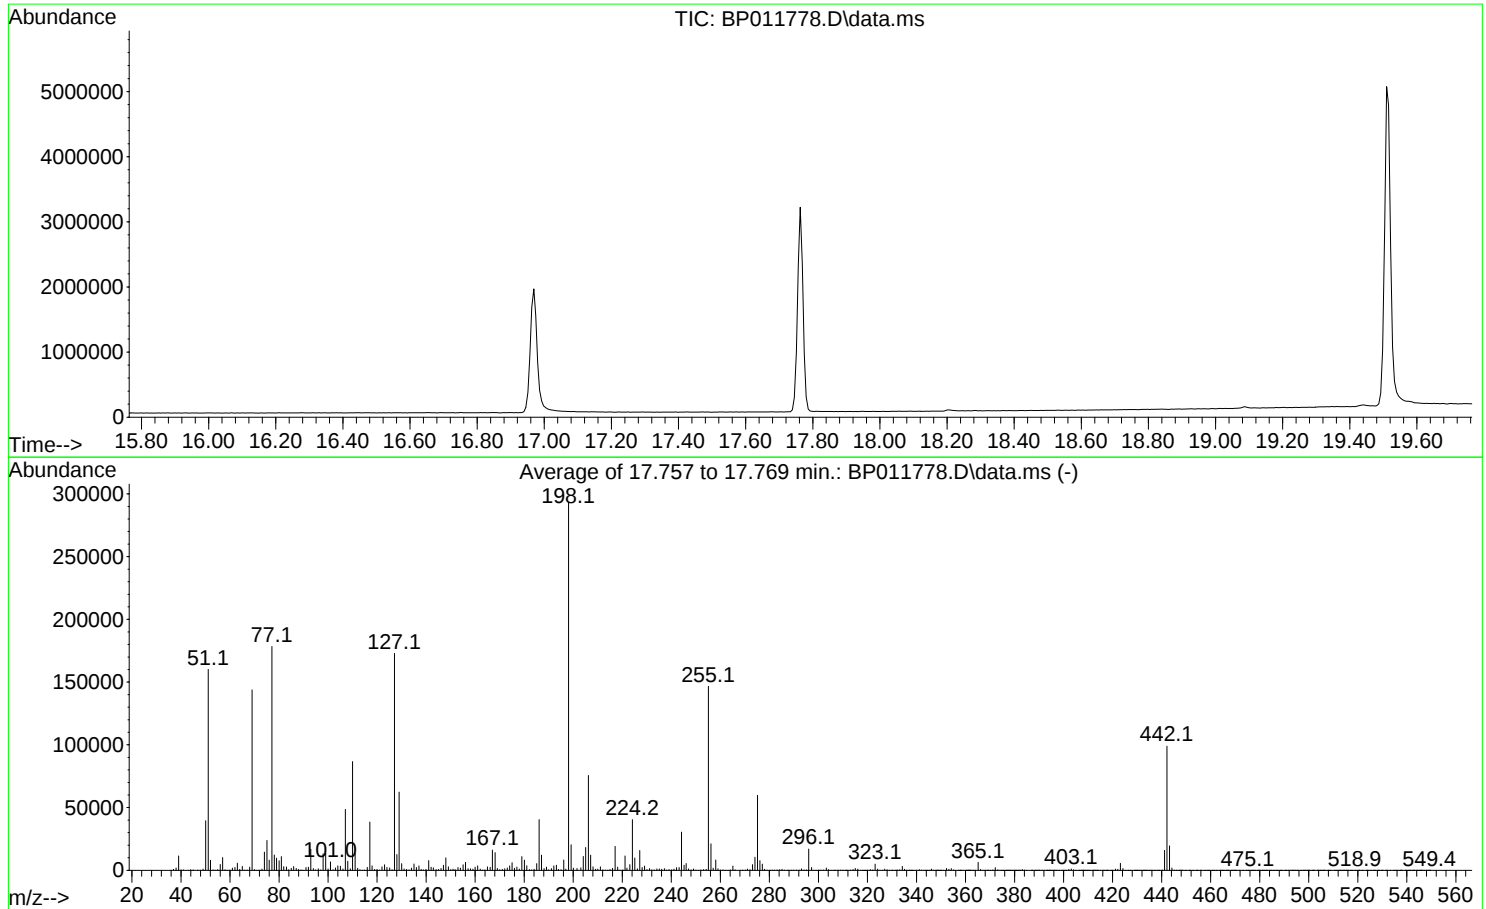




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.6	160188	PASS
68	69	0.00	2	1.7	2474	PASS
69	198	0.00	100	49.0	143745	PASS
70	69	0.00	2	0.4	637	PASS
127	198	10	80	59.0	172864	PASS
197	198	0.00	2	0.3	917	PASS
198	198	100	100	100.0	293225	PASS
199	198	5	9	6.9	20373	PASS
275	198	10	60	20.4	59731	PASS
365	198	1	100	2.1	6274	PASS
441	198	0.01	100	5.4	15947	PASS
442	442	100	100	100.0	98850	PASS
443	442	15	24	19.7	19452	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
 Data File : BP011778.D
 Acq On : 23 Sep 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 24 04:45:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 02:45:14 2022
 Response via : Initial Calibration

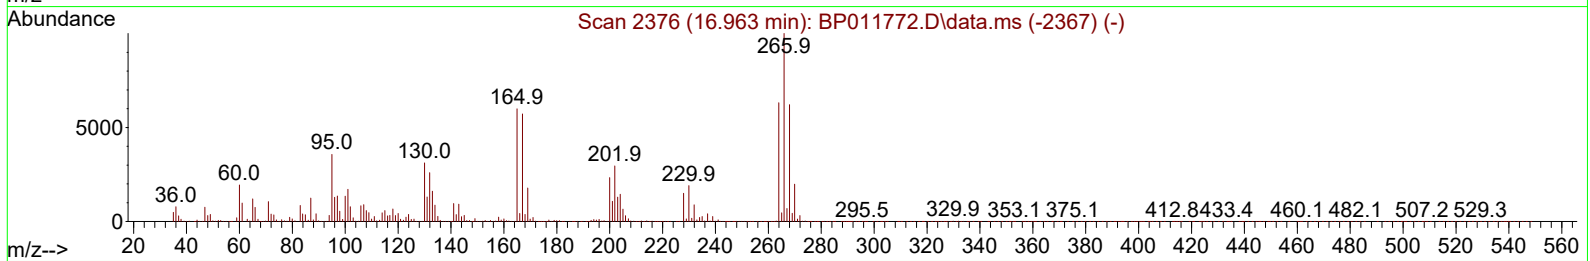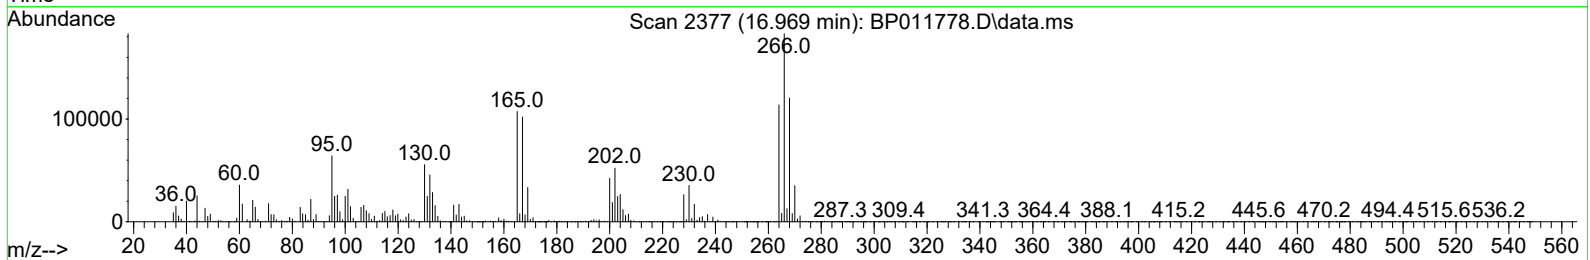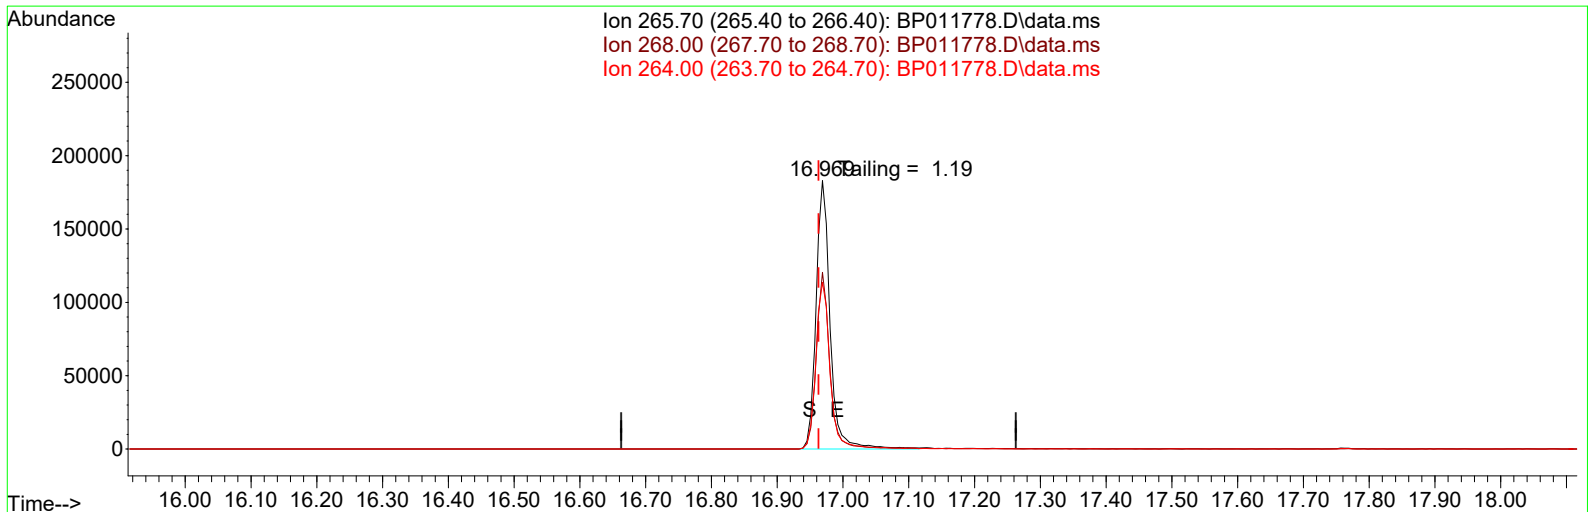

TIC: BP011778.D\data.ms

(70) Pentachlorophenol (C)

16.969min (+ 0.006) 2038145.44 ng




response 270351

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	65.81
264.00	63.20	62.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092322\
Data File : BP011778.D
Acq On : 23 Sep 2022 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 24 04:45:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 02:45:14 2022
Response via : Initial Calibration

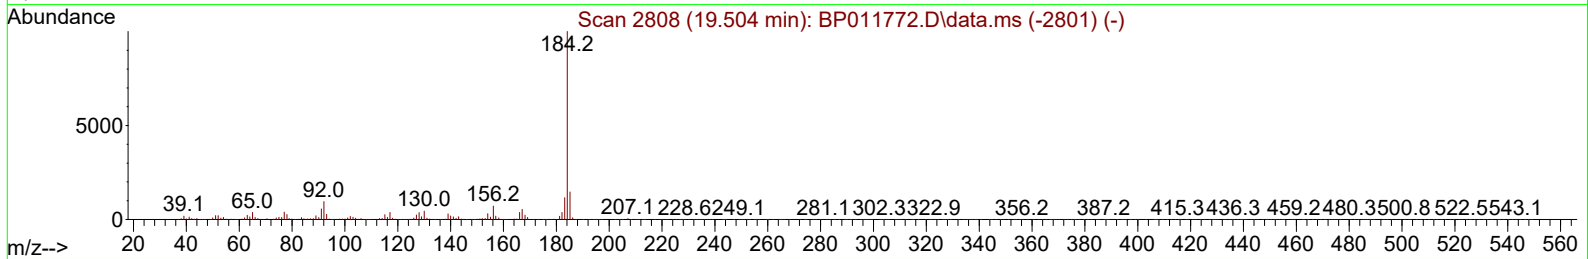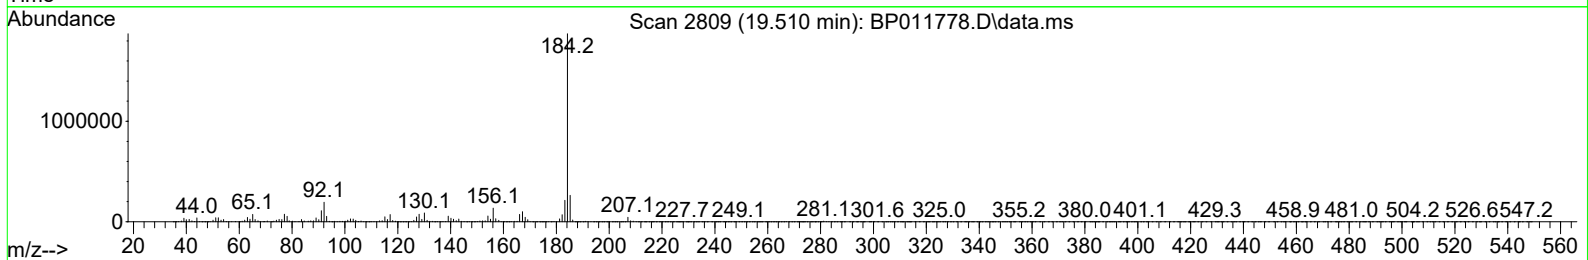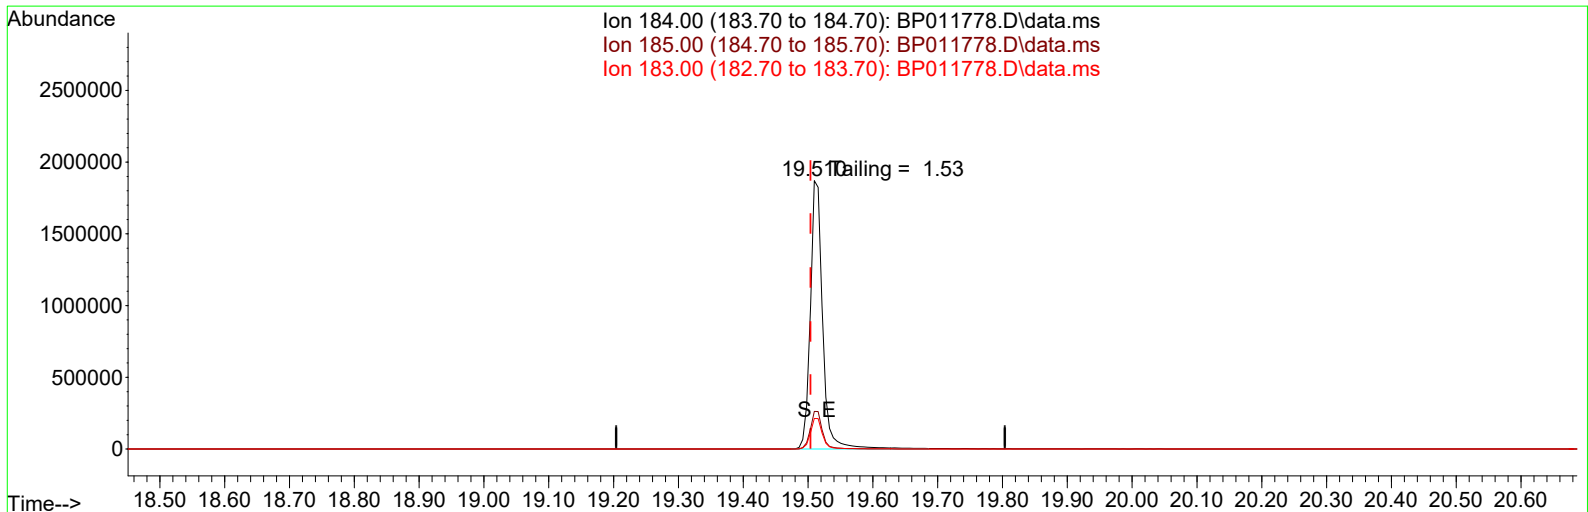

TIC: BP011778.D\data.ms

(77) Benzidine

19.510min (+ 0.006) 4904093.93 ng

response 2474650

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.01
183.00	11.60	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2022	BNA_P	<u>BP011778.D</u>
Compound Name	Response	Retention Time
DDT	977463	20.71
DDD	6729	20.28
DDE	420	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7149	984612	0.73

Instrument :
BNA_P
ClientSampleId :
DFTPP