
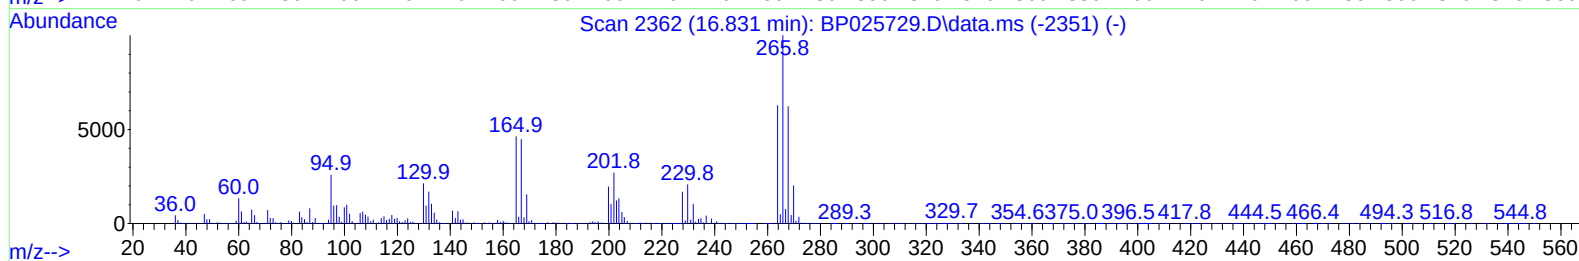
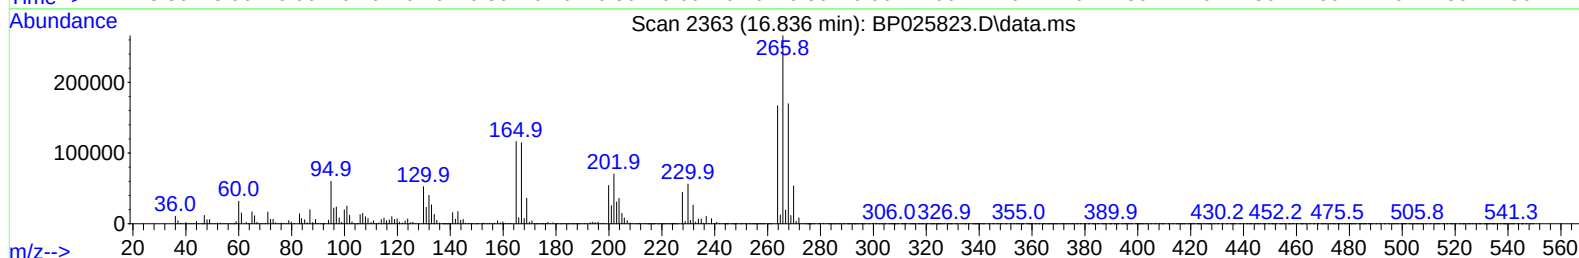


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
Data File : BP025823.D
Acq On : 23 Sep 2025 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 11:28:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

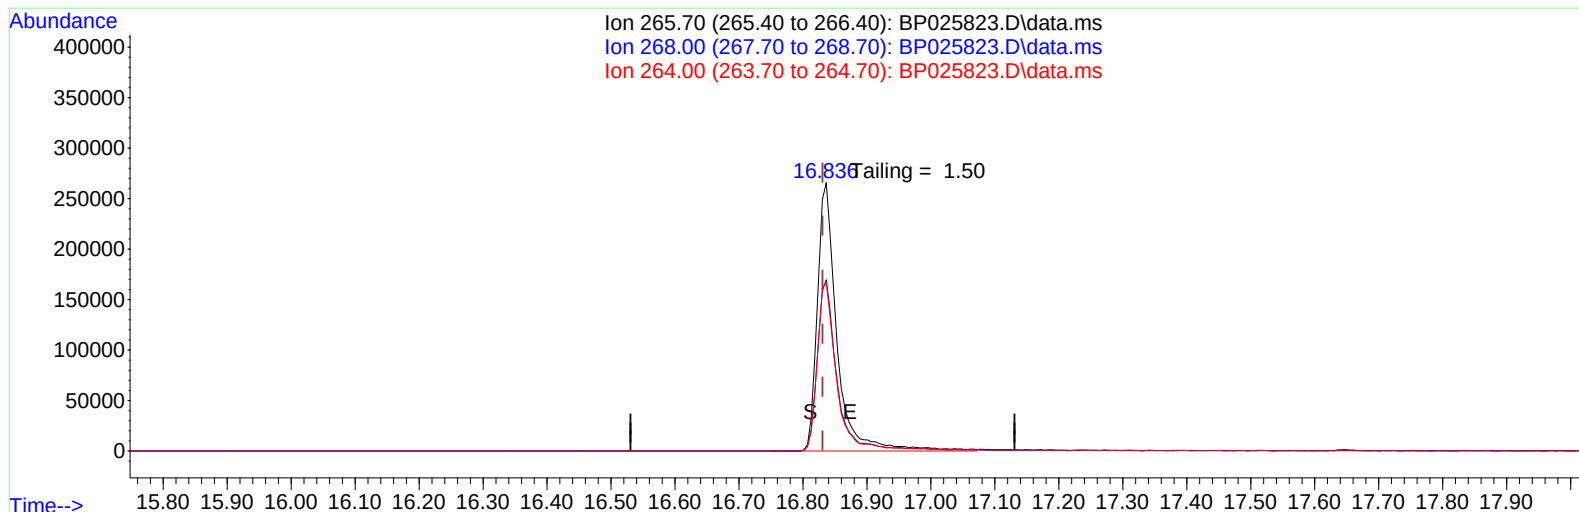

TIC: BP025823.D\data.ms

(70) Pentachlorophenol (C)




16.836min (+ 0.006) 4627969.76 ng

response 561305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.82
264.00	62.70	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
Data File : BP025823.D
Acq On : 23 Sep 2025 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 11:28:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

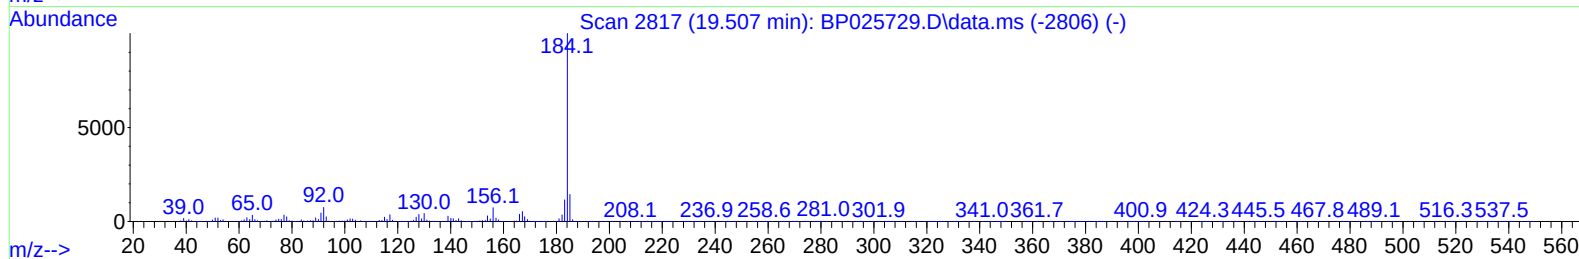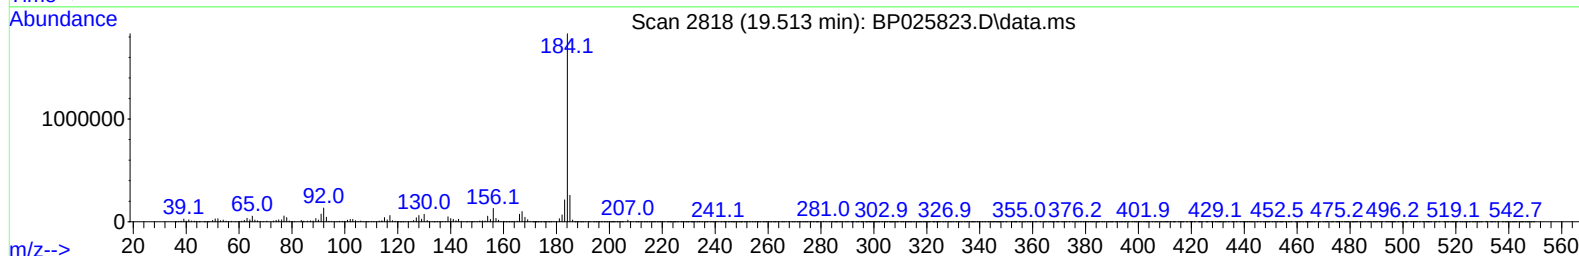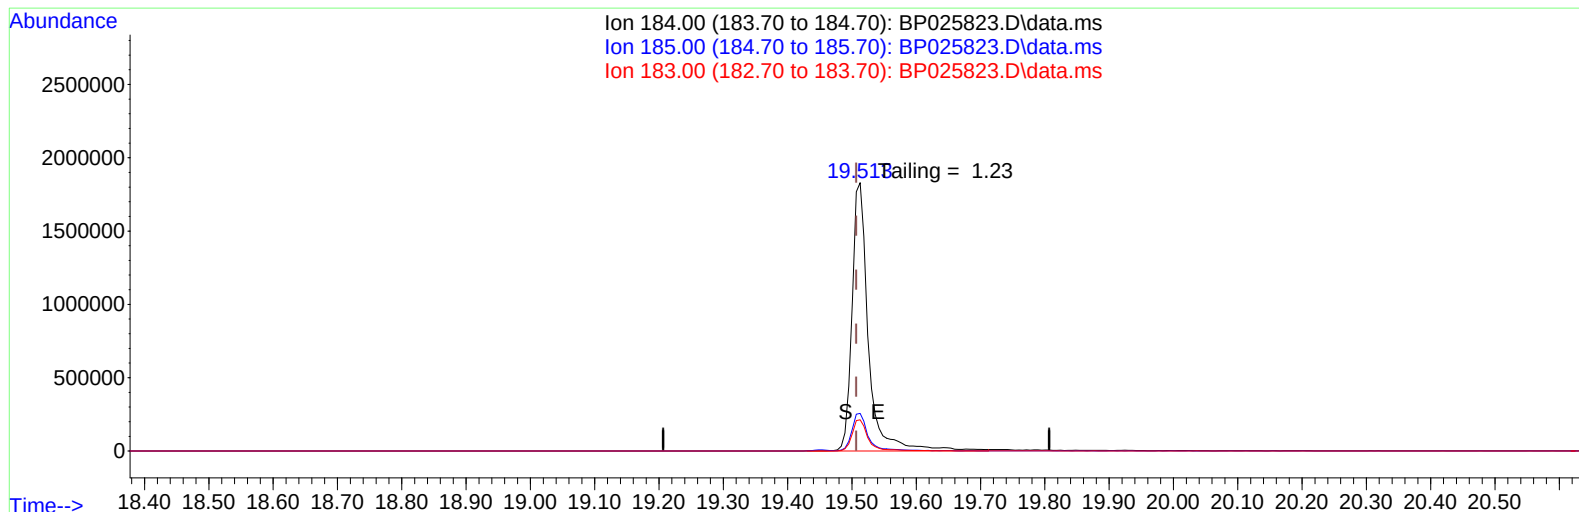

TIC: BP025823.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 1208647.75 ng

response 3203028

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.05
183.00	11.50	11.63
0.00	0.00	0.00