
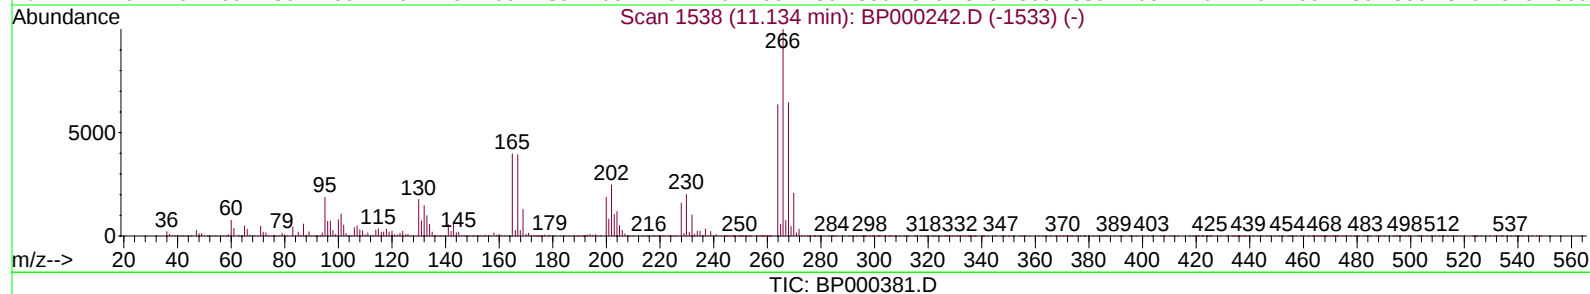
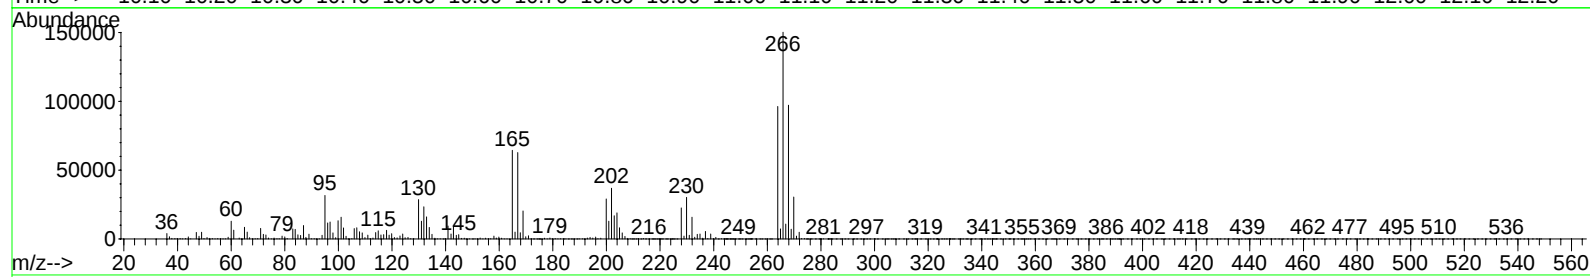


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP092419\
 Data File : BP000381.D
 Acq On : 24 Sep 2019 11:30
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 19:13:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 19 14:44:51 2019
 Response via : Initial Calibration

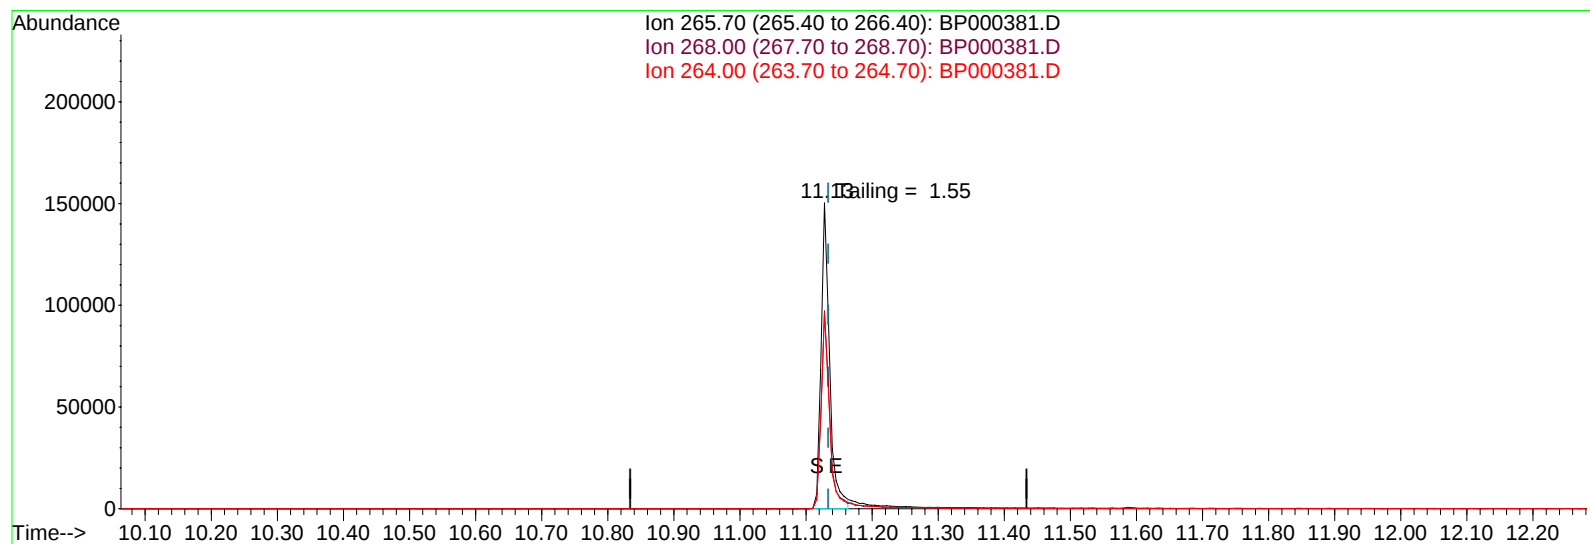

(70) Pentachlorophenol (C)




11.128min (-0.006) 291437.21ng

response 145208

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.70
264.00	63.50	64.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP092419\
 Data File : BP000381.D
 Acq On : 24 Sep 2019 11:30
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 19:13:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 19 14:44:51 2019
 Response via : Initial Calibration

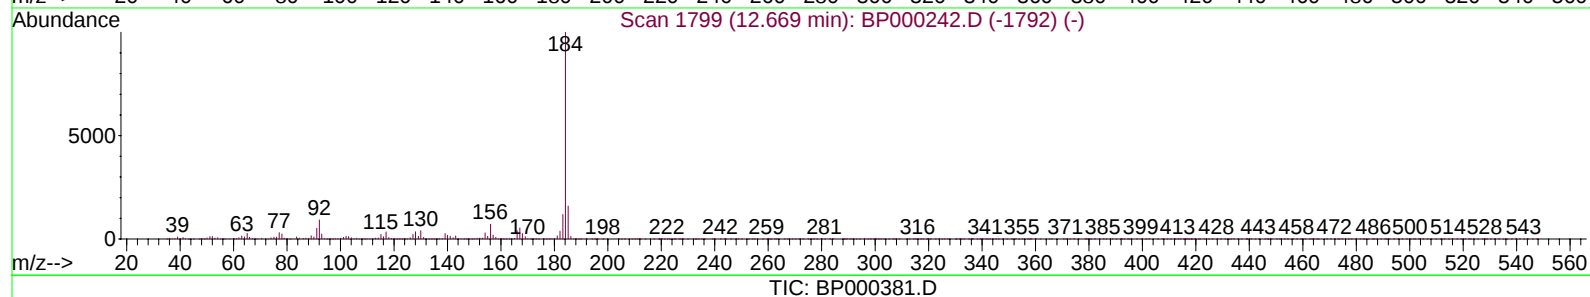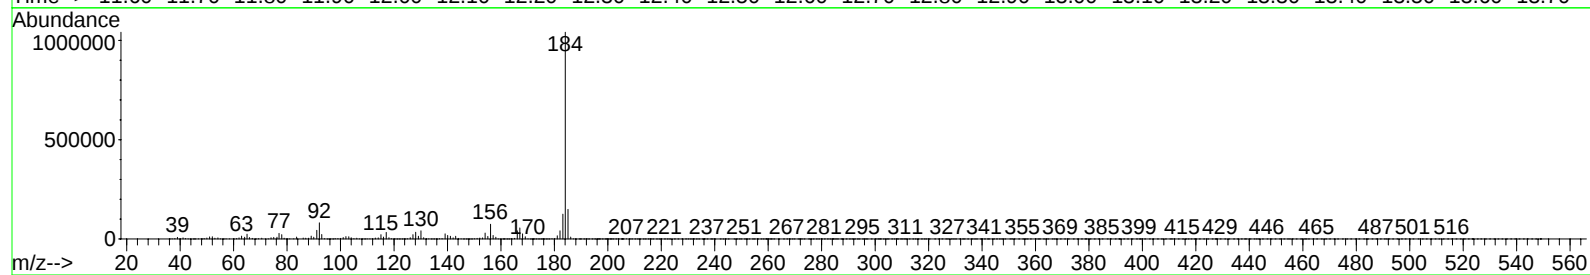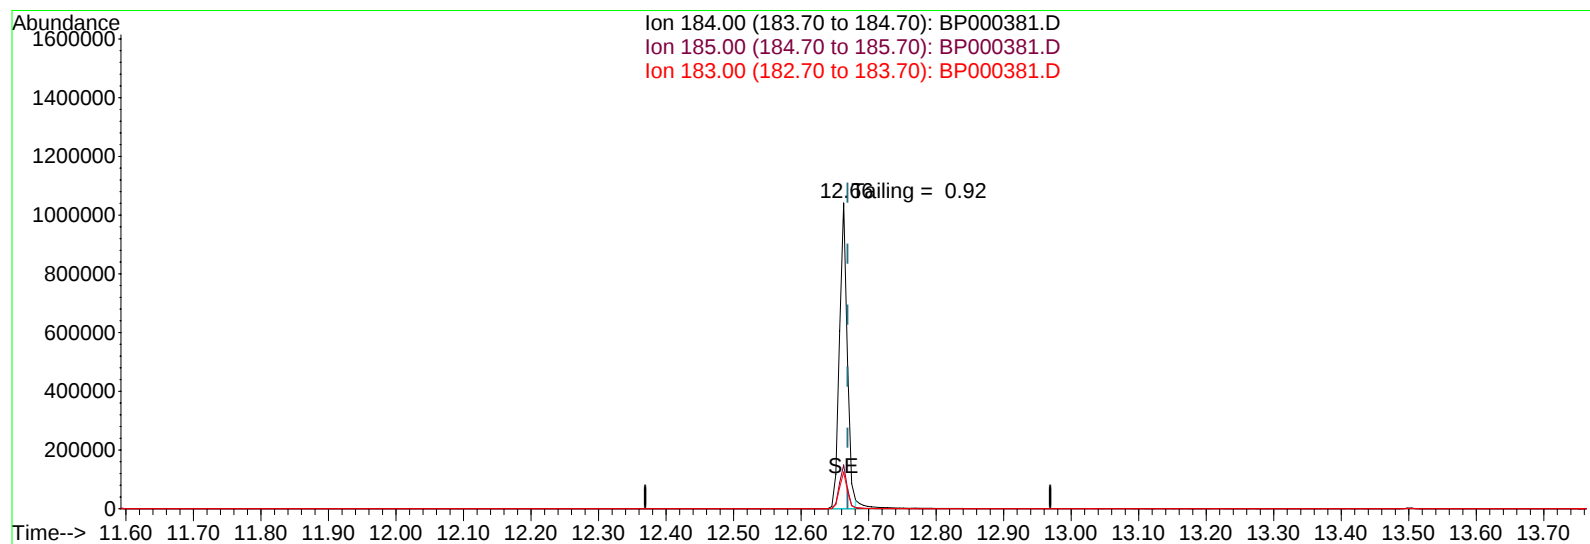

(77) Benzidine

12.663min (-0.006) 243996.92ng

response 862701

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	14.35
183.00	11.90	12.04
0.00	0.00	0.00